




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
Data File : BP020900.D
Acq On : 11 Jul 2024 12:19
Operator : MA/JU
Sample : P3138-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZF7

Manual IntegrationsAPPROVED

Quant Time: Jul 11 23:02:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 10 18:38:19 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024

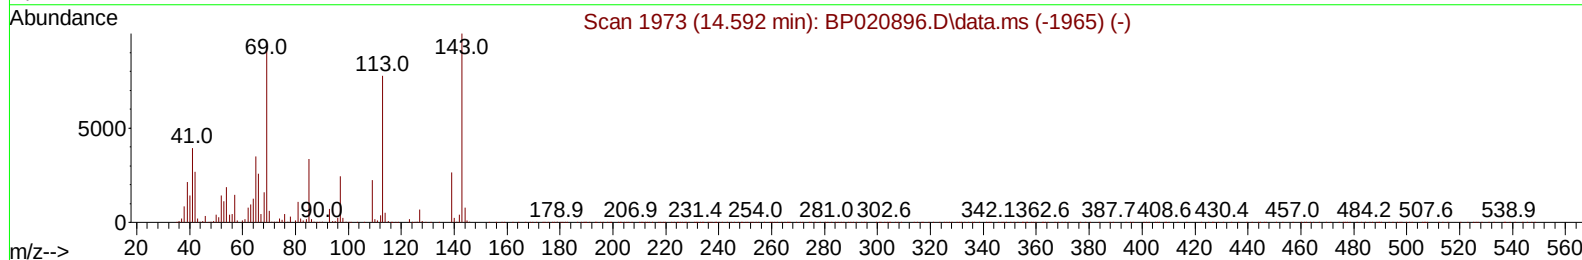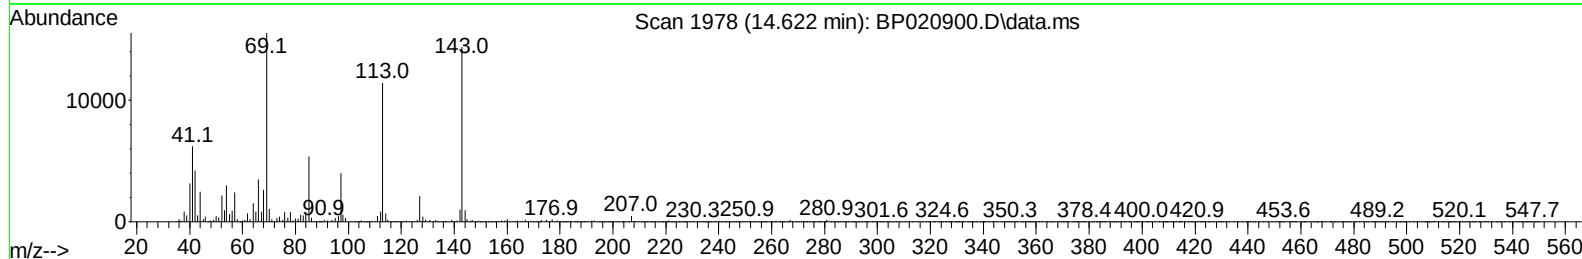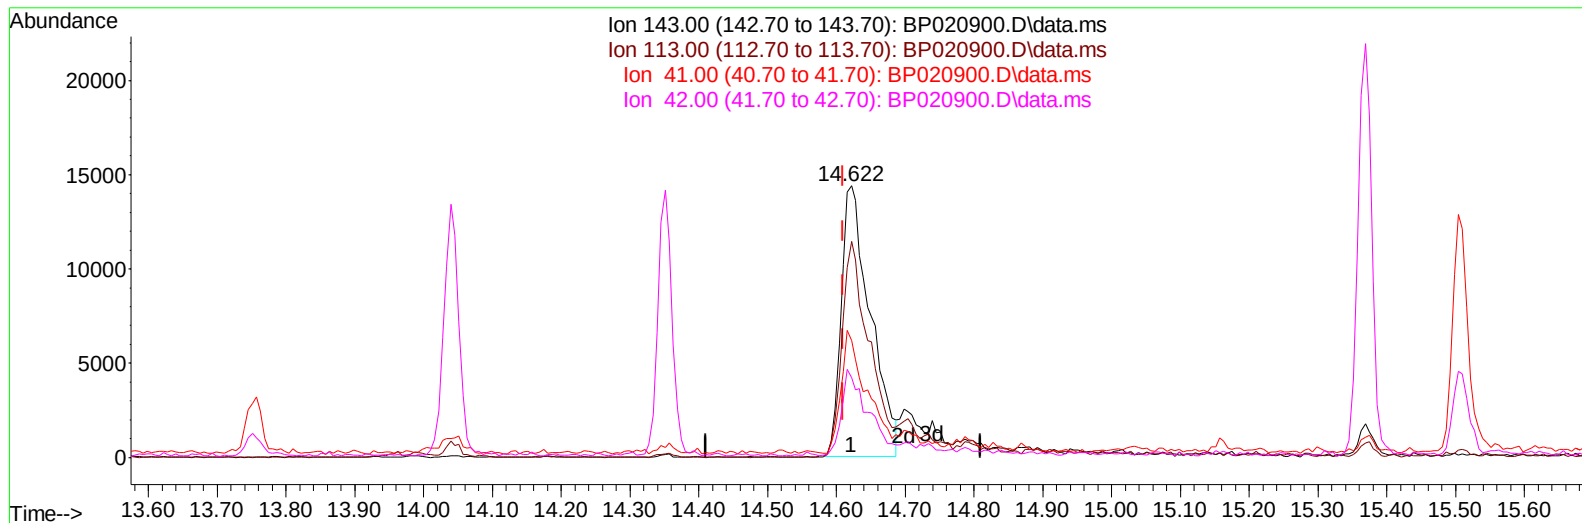

TIC: BP020900.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.622min (+ 0.012) 5.82 ng/ul

response 42260

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	79.50
41.00	37.90	43.03
42.00	27.10	29.34




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
Data File : BP020900.D
Acq On : 11 Jul 2024 12:19
Operator : MA/JU
Sample : P3138-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZF7

Manual IntegrationsAPPROVED

Quant Time: Jul 11 23:02:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 10 18:38:19 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024

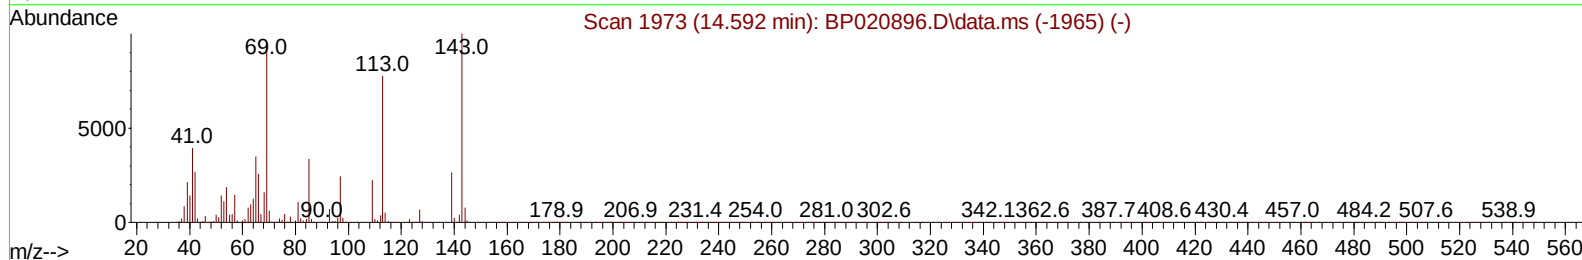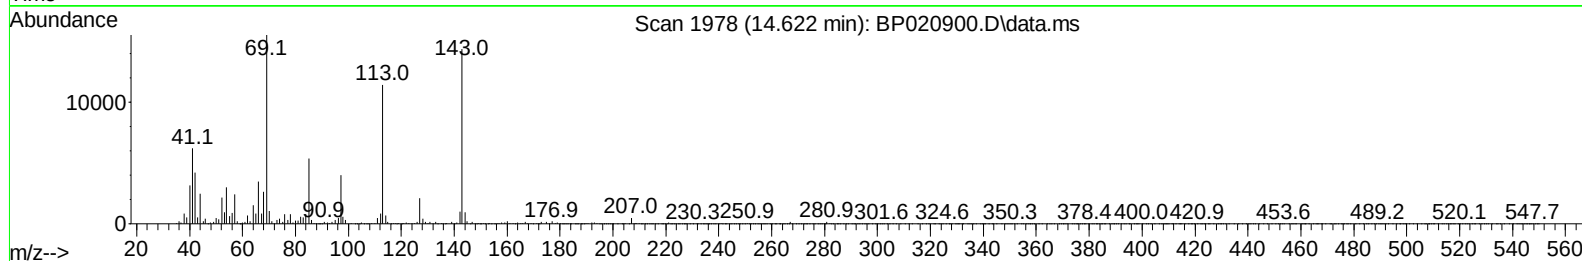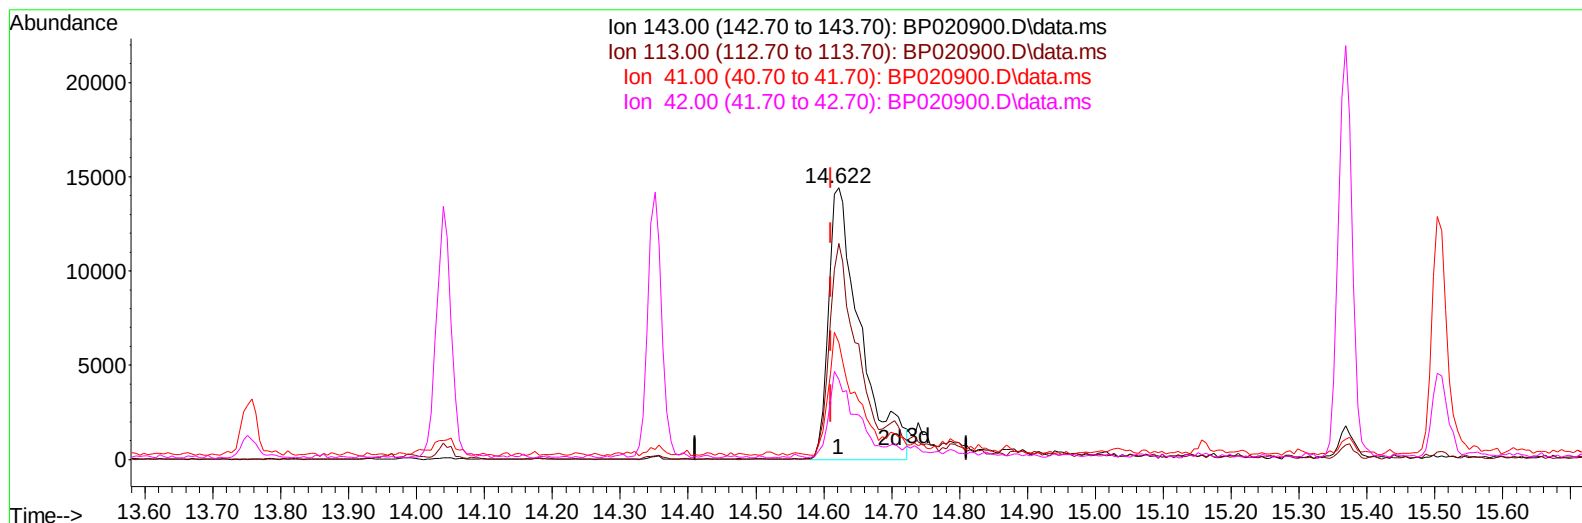

TIC: BP020900.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.622min (+ 0.012) 6.47 ng/ul m

response 46963

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	74.70	79.50
41.00	37.90	43.03
42.00	27.10	29.34

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
 Data File : BP020900.D
 Acq On : 11 Jul 2024 12:19
 Operator : MA/JU
 Sample : P3138-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YDZF7

Manual IntegrationsAPPROVED

Quant Time: Jul 11 23:15:42 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 10 18:38:19 2024
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
 Supervised By :mohammad ahmed 07/13/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.716	152	233303	20.000	ng/ul	0.00
20) Naphthalene-d8	10.487	136	1024095	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.351	164	702315	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.163	188	1386122	20.000	ng/ul	-0.02
79) Chrysene-d12	21.615	240	990267	20.000	ng/ul	0.00
88) Perylene-d12	24.968	264	1110234	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	20898	4.076	ng/uL	0.00
4) Pyridine-d5	3.669	84	124921	8.416	ng/ul	0.00
7) Phenol-d5	6.910	99	145522	7.651	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.063	67	356178	30.900	ng/ul	0.00
11) 2-Chlorophenol-d4	7.263	132	415233	26.496	ng/ul	0.00
15) 4-Methylphenol-d8	8.428	113	270892	17.148	ng/ul	0.00
21) Nitrobenzene-d5	8.875	128	235666	29.628	ng/ul	0.00
24) 2-Nitrophenol-d4	9.587	143	269837	29.639	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.122	165	452197	27.469	ng/ul	0.00
31) 4-Chloroaniline-d4	10.640	131	478033	21.919	ng/ul	0.00
46) Dimethylphthalate-d6	13.757	166	1595067	31.242	ng/ul	-0.01
49) Acenaphthylene-d8	14.039	160	1713834	29.896	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.622	143	46963m	6.465	ng/ul	0.01
60) Fluorene-d10	15.369	176	1309637	31.268	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.510	200	249208	29.714	ng/ul	0.00
73) Anthracene-d10	17.269	188	2068050	33.592	ng/ul	0.00
81) Pyrene-d10	19.651	212	2114241	34.534	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.745	264	1885044	34.426	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
Data File : BP020900.D
Acq On : 11 Jul 2024 12:19
Operator : MA/JU
Sample : P3138-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZF7

Manual IntegrationsAPPROVED

Quant Time: Jul 11 23:15:42 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 10 18:38:19 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/12/2024
Supervised By :mohammad ahmed 07/13/2024

