

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
 Data File : BP020930.D
 Acq On : 12 Jul 2024 11:24
 Operator : MA/JU
 Sample : P3087-17
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A4BR2

Quant Time: Jul 12 23:13:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Jul 10 18:38:19 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.710	152	213395	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.487	136	898634	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.351	164	579667	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.157	188	1149270	20.000	ng/u1	-0.02
79) Chrysene-d12	21.621	240	1087108	20.000	ng/u1	0.00
88) Perylene-d12	24.962	264	1275989	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	18146	3.870	ng/uL	0.00
4) Pyridine-d5	3.669	84	249870	18.405	ng/u1	0.00
7) Phenol-d5	6.916	99	384334	22.091	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.063	67	241070	22.865	ng/u1	0.00
11) 2-Chlorophenol-d4	7.263	132	328182	22.895	ng/u1	0.00
15) 4-Methylphenol-d8	8.434	113	322024	22.286	ng/u1	0.00
21) Nitrobenzene-d5	8.875	128	156928	22.483	ng/u1	0.00
24) 2-Nitrophenol-d4	9.581	143	185244	23.188	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.128	165	318346	22.038	ng/u1	0.00
31) 4-Chloroaniline-d4	10.628	131	431857	22.566	ng/u1	-0.01
46) Dimethylphthalate-d6	13.757	166	1028687	24.412	ng/u1	-0.01
49) Acenaphthylene-d8	14.039	160	1129189	23.865	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.610	143	122101	20.366	ng/u1	0.00
60) Fluorene-d10	15.357	176	848794	24.553	ng/u1	-0.02
65) 4,6-Dinitro-2-methylph...	15.510	200	125175	18.001	ng/u1	0.00
73) Anthracene-d10	17.257	188	1261223	24.708	ng/u1	-0.02
81) Pyrene-d10	19.645	212	1495377	22.249	ng/u1	-0.02
92) Benzo(a)pyrene-d12	24.721	264	1603417	25.479	ng/u1	-0.04
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.516	149	52997	1.070	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
Data File : BP020930.D
Acq On : 12 Jul 2024 11:24
Operator : MA/JU
Sample : P3087-17
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A4BR2

Quant Time: Jul 12 23:13:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Jul 10 18:38:19 2024
Response via : Initial Calibration

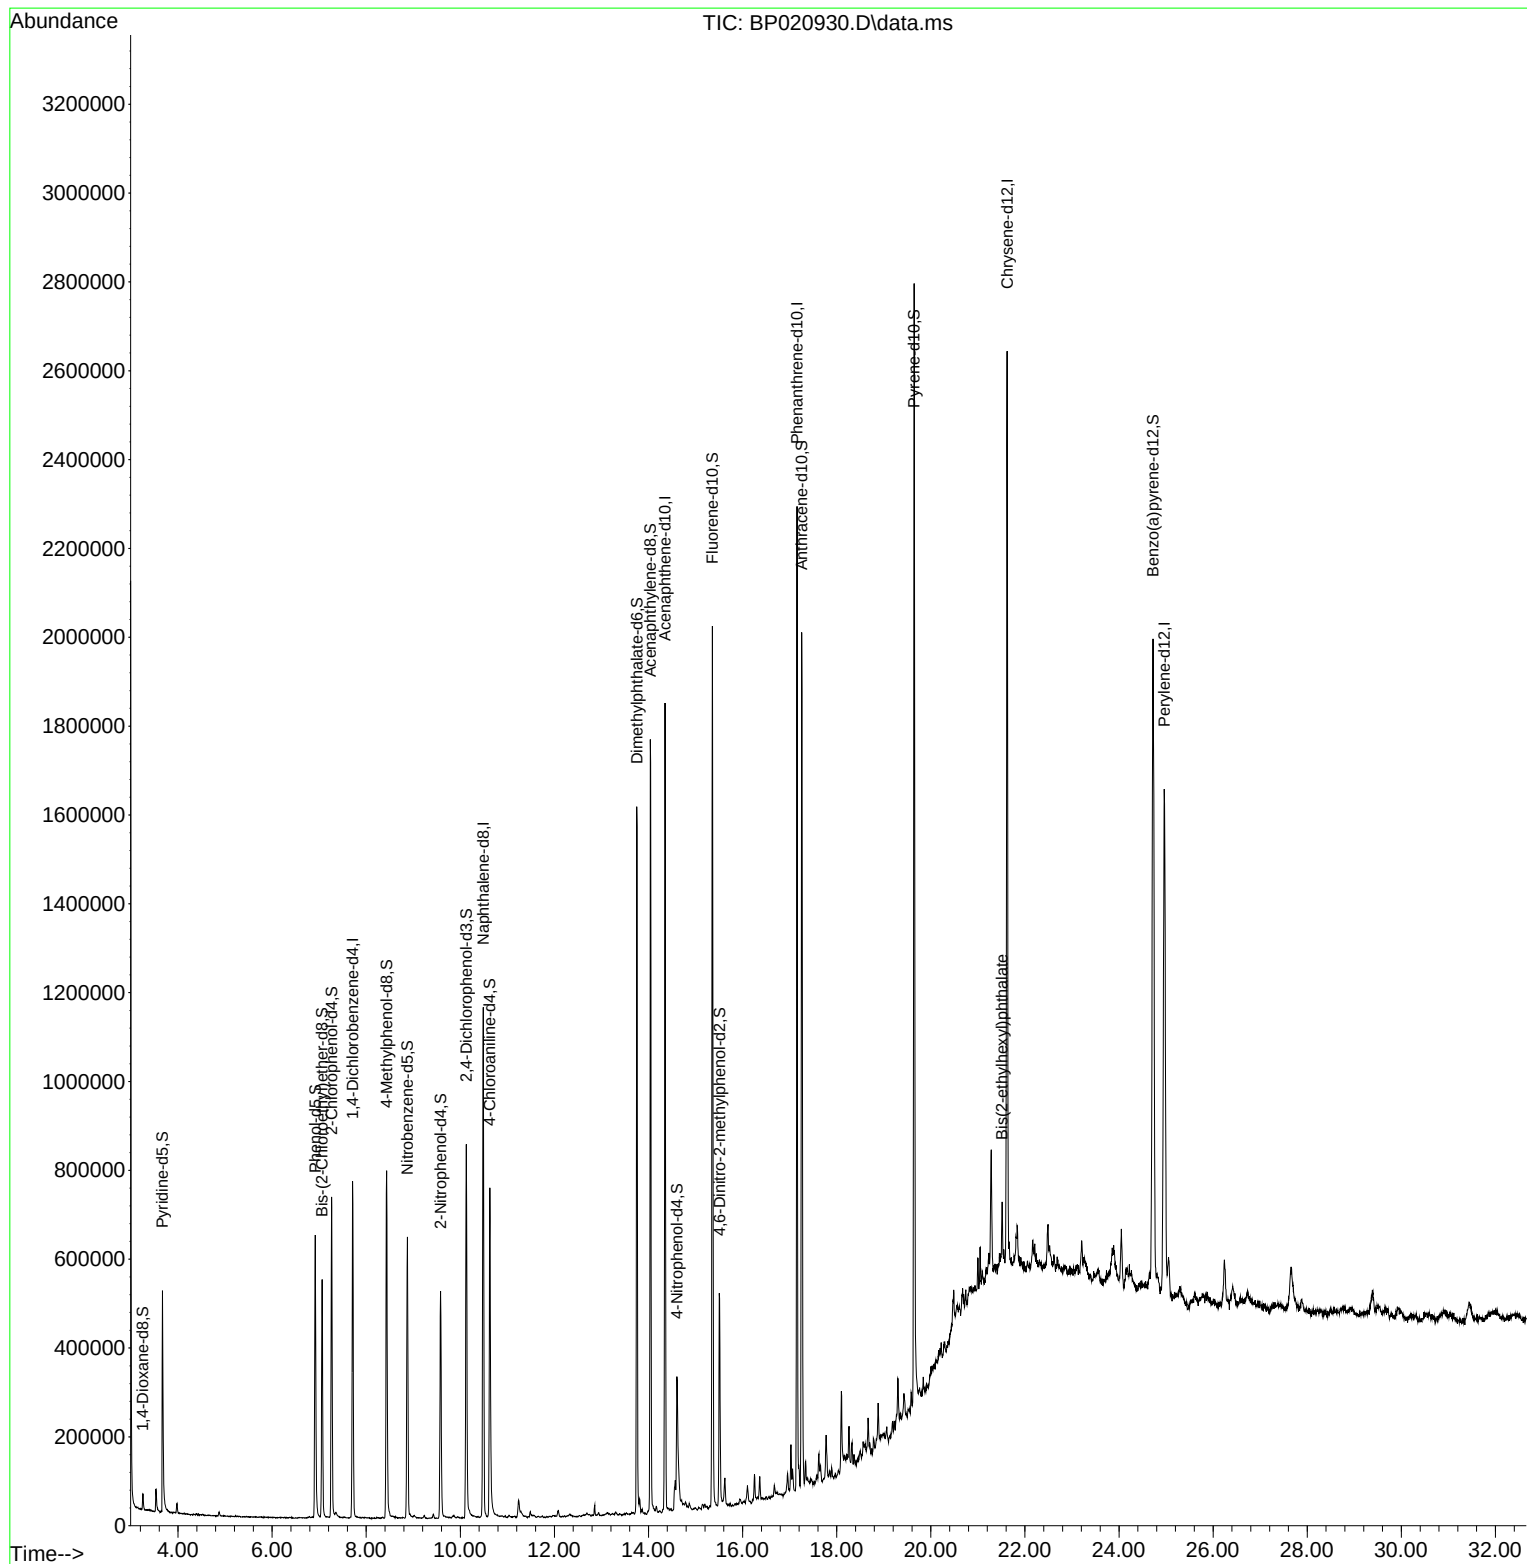

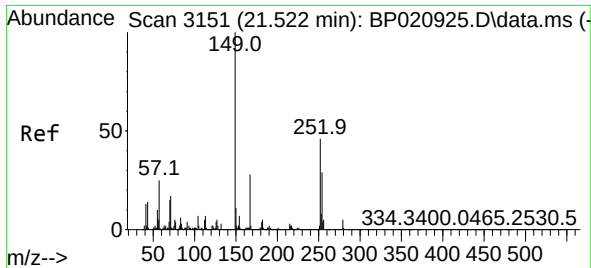

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.070 ng/ul
 RT: 21.516 min Scan# 31
 Delta R.T. -0.024 min
 Lab File: BP020930.D
 Acq: 12 Jul 2024 11:24

Instrument :
 BNA_P
 ClientSampleId :
 A4BR2

Tgt Ion:	149	Resp:	52997
Ion Ratio	Lower	Upper	
149	100		
167	27.8	22.1	33.1
279	5.2	3.7	5.5

