

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
 Data File : BP020950.D
 Acq On : 13 Jul 2024 02:45
 Operator : MA/JU
 Sample : P3137-04
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YDZE8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/13/2024
 Supervised By :mohammad ahmed 07/13/2024

Quant Time: Jul 13 03:48:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jul 12 23:34:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.710	152	186158	20.000	ng/u1	0.00
20) Naphthalene-d8	10.481	136	727719	20.000	ng/u1	0.01
38) Acenaphthene-d10	14.340	164	487976	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.163	188	1071980	20.000	ng/u1	0.00
79) Chrysene-d12	21.610	240	1067926	20.000	ng/u1	0.00
88) Perylene-d12	24.939	264	1266321	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.252	96	15492	3.787	ng/uL	0.00
4) Pyridine-d5	3.670	84	138511	11.695	ng/u1	0.00
7) Phenol-d5	6.916	99	142124	9.364	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.058	67	104982	11.414	ng/u1	0.00
11) 2-Chlorophenol-d4	7.263	132	171658	13.728	ng/u1	0.01
15) 4-Methylphenol-d8	8.434	113	196666	15.602	ng/u1	0.01
21) Nitrobenzene-d5	8.863	128	64677	11.443	ng/u1	0.00
24) 2-Nitrophenol-d4	9.575	143	73816	11.410	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.128	165	155166	13.264	ng/u1	0.02
31) 4-Chloroaniline-d4	10.634	131	188841	12.185	ng/u1	0.00
46) Dimethylphthalate-d6	13.757	166	476830	13.442	ng/u1	0.00
49) Acenaphthylene-d8	14.034	160	504362	12.662	ng/u1	0.00
54) 4-Nitrophenol-d4	14.640	143	10813m	2.142	ng/u1	0.04
60) Fluorene-d10	15.351	176	397875	13.672	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.498	200	23900	3.685	ng/u1	0.00
73) Anthracene-d10	17.257	188	657048	13.800	ng/u1	0.00
81) Pyrene-d10	19.651	212	788229	11.939	ng/u1	0.01
92) Benzo(a)pyrene-d12	24.721	264	843582	13.507	ng/u1	0.01
Target Compounds						
2) 1,4-Dioxane	3.287	88	23638	5.254	ng/uL	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
Data File : BP020950.D
Acq On : 13 Jul 2024 02:45
Operator : MA/JU
Sample : P3137-04
Misc :
ALS Vial : 58 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
YDZE8

Quant Time: Jul 13 03:48:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jul 12 23:34:01 2024
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Yogesh Patel 07/13/2024
Supervised By :mohammad ahmed 07/13/2024

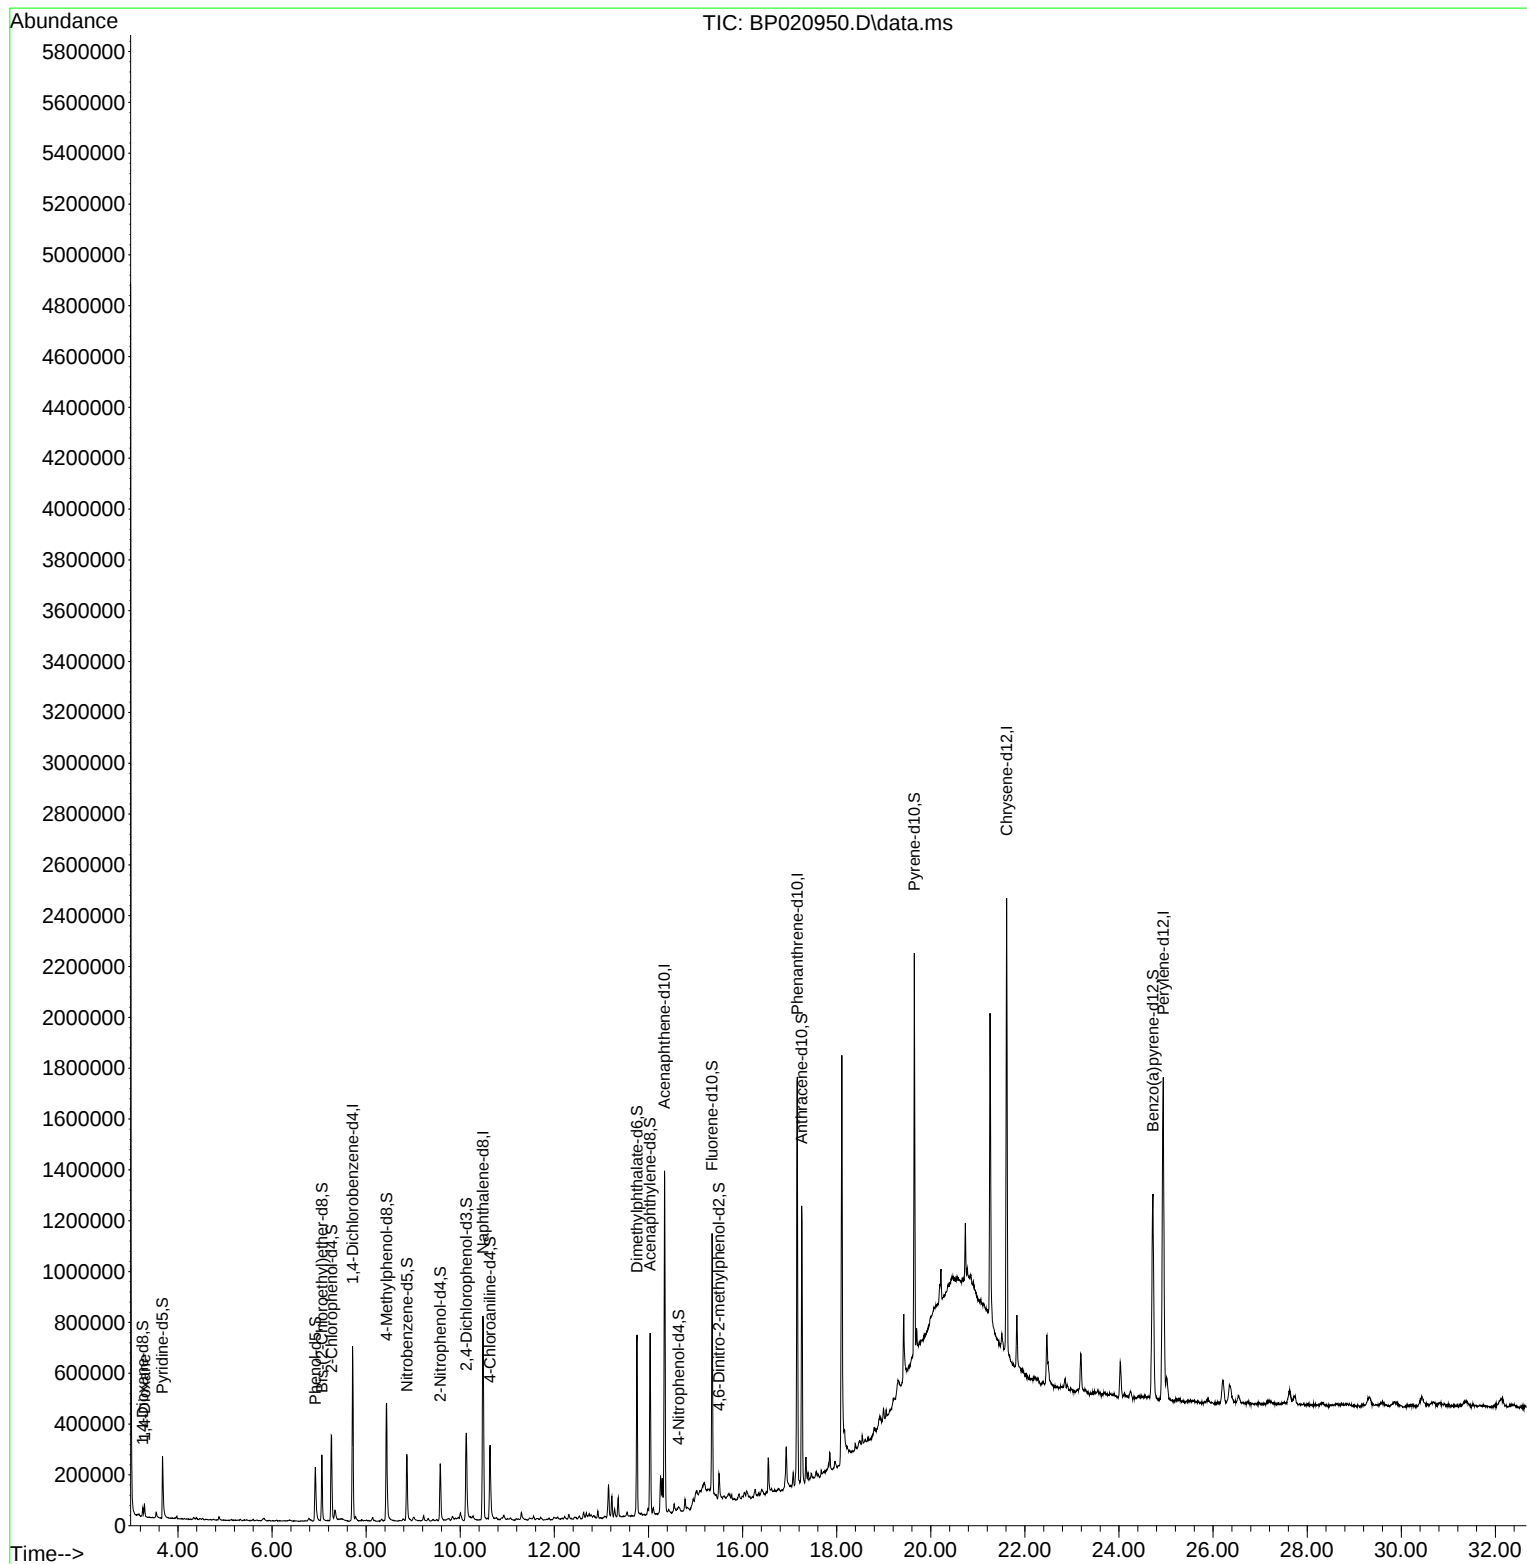

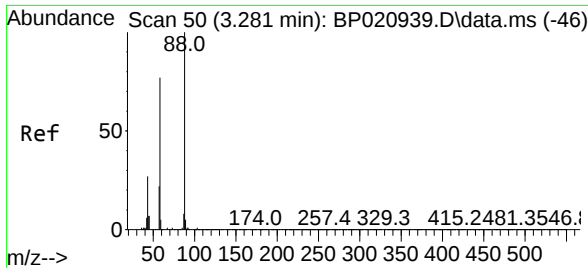

#2
 1,4-Dioxane
 Concen: 5.254 ng/uL
 RT: 3.287 min Scan# 51
 Delta R.T. 0.006 min
 Lab File: BP020950.D
 Acq: 13 Jul 2024 02:45

Instrument :
 BNA_P
 ClientSampleId :
 YDZE8

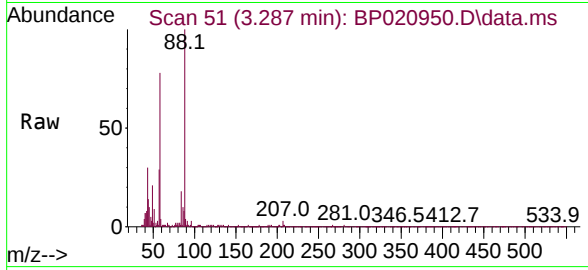

Tgt Ion: 88 Resp: 23638
 Ion Ratio Lower Upper
 88 100
 43 30.3 25.4 38.0
 58 78.4 59.2 88.8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/13/2024
 Supervised By :mohammad ahmed 07/13/2024

