

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
 Data File : BP020900.D
 Acq On : 11 Jul 2024 12:19
 Operator : MA/JU
 Sample : P3138-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 YDZF7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020900.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	41	45	50	rBV	43864	56446	1.06%	0.099%
2	3.669	113	116	130	rBV	240934	369188	6.91%	0.647%
3	3.975	165	168	173	rVB	10578	14136	0.26%	0.025%
4	4.393	236	239	243	rBV	6112	7214	0.14%	0.013%
5	4.875	316	321	329	rVB	9455	16375	0.31%	0.029%
6	6.834	650	654	660	rVB3	6179	8793	0.16%	0.015%
7	6.910	661	667	684	rVV	225810	413204	7.74%	0.724%
8	7.063	686	693	711	rVV	787929	1281072	23.98%	2.244%
9	7.263	720	727	744	rBV	906702	1497620	28.04%	2.624%
10	7.716	796	804	817	rBV	844136	1384201	25.91%	2.425%
11	8.428	918	925	941	rBV	617296	1196636	22.40%	2.096%
12	8.875	991	1001	1011	rBV	940947	1660421	31.08%	2.909%
13	9.004	1019	1023	1029	rVB8	5056	8918	0.17%	0.016%
14	9.240	1058	1063	1069	rVB6	5107	7870	0.15%	0.014%
15	9.587	1112	1122	1134	rBV	804166	1436995	26.90%	2.517%
16	10.122	1206	1213	1239	rBV	1100975	2117601	39.64%	3.710%
17	10.487	1268	1275	1287	rVB	1341665	2117975	39.65%	3.710%
18	10.640	1293	1301	1315	rBV	803280	1573855	29.46%	2.757%
19	11.316	1409	1416	1424	rBV	7562	21066	0.39%	0.037%
20	11.916	1514	1518	1526	rVB	4309	8601	0.16%	0.015%
21	12.098	1541	1549	1557	rBV2	13621	34699	0.65%	0.061%
22	12.692	1645	1650	1658	rVB2	4791	10452	0.20%	0.018%
23	12.939	1685	1692	1697	rBV7	5611	10405	0.19%	0.018%
24	13.304	1750	1754	1762	rVB6	5023	9913	0.19%	0.017%
25	13.757	1822	1831	1848	rBV	2257720	3400414	63.66%	5.957%
26	14.039	1870	1879	1891	rBV	2541407	3893678	72.89%	6.821%
27	14.351	1925	1932	1945	rBV	2093089	2996780	56.10%	5.250%
28	14.622	1970	1978	1988	rBV	101368	289242	5.41%	0.507%
29	15.157	2065	2069	2072	rBV	8527	11281	0.21%	0.020%
30	15.192	2072	2075	2082	rVB3	7162	12567	0.24%	0.022%
31	15.369	2098	2105	2122	rBV	3433500	4857203	90.93%	8.509%
32	15.510	2122	2129	2143	rVV	1012422	1647272	30.84%	2.886%
33	15.616	2143	2147	2156	rVB3	15869	33315	0.62%	0.058%
34	15.745	2166	2169	2173	rVB5	5555	7433	0.14%	0.013%
35	15.951	2199	2204	2209	rVB9	4715	7209	0.13%	0.013%
36	16.351	2269	2272	2276	rVB5	5763	7586	0.14%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
Data File : BP020900.D
Acq On : 11 Jul 2024 12:19
Operator : MA/JU
Sample : P3138-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZF7

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION

37	17.086	2393	2397	2400	rBV5	8016	10948	0.20%	0.019%
38	17.163	2404	2410	2421	rBV	2242461	3346969	62.66%	5.863%
39	17.269	2421	2428	2440	rBV	3472599	5228290	97.88%	9.159%
40	17.863	2525	2529	2536	rBV9	17411	29799	0.56%	0.052%
41	18.092	2563	2568	2574	rBV2	84491	135903	2.54%	0.238%
42	19.198	2751	2756	2763	rBV3	48358	83501	1.56%	0.146%
43	19.274	2765	2769	2772	rVB	30007	41872	0.78%	0.073%
44	19.433	2792	2796	2802	rBV5	42531	67842	1.27%	0.119%
45	19.651	2827	2833	2840	rBV	4012832	5341558	100.00%	9.357%
46	21.615	3161	3167	3182	rBV	1500295	2719089	50.90%	4.763%
47	24.745	3690	3699	3715	rVB2	1892154	4864521	91.07%	8.522%
48	24.968	3729	3737	3750	rVB	952602	2786152	52.16%	4.881%




Sum of corrected areas: 57084080

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
Data File : BP020900.D
Acq On : 11 Jul 2024 12:19
Operator : MA/JU
Sample : P3138-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

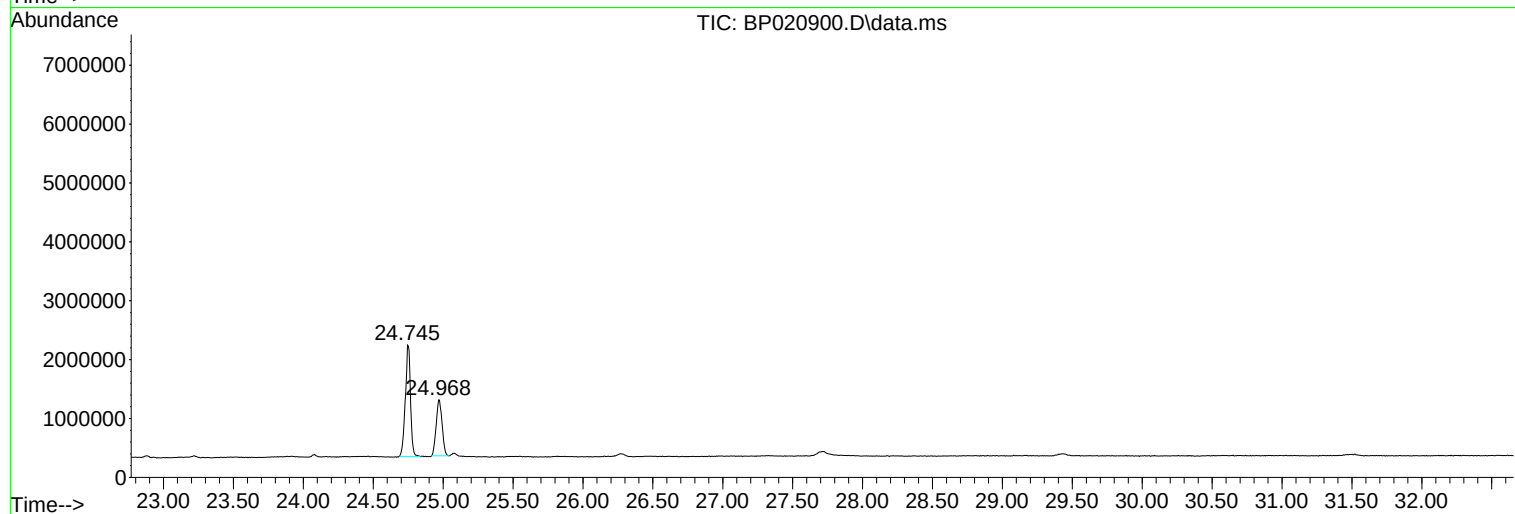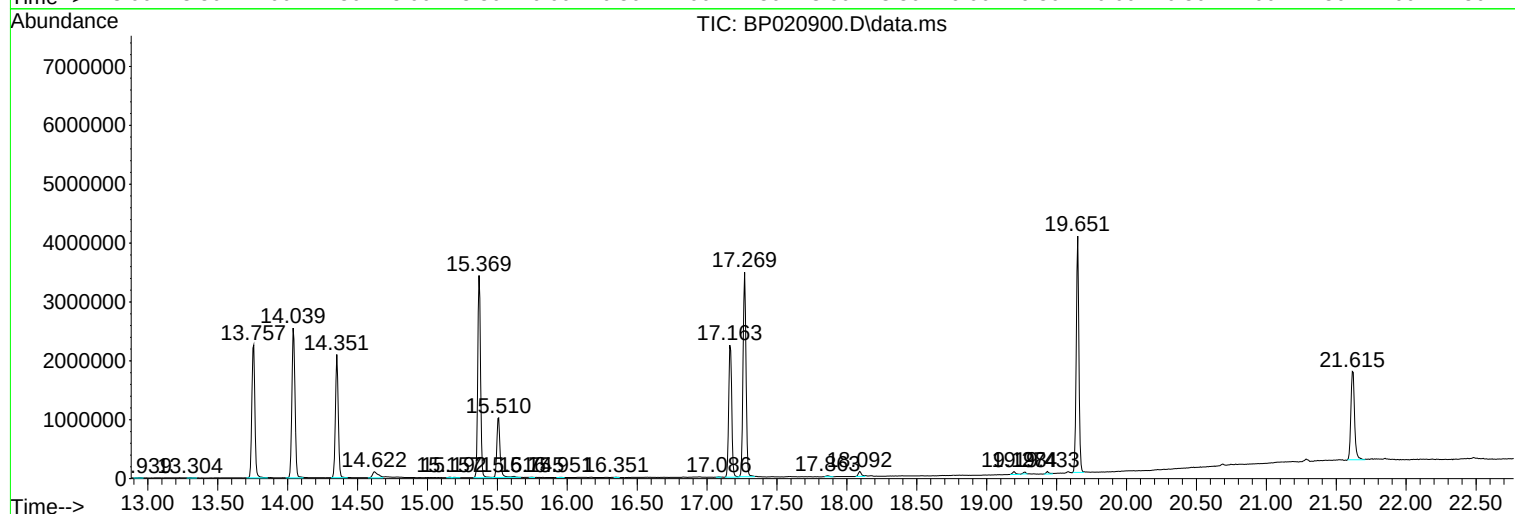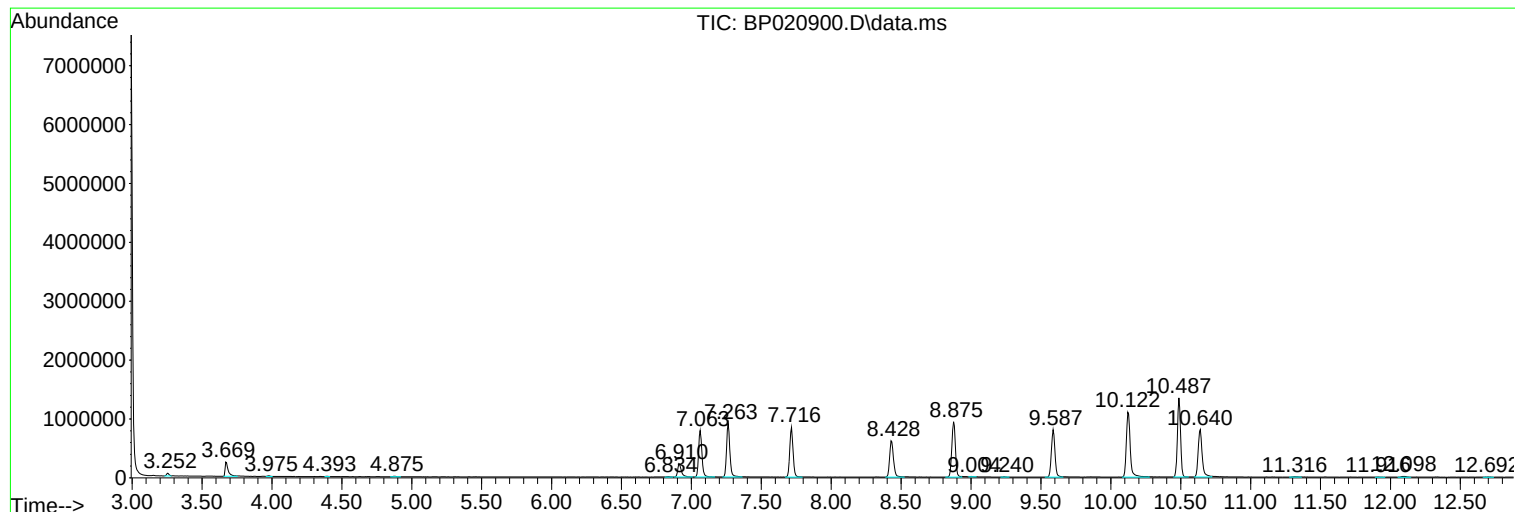

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
Data File : BP020900.D
Acq On : 11 Jul 2024 12:19
Operator : MA/JU
Sample : P3138-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
Data File : BP020900.D
Acq On : 11 Jul 2024 12:19
Operator : MA/JU
Sample : P3138-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
YDZF7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc