

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
 Data File : BP020940.D
 Acq On : 12 Jul 2024 19:27
 Operator : MA/JU
 Sample : PB162041BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK041

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP020940.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	41	45	50	rVB	46327	60840	1.37%	0.144%
2	3.664	112	115	130	rBV	491671	774622	17.41%	1.830%
3	3.970	164	167	173	rVB2	10188	13912	0.31%	0.033%
4	6.911	660	667	685	rBV	591211	1033802	23.23%	2.442%
5	7.058	685	692	702	rBV	491218	803484	18.05%	1.898%
6	7.252	718	725	743	rBV	645535	1055596	23.72%	2.493%
7	7.711	796	803	815	rBV	555355	904577	20.33%	2.137%
8	8.422	916	924	942	rBV	679545	1295644	29.11%	3.060%
9	8.863	991	999	1009	rBV	597822	1014223	22.79%	2.396%
10	9.581	1111	1121	1136	rBV	504306	903863	20.31%	2.135%
11	10.116	1205	1212	1236	rBV	704608	1328696	29.86%	3.138%
12	10.481	1266	1274	1291	rBV	723964	1241801	27.90%	2.933%
13	10.634	1291	1300	1314	rBV	587908	1228143	27.60%	2.901%
14	12.087	1540	1547	1553	rBV3	11923	23681	0.53%	0.056%
15	13.751	1822	1830	1846	rBV	1427881	2113285	47.49%	4.991%
16	13.869	1846	1850	1854	rVB7	3033	5181	0.12%	0.012%
17	14.034	1871	1878	1895	rBV	1565663	2383391	53.56%	5.629%
18	14.346	1924	1931	1944	rVB	1044049	1704460	38.30%	4.026%
19	14.604	1969	1975	1988	rBV	372687	858086	19.28%	2.027%
20	14.875	2018	2021	2026	rVB7	3643	5477	0.12%	0.013%
21	15.357	2095	2103	2113	rBV	2042212	2983703	67.05%	7.047%
22	15.504	2121	2128	2141	rBV	583605	1036602	23.29%	2.448%
23	15.610	2143	2146	2151	rVB6	10993	16579	0.37%	0.039%
24	15.875	2188	2191	2196	rVB6	3928	7159	0.16%	0.017%
25	15.951	2200	2204	2208	rBV6	2829	5413	0.12%	0.013%
26	16.163	2235	2240	2246	rVB6	8866	14092	0.32%	0.033%
27	16.569	2303	2309	2311	rBV7	3870	7928	0.18%	0.019%
28	16.828	2347	2353	2357	rBV9	4895	9049	0.20%	0.021%
29	17.163	2403	2410	2420	rBV	1547873	2138244	48.05%	5.050%
30	17.269	2420	2428	2443	rVV	2125034	3440454	77.31%	8.126%
31	17.863	2524	2529	2531	rBV6	8989	11853	0.27%	0.028%
32	18.098	2564	2569	2579	rBV3	61114	144904	3.26%	0.342%
33	19.198	2752	2756	2761	rBV2	31028	48242	1.08%	0.114%
34	19.275	2765	2769	2773	rBV2	33327	57136	1.28%	0.135%
35	19.428	2792	2795	2798	rBV5	28577	37130	0.83%	0.088%
36	19.651	2827	2833	2843	rBV2	2838947	4214356	94.70%	9.954%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
Data File : BP020940.D
Acq On : 12 Jul 2024 19:27
Operator : MA/JU
Sample : PB162041BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK041

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Title : SVOA CALIBRATION

37	21.616	3161	3167	3177	rBV2	1329887	2459631	55.27%	5.809%
38	24.727	3686	3696	3709	rVB2	1664107	4450245	100.00%	10.511%
39	24.951	3726	3734	3744	rBV	1028470	2502710	56.24%	5.911%




Sum of corrected areas: 42338194

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
Data File : BP020940.D
Acq On : 12 Jul 2024 19:27
Operator : MA/JU
Sample : PB162041BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK041

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

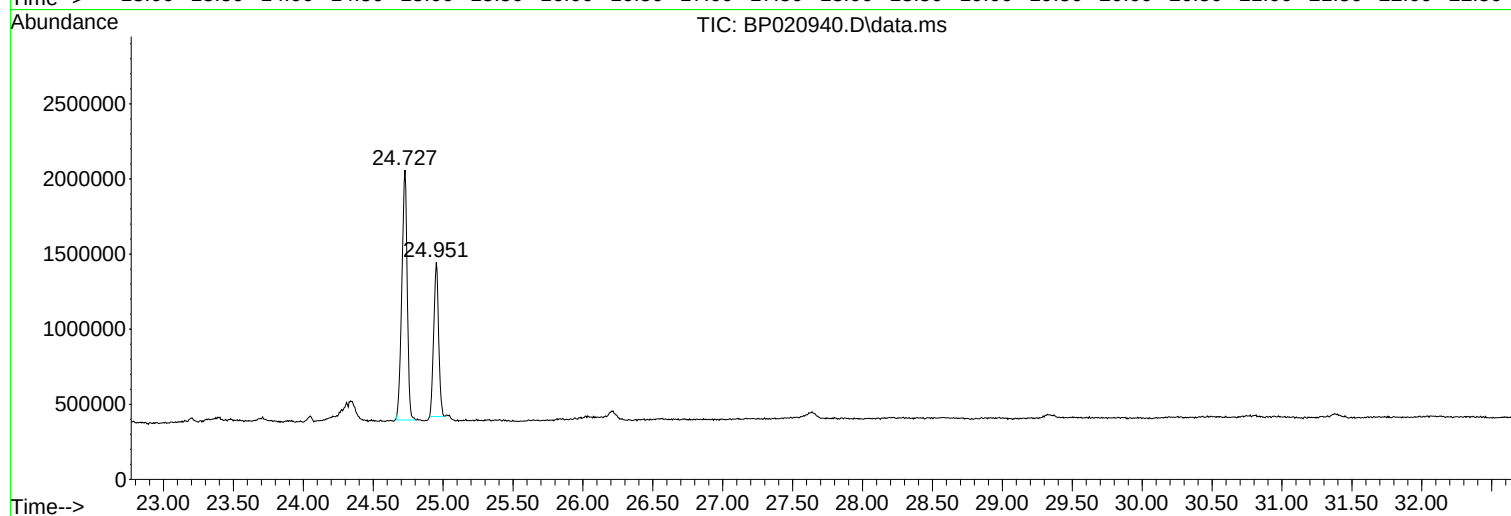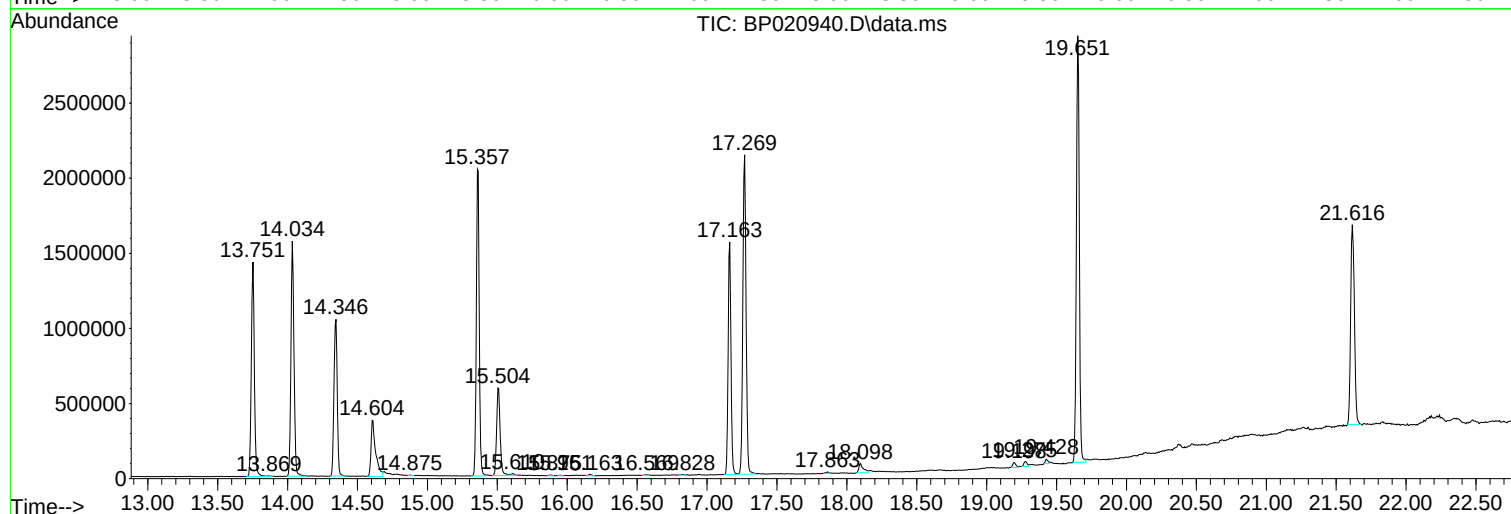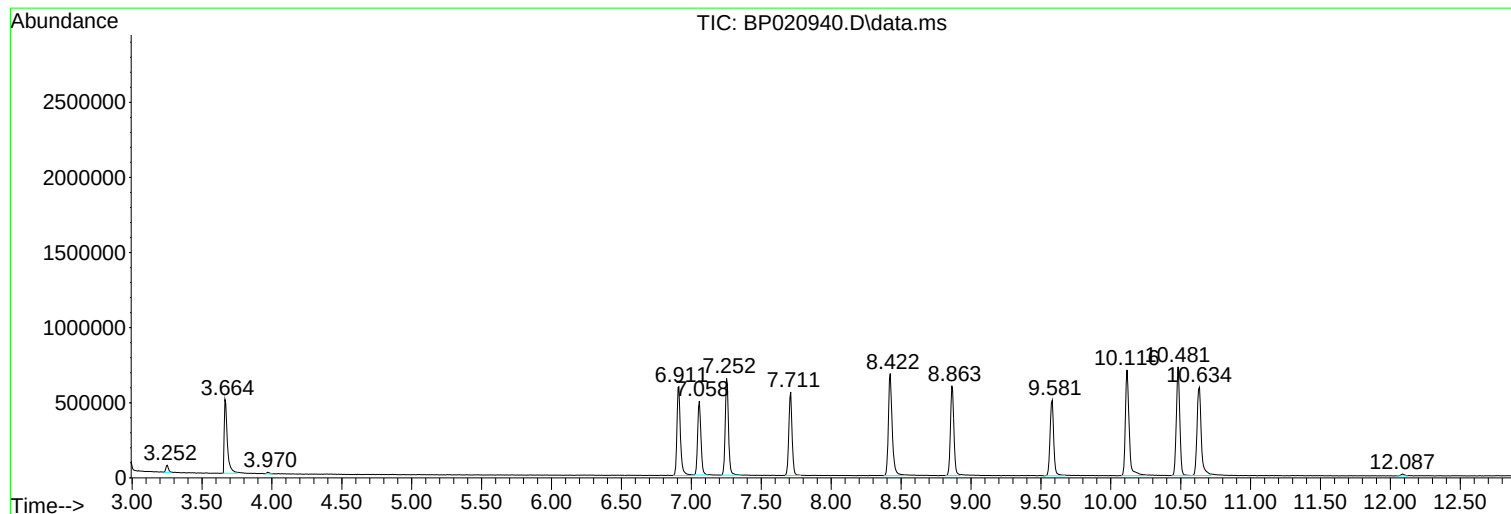

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
Data File : BP020940.D
Acq On : 12 Jul 2024 19:27
Operator : MA/JU
Sample : PB162041BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK041

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071124\
Data File : BP020940.D
Acq On : 12 Jul 2024 19:27
Operator : MA/JU
Sample : PB162041BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK041

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071024.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc