
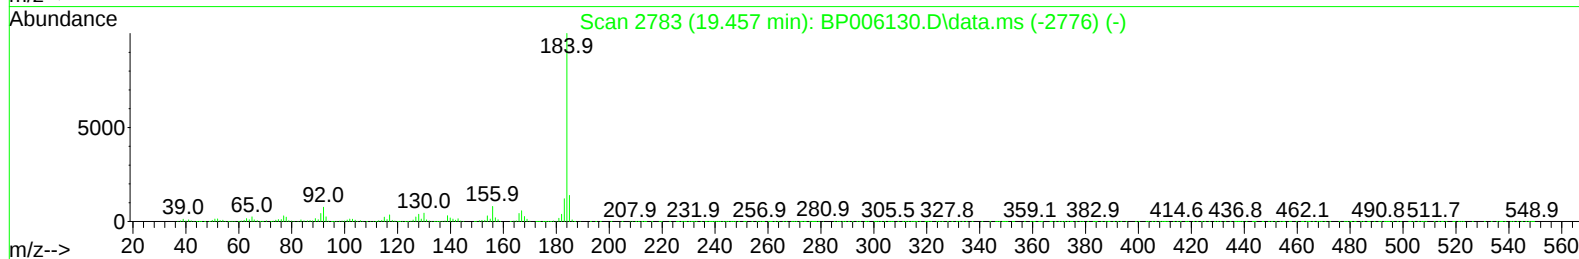
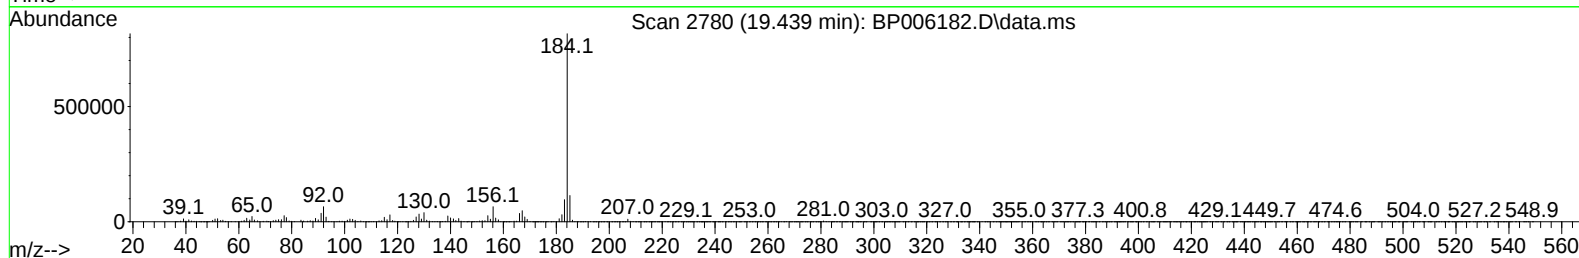


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071221\
Data File : BP006182.D
Acq On : 12 Jul 2021 13:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 14:30:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 07 16:08:13 2021
Response via : Initial Calibration

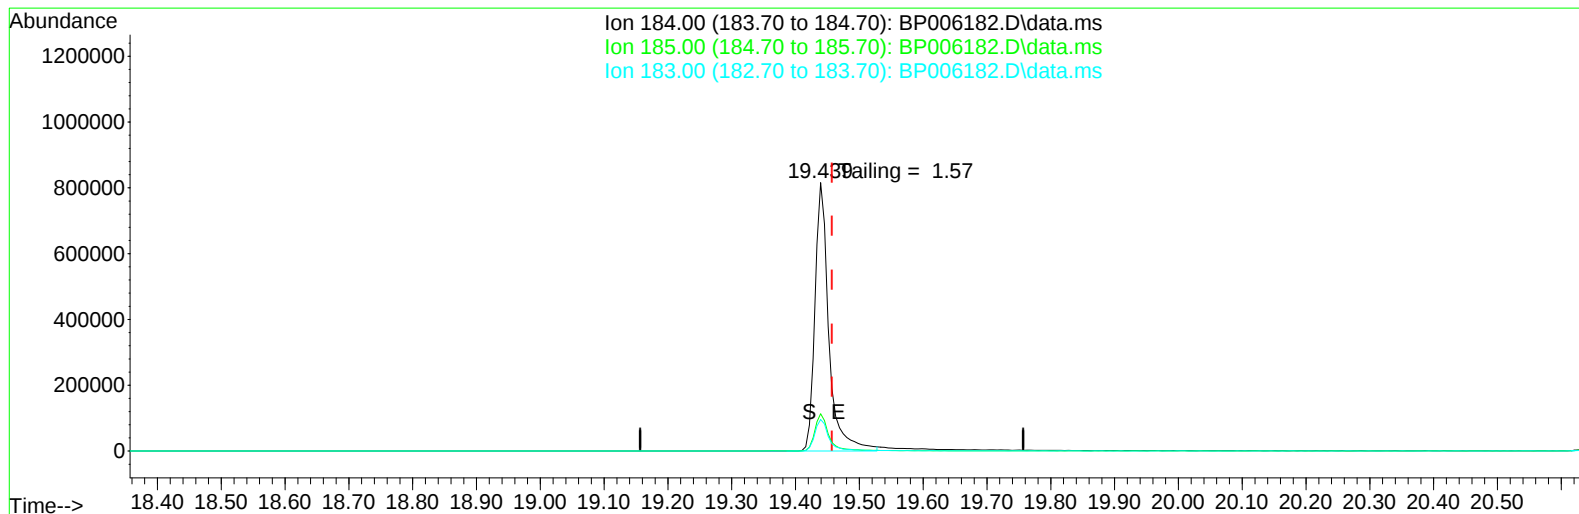




TIC: BP006182.D\data.ms

(77) Benzidine**19.439min (-0.018) 40970.70 ng****response 1284133**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.92
183.00	11.90	11.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071221\
Data File : BP006182.D
Acq On : 12 Jul 2021 13:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 12 14:30:56 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 07 16:08:13 2021
Response via : Initial Calibration

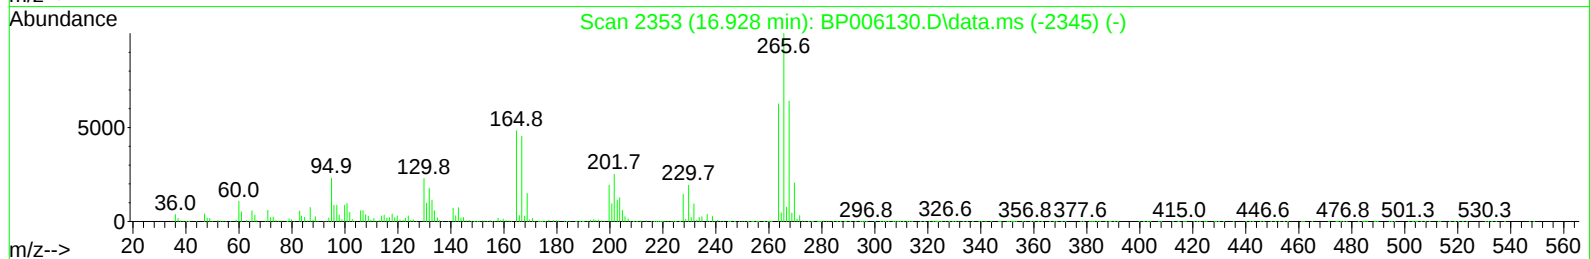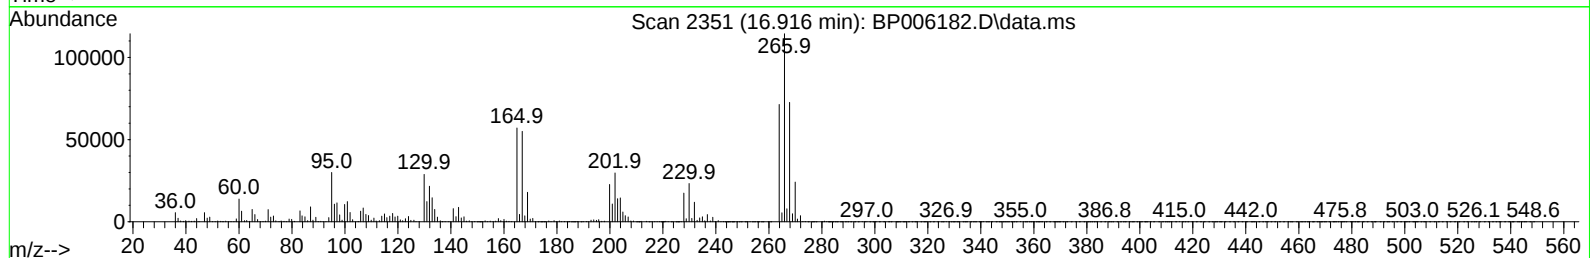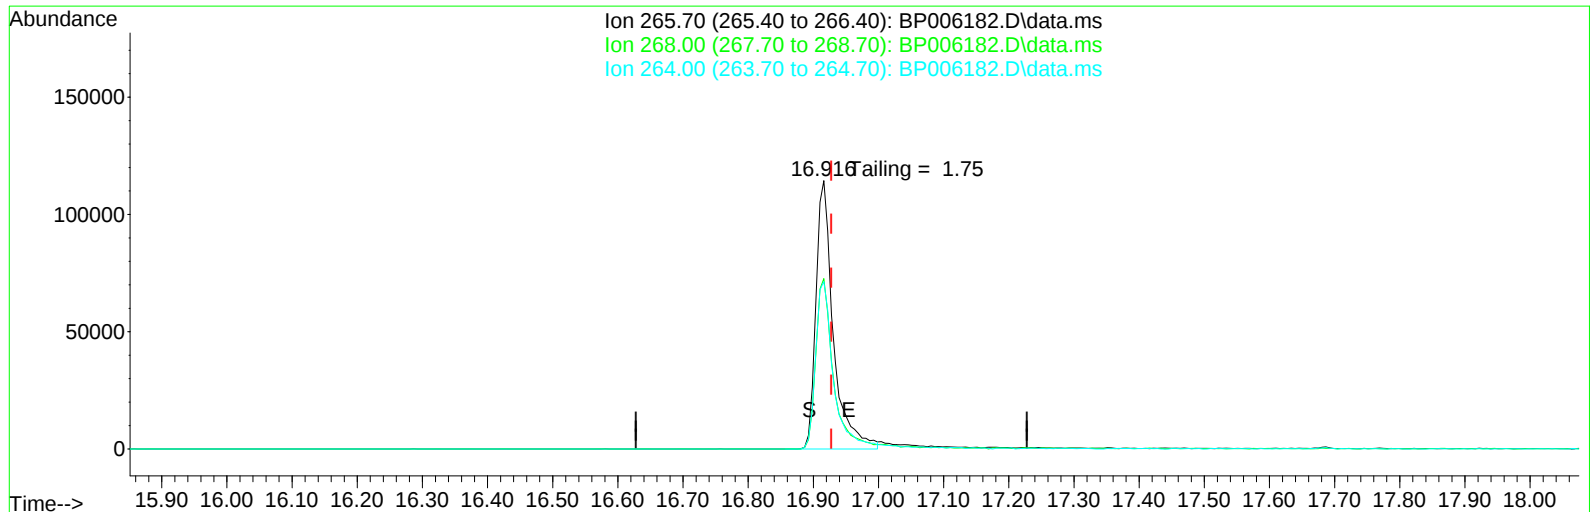

TIC: BP006182.D\data.ms

(70) Pentachlorophenol (C)

16.916min (-0.012) 145294.62 ng

response 221279

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.50
264.00	62.90	62.35
0.00	0.00	0.00