
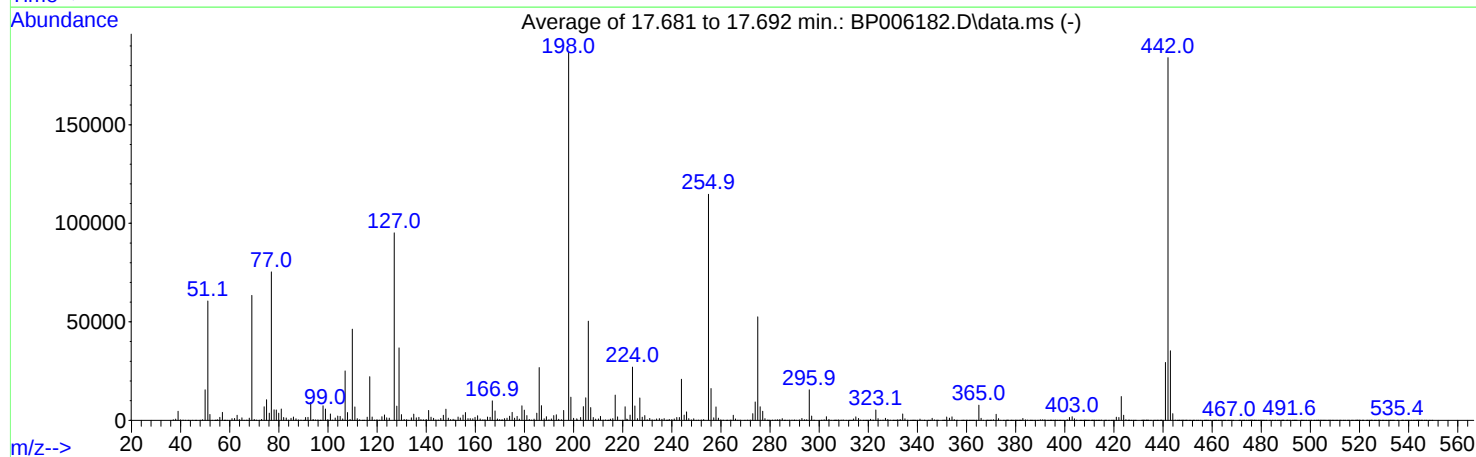


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071221\
 Data File : BP006182.D
 Acq On : 12 Jul 2021 13:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 12 14:59:51 2021

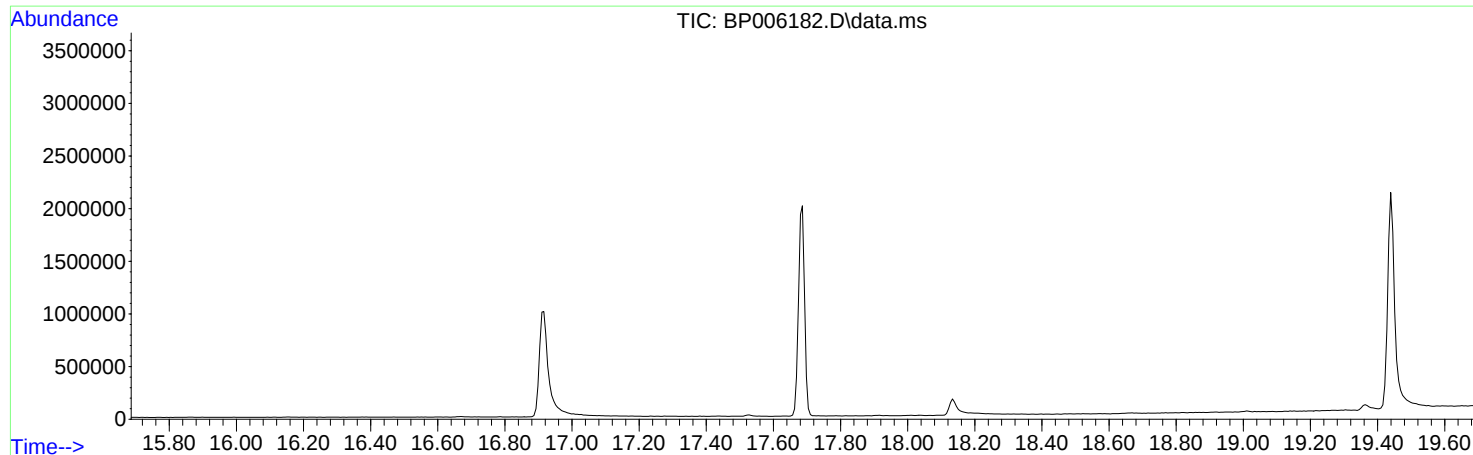




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	60584	PASS
68	69	0.00	2	1.7	1105	PASS
69	198	0.00	100	34.0	63411	PASS
70	69	0.00	2	0.7	461	PASS
127	198	10	80	51.0	95169	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	186667	PASS
199	198	5	9	6.3	11820	PASS
275	198	10	60	28.1	52506	PASS
365	198	1	100	4.1	7730	PASS
441	198	0.01	100	15.7	29379	PASS
442	442	100	100	100.0	184079	PASS
443	442	15	24	19.2	35301	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071221\
 Data File : BP006182.D
 Acq On : 12 Jul 2021 13:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 12 14:30:56 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 07 16:08:13 2021
 Response via : Initial Calibration

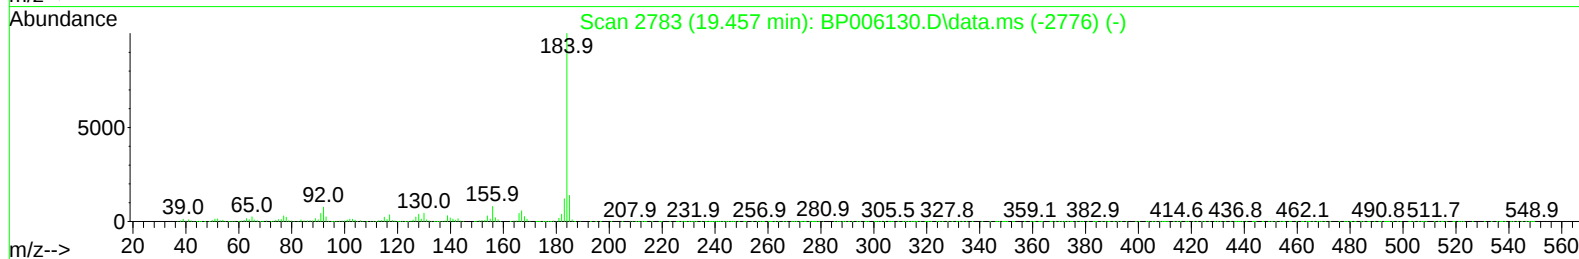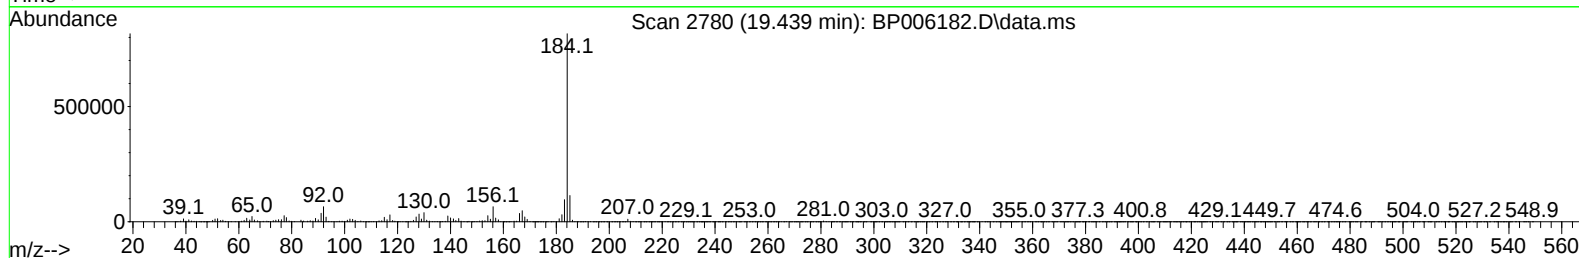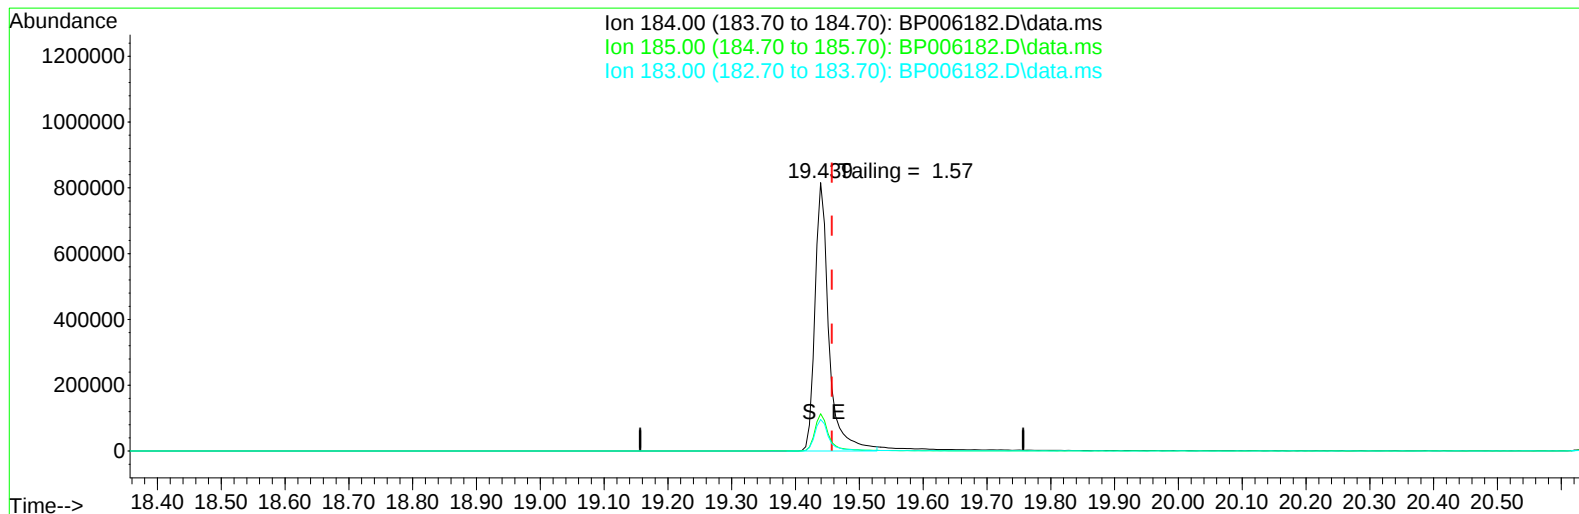

TIC: BP006182.D\data.ms

(77) Benzidine

19.439min (-0.018) 40970.70 ng




response 1284133

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.92
183.00	11.90	11.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071221\
 Data File : BP006182.D
 Acq On : 12 Jul 2021 13:44
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 12 14:30:56 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 07 16:08:13 2021
 Response via : Initial Calibration

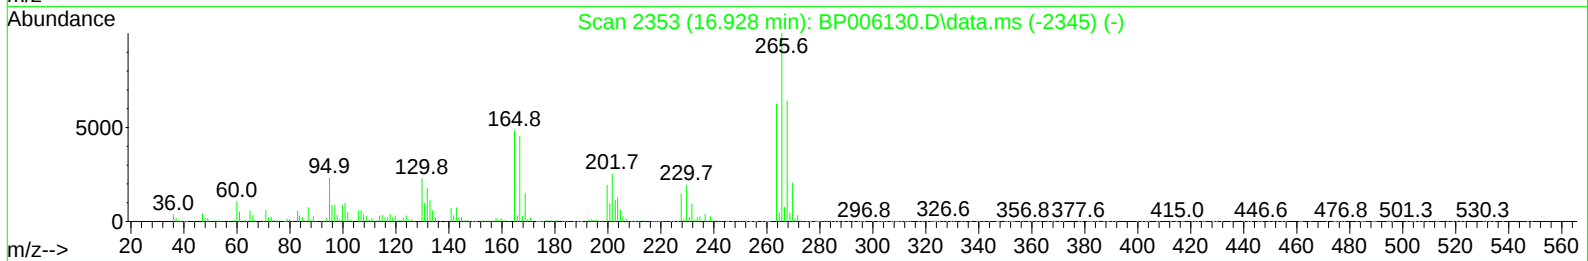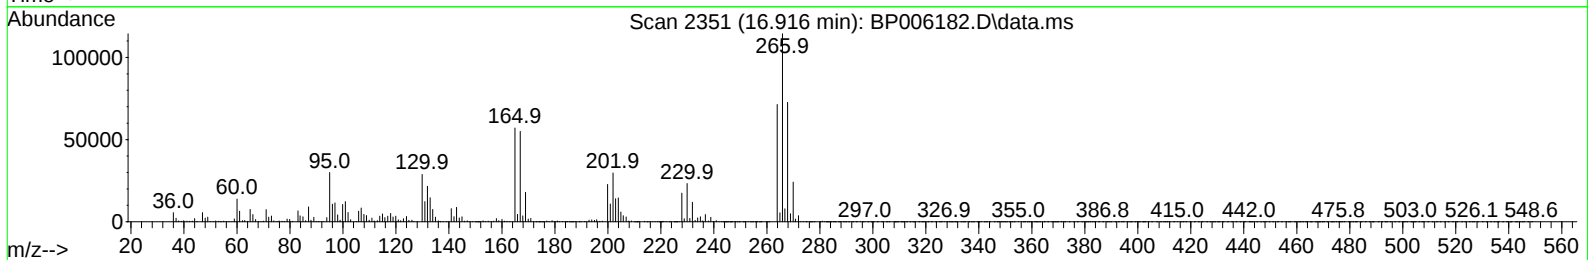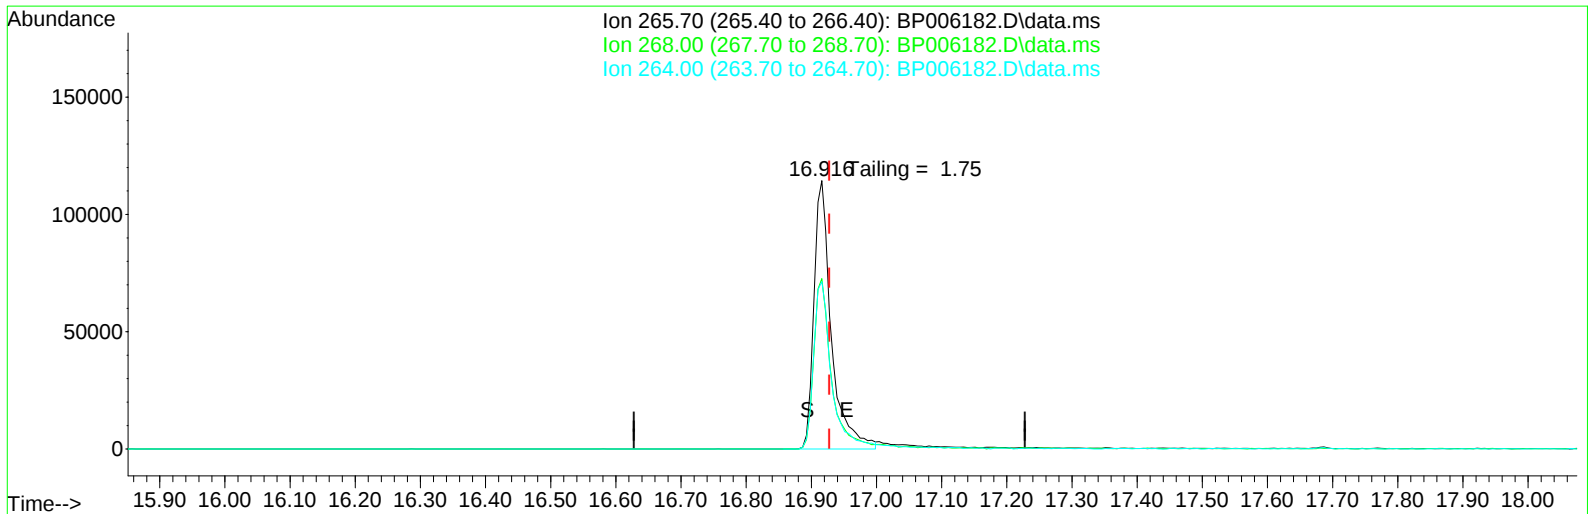

TIC: BP006182.D\data.ms

(70) Pentachlorophenol (C)

16.916min (-0.012) 145294.62 ng

response 221279

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.50
264.00	62.90	62.35
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/12/2021	BNA_P	BP006182.D
Compound Name	Response	Retention Time
DDT	672447	20.62
DDD	5754	20.21
DDE	2168	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7922	680369	1.16

Instrument :
BNA_P
ClientSampleId :
DFTPP