
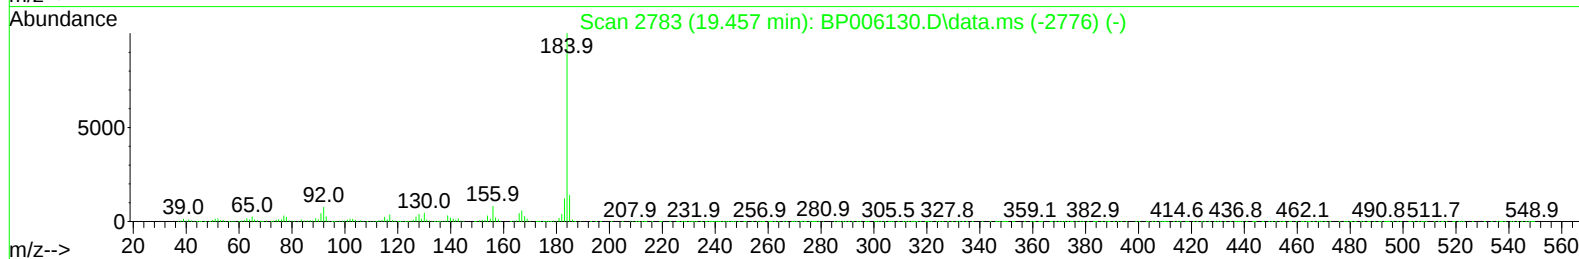
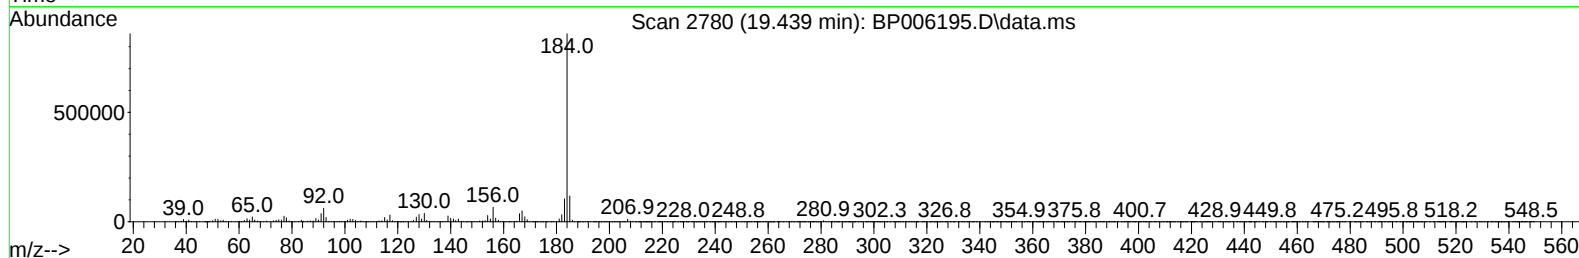


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071321\
 Data File : BP006195.D
 Acq On : 13 Jul 2021 11:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 12:38:38 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 14:59:51 2021
 Response via : Initial Calibration

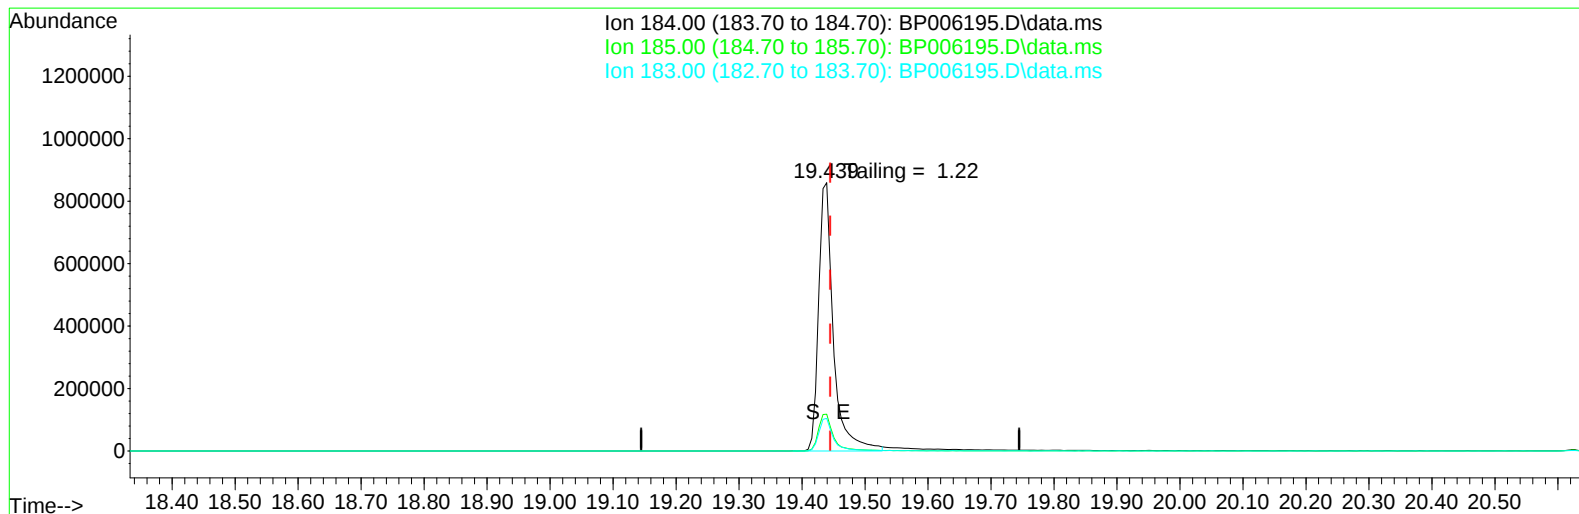




TIC: BP006195.D\data.ms

(77) Benzidine**19.439min (-0.006) 15096.76 ng****response 1448618**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.70
183.00	11.90	12.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071321\
Data File : BP006195.D
Acq On : 13 Jul 2021 11:08
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 13 12:38:38 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 12 14:59:51 2021
Response via : Initial Calibration

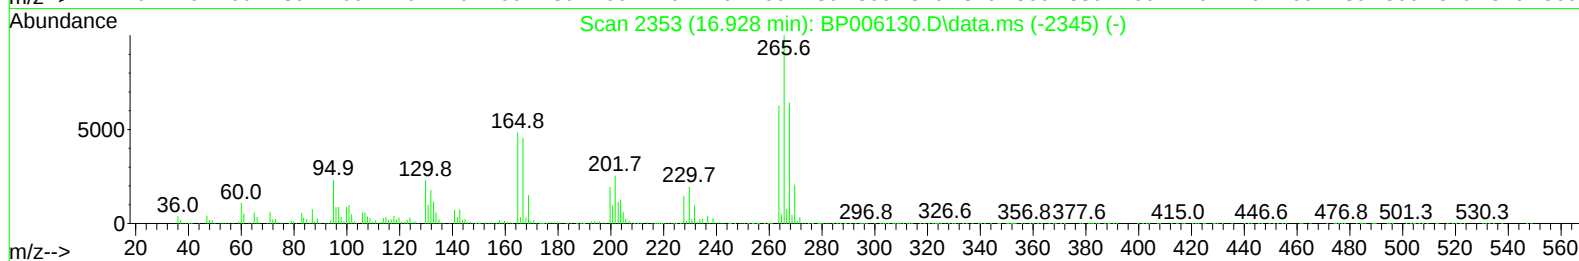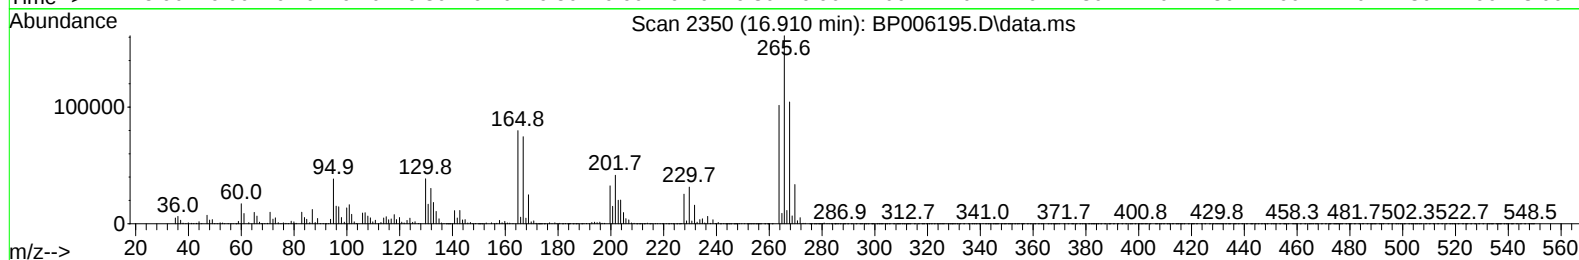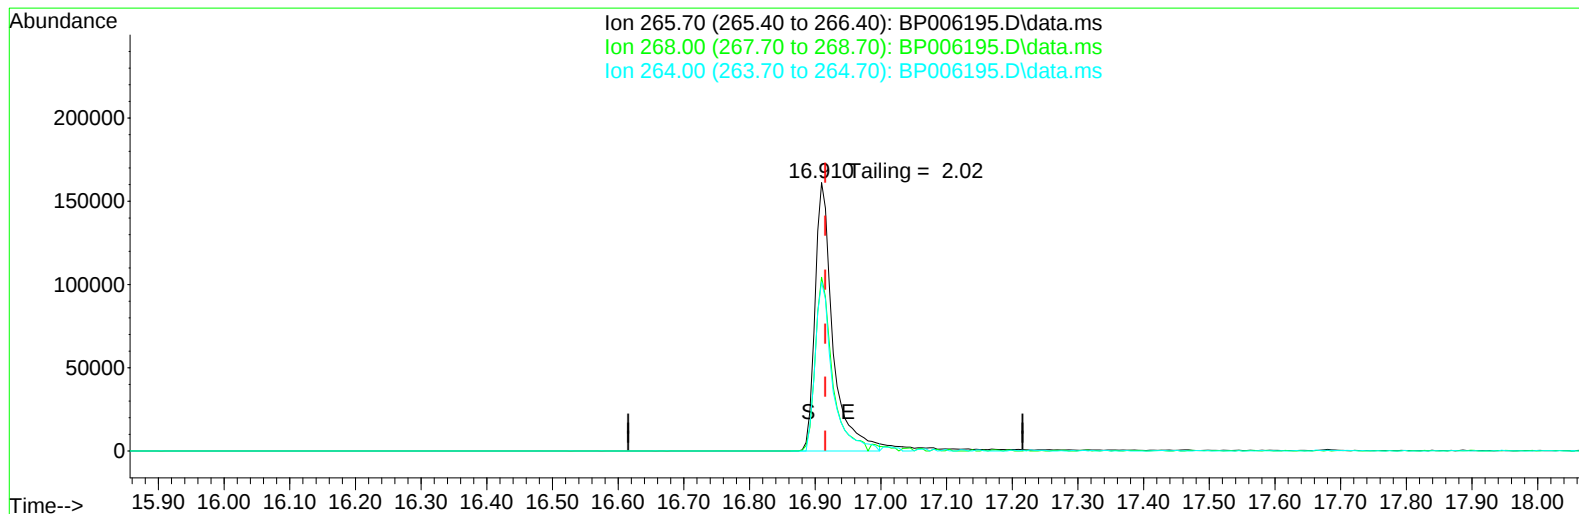

TIC: BP006195.D\data.ms

(70) Pentachlorophenol (C)

16.910min (-0.006) 124606.02 ng

response 314939

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	68.92
264.00	62.90	62.97
0.00	0.00	0.00