
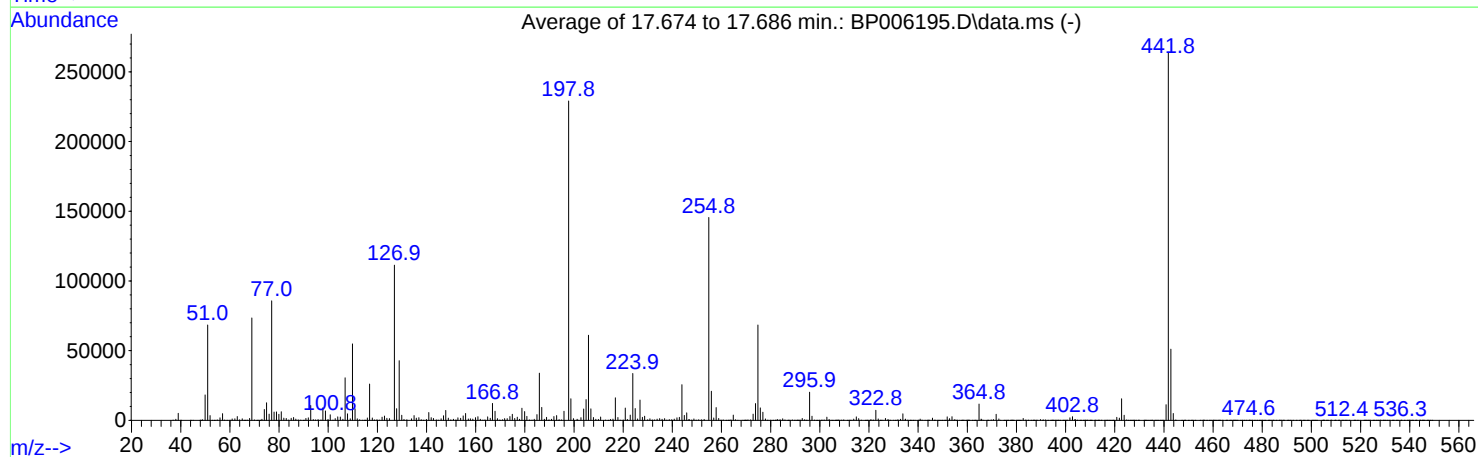


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071321\
 Data File : BP006195.D
 Acq On : 13 Jul 2021 11:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 12 14:59:51 2021

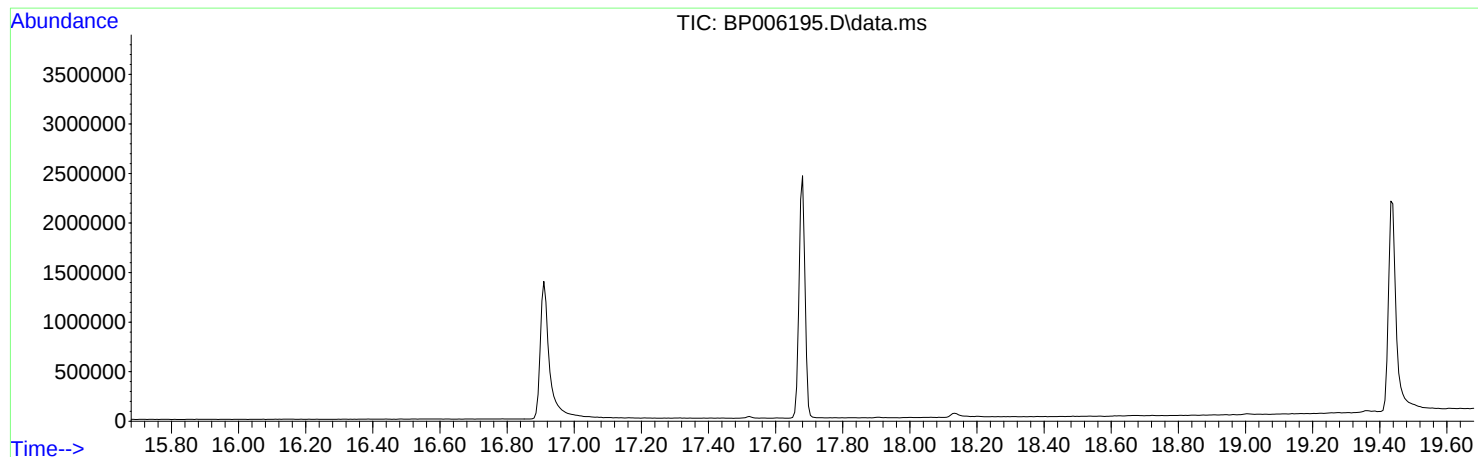




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.9	68428	PASS
68	69	0.00	2	1.9	1425	PASS
69	198	0.00	100	32.1	73453	PASS
70	69	0.00	2	0.6	413	PASS
127	198	10	80	48.6	111339	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	229057	PASS
199	198	5	9	6.8	15529	PASS
275	198	10	60	29.8	68357	PASS
365	198	1	100	5.1	11681	PASS
441	198	0.01	100	4.9	11269	PASS
442	442	100	100	100.0	263872	PASS
443	442	15	24	19.3	51035	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071321\
 Data File : BP006195.D
 Acq On : 13 Jul 2021 11:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 13 12:38:38 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 14:59:51 2021
 Response via : Initial Calibration

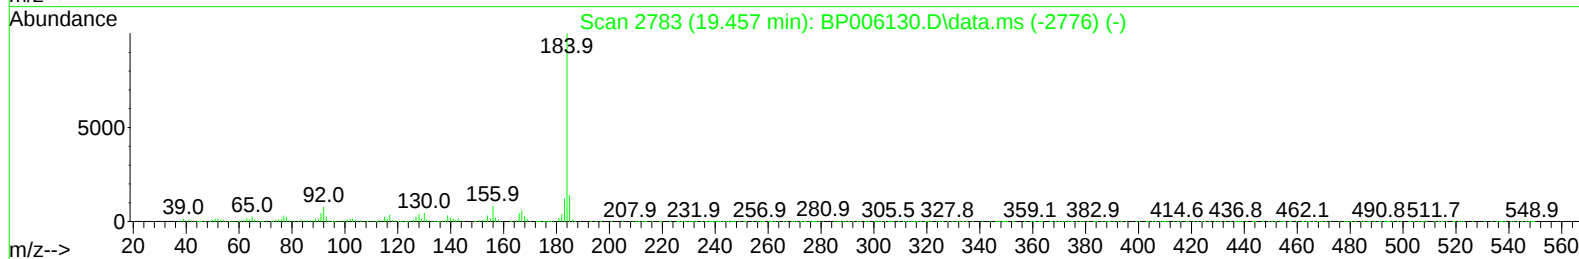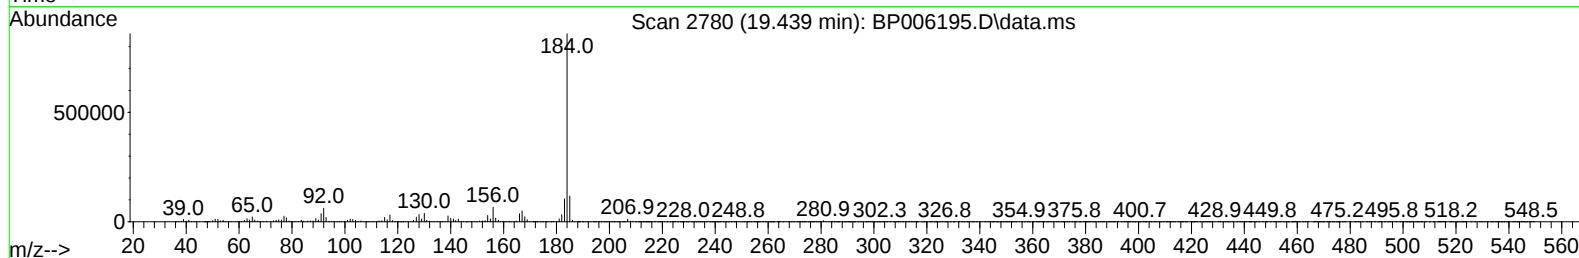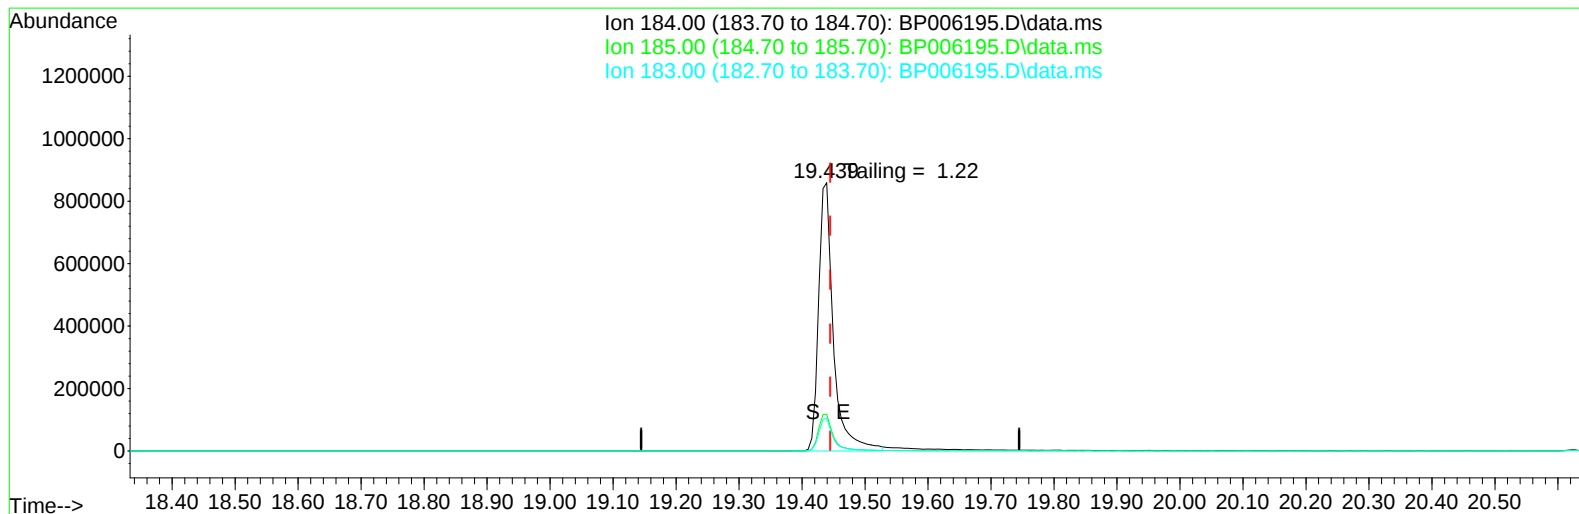

TIC: BP006195.D\data.ms

(77) Benzidine

19.439min (-0.006) 15096.76 ng




response 1448618

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	13.70
183.00	11.90	12.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071321\
 Data File : BP006195.D
 Acq On : 13 Jul 2021 11:08
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 13 12:38:38 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 14:59:51 2021
 Response via : Initial Calibration

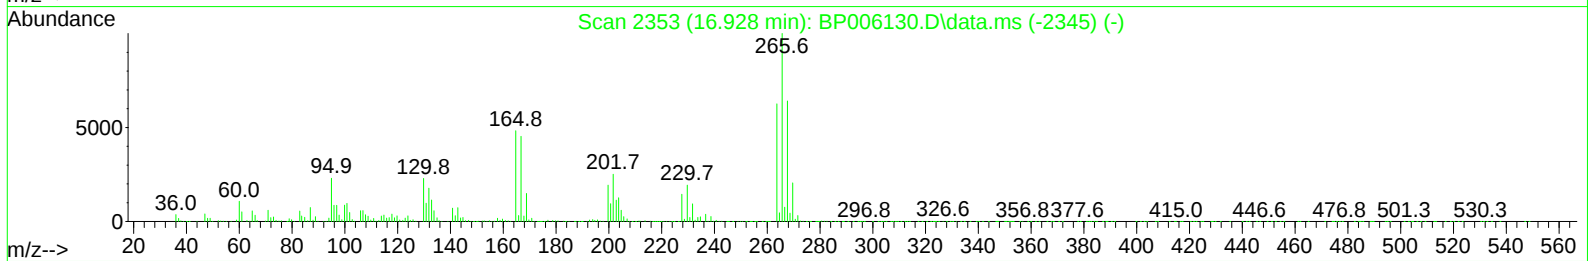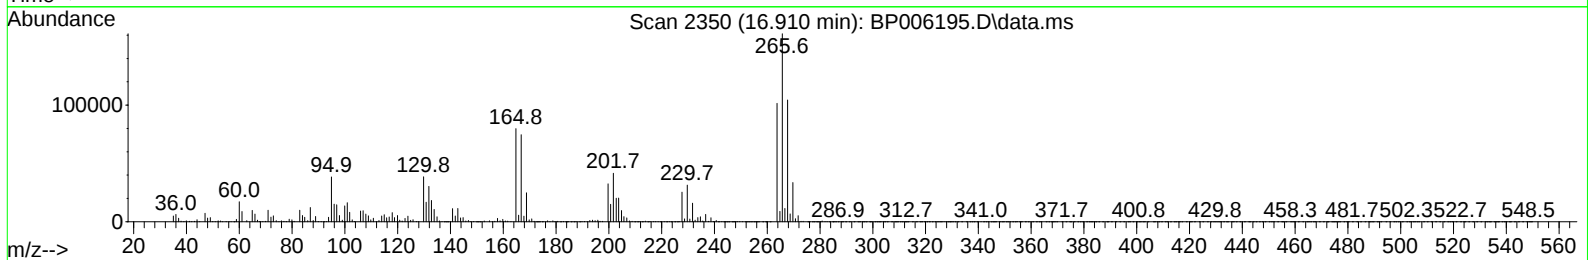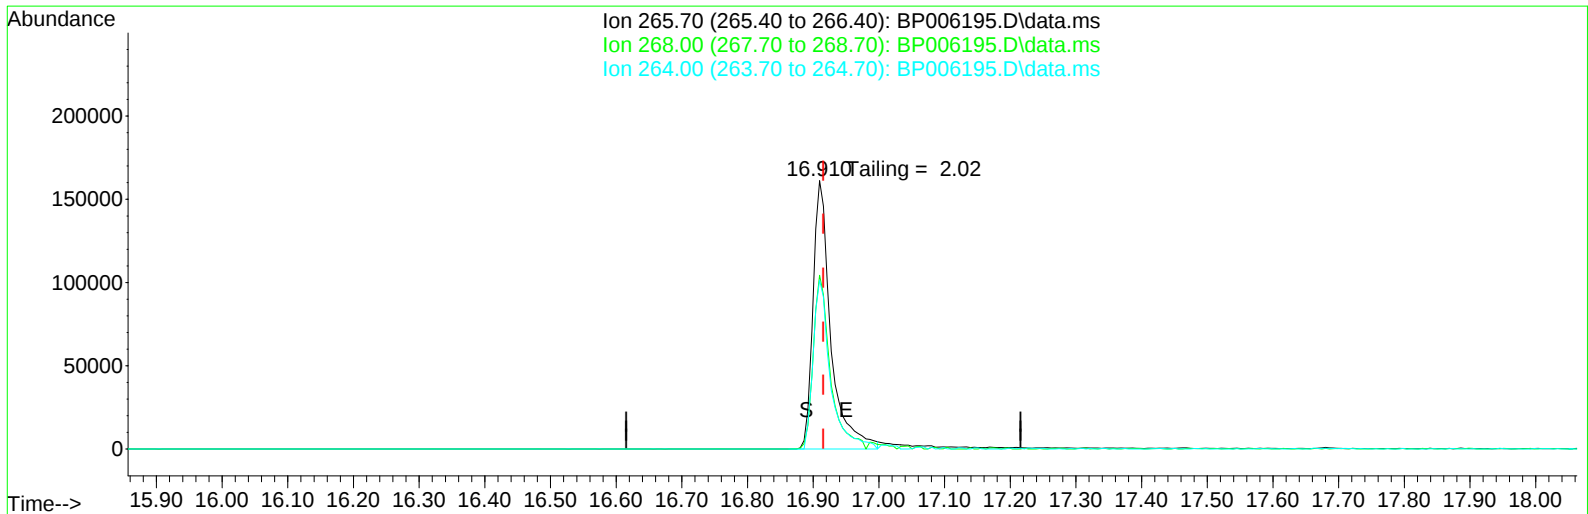

TIC: BP006195.D\data.ms

(70) Pentachlorophenol (C)

16.910min (-0.006) 124606.02 ng

response 314939

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	68.92
264.00	62.90	62.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/13/2021	BNA_P	BP006195.D
Compound Name	Response	Retention Time
DDT	751788	20.62
DDD	6076	20.2
DDE	2955	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9031	760819	1.19