
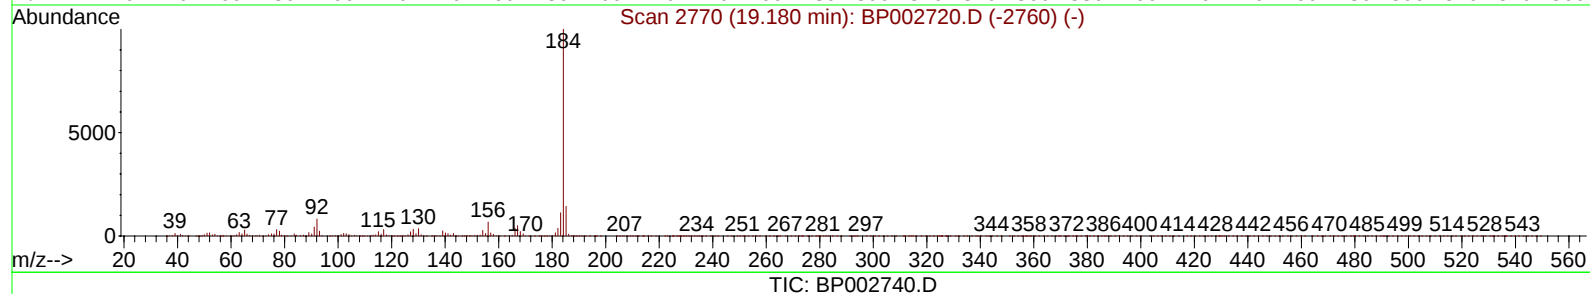
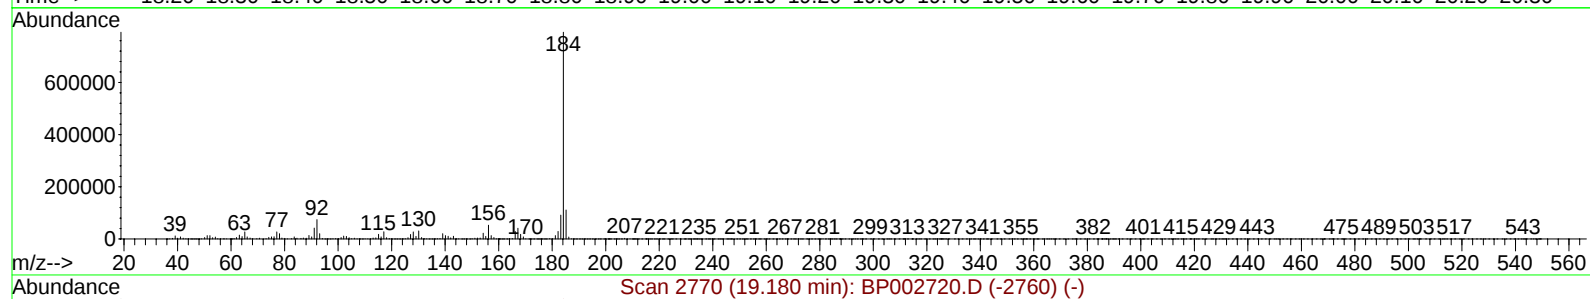


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP071420\
 Data File : BP002740.D
 Acq On : 14 Jul 2020 09:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 15:56:39 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 13 10:54:03 2020
 Response via : Initial Calibration

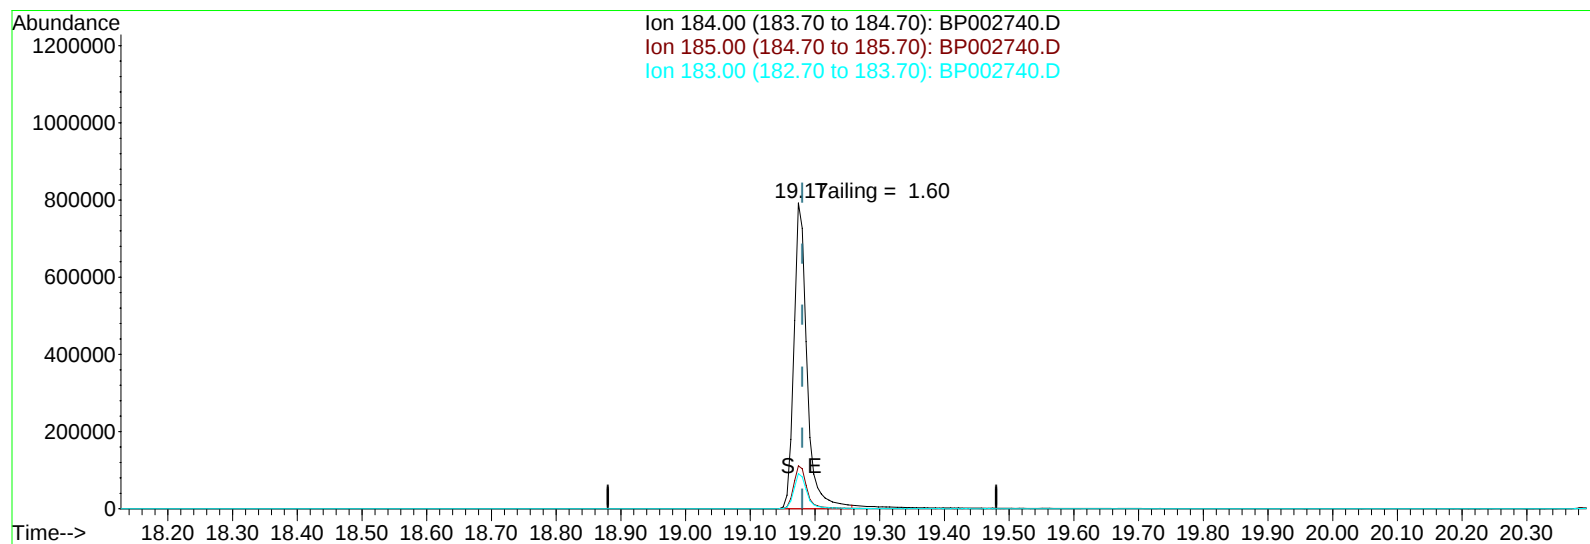

TIC: BP002740.D

(77) Benzidine




19.174min (-0.006) 1492281.70ng

response 1146661

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	14.02
183.00	11.20	11.50
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP071420\
Data File : BP002740.D
Acq On : 14 Jul 2020 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 15:56:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 13 10:54:03 2020
Response via : Initial Calibration

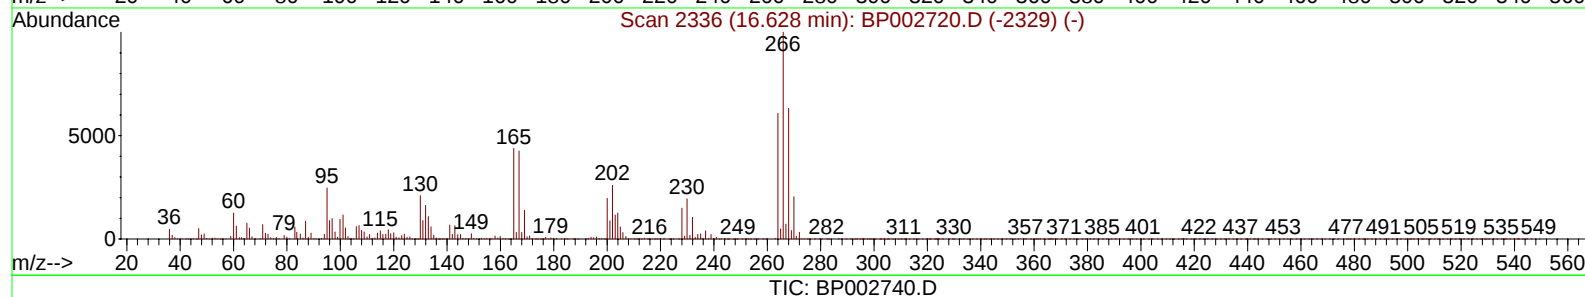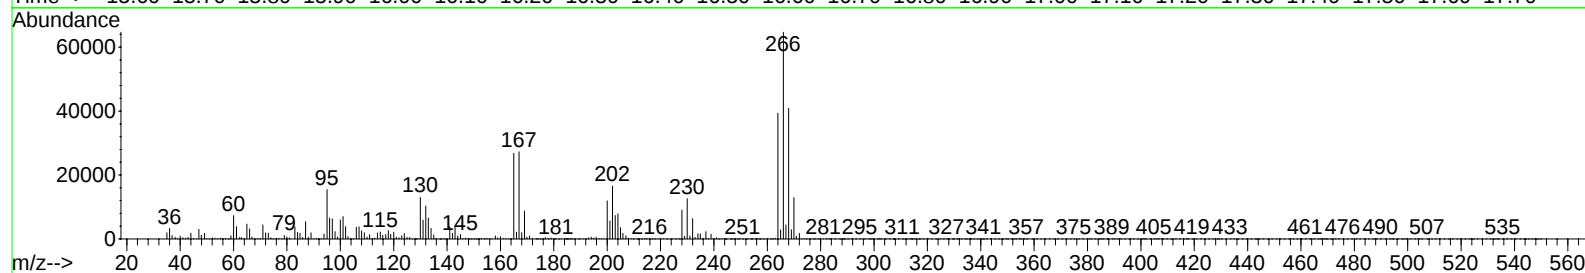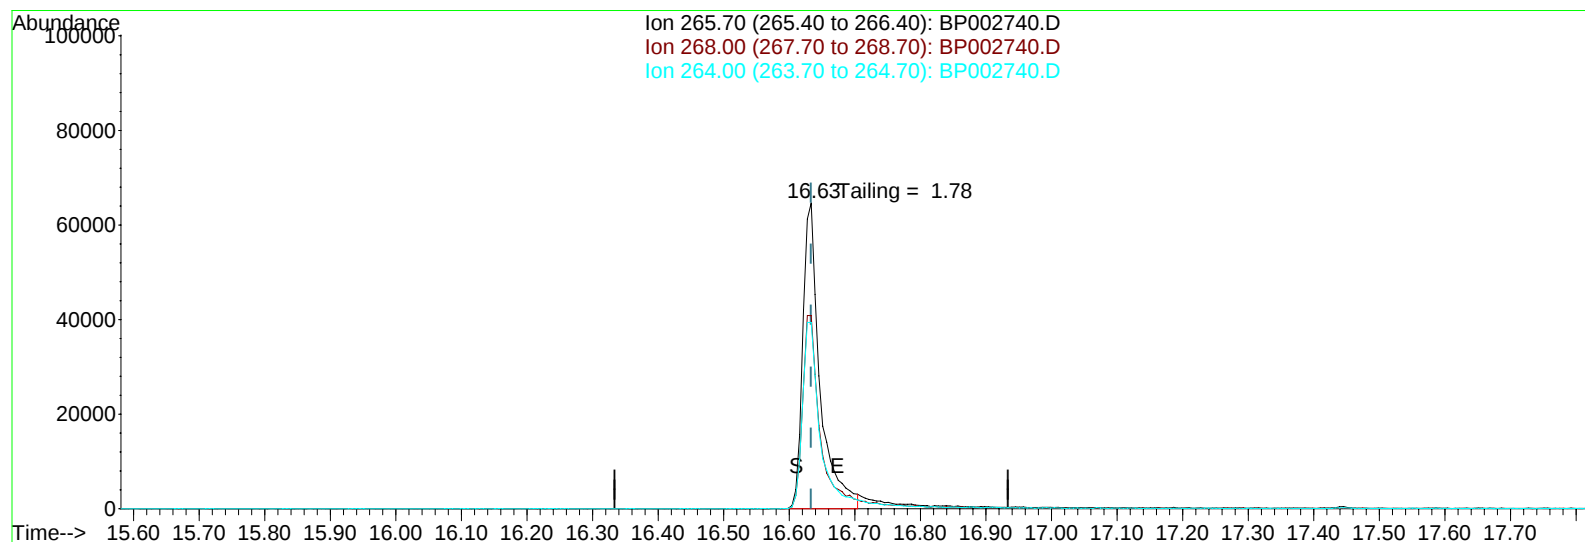

(70) Pentachlorophenol (C)

16.633min (+0.000) 63094.45ng

response 127414

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	63.14
264.00	60.70	60.86
0.00	0.00	0.00