


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071420\
 Data File : BP002740.D
 Acq On : 14 Jul 2020 09:18
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP071020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 13 10:54:03 2020

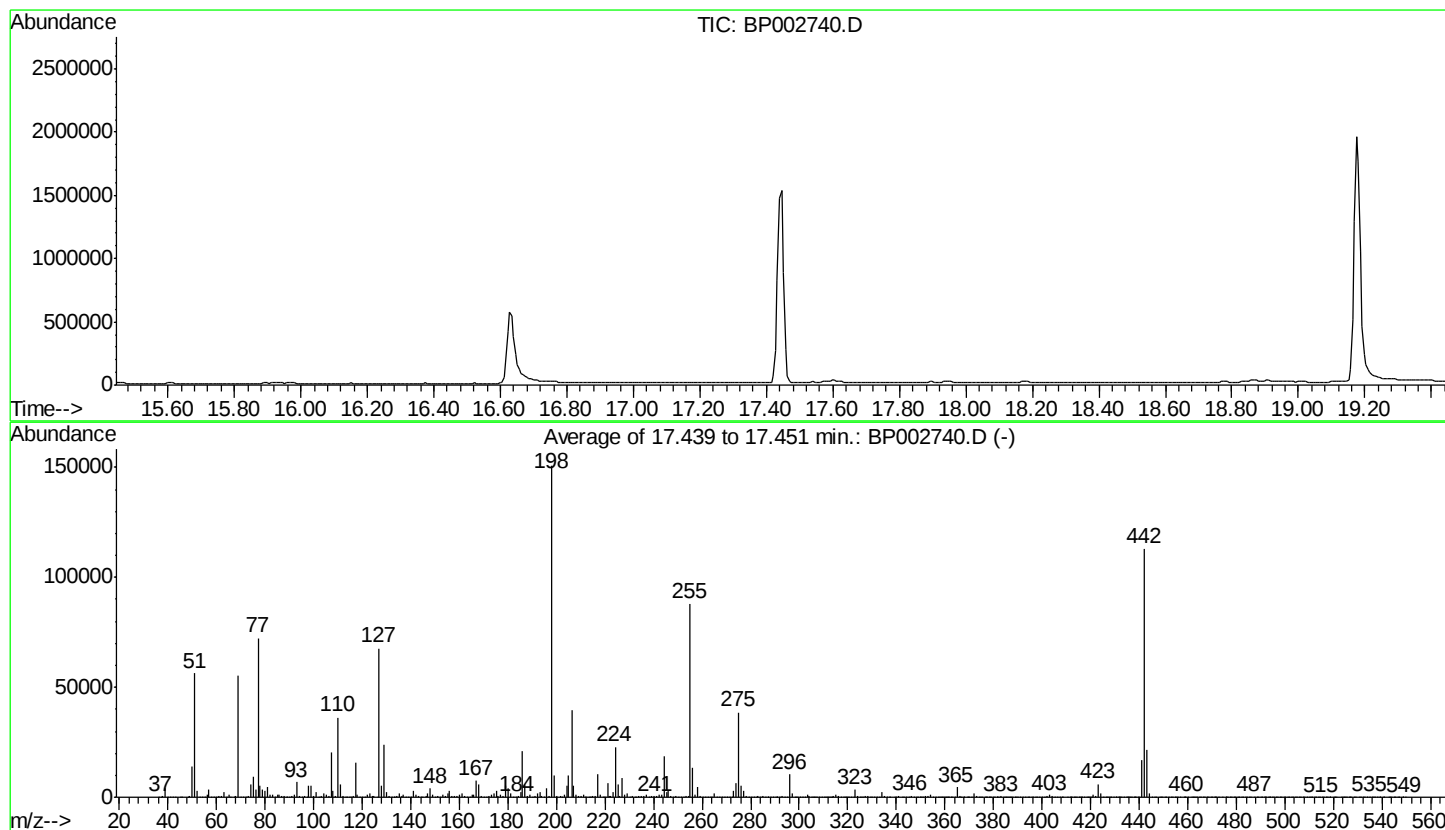

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	56477	PASS
68	69	0.00	2	1.6	862	PASS
69	198	0.00	100	36.8	55505	PASS
70	69	0.00	2	0.5	289	PASS
127	198	10	80	44.9	67702	PASS
197	198	0.00	2	0.4	651	PASS
198	198	100	100	100.0	150848	PASS
199	198	5	9	6.6	9955	PASS
275	198	10	60	25.6	38598	PASS
365	198	1	100	3.0	4525	PASS
441	198	0.01	100	11.1	16810	PASS
442	198	50	100	75.0	113135	PASS
443	442	15	24	19.1	21592	PASS