
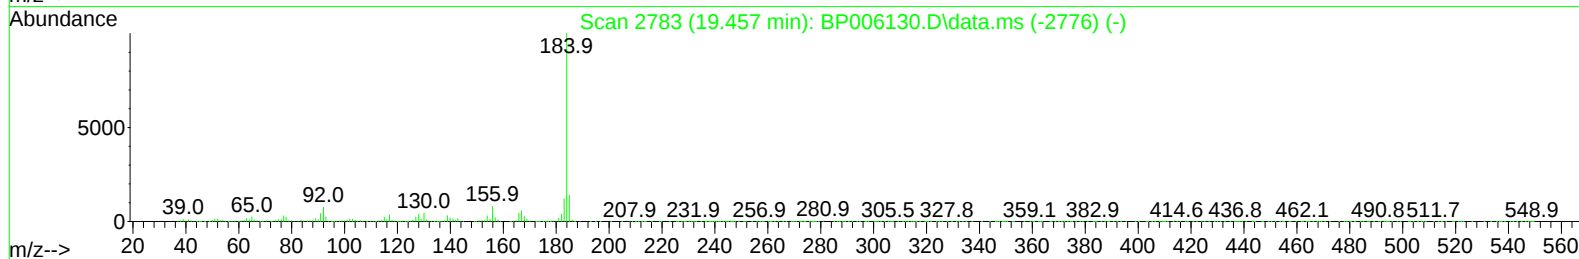
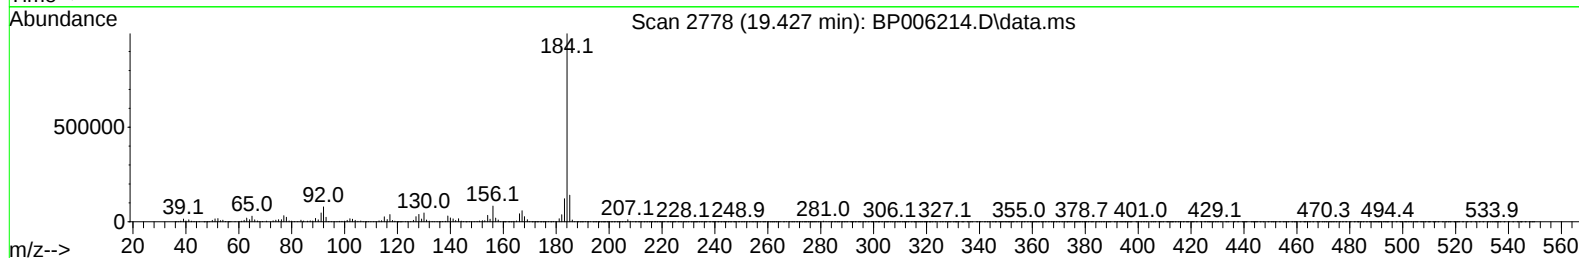


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071421\
 Data File : BP006214.D
 Acq On : 14 Jul 2021 12:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 13:59:18 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 14:59:51 2021
 Response via : Initial Calibration

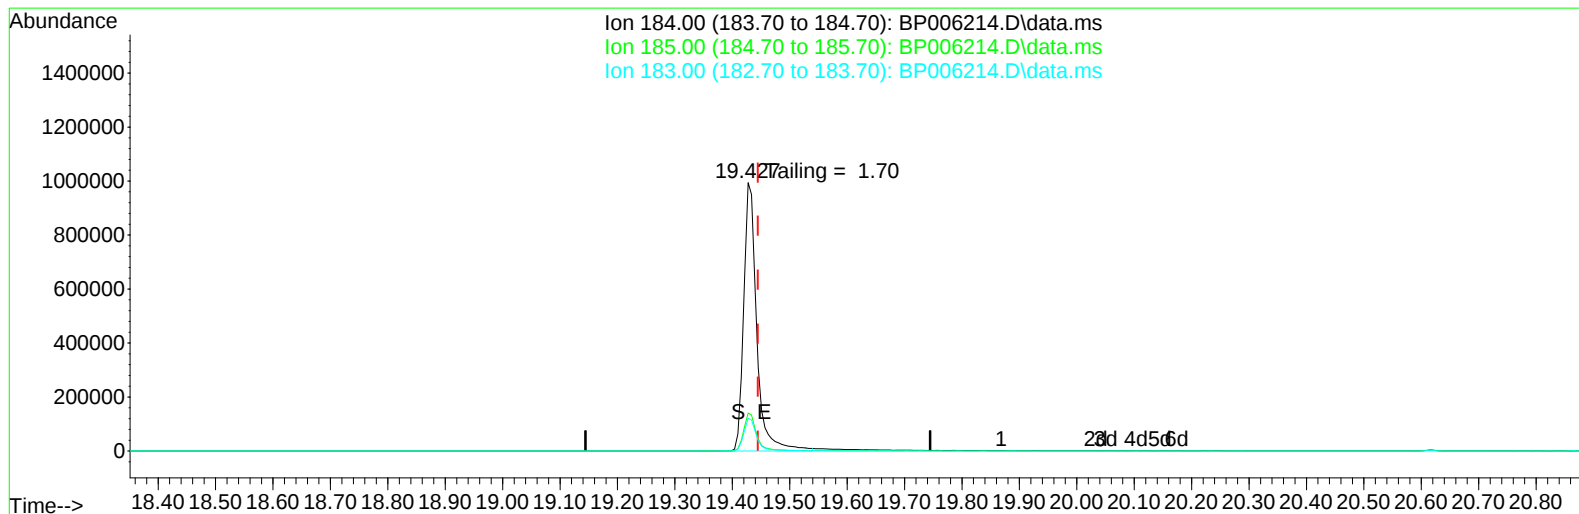

TIC: BP006214.D\data.ms

(77) Benzidine




19.427min (-0.017) 367945.30 ng m

response 1549292

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.16
183.00	11.90	12.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071421\
 Data File : BP006214.D
 Acq On : 14 Jul 2021 12:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 14 13:59:18 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 14:59:51 2021
 Response via : Initial Calibration

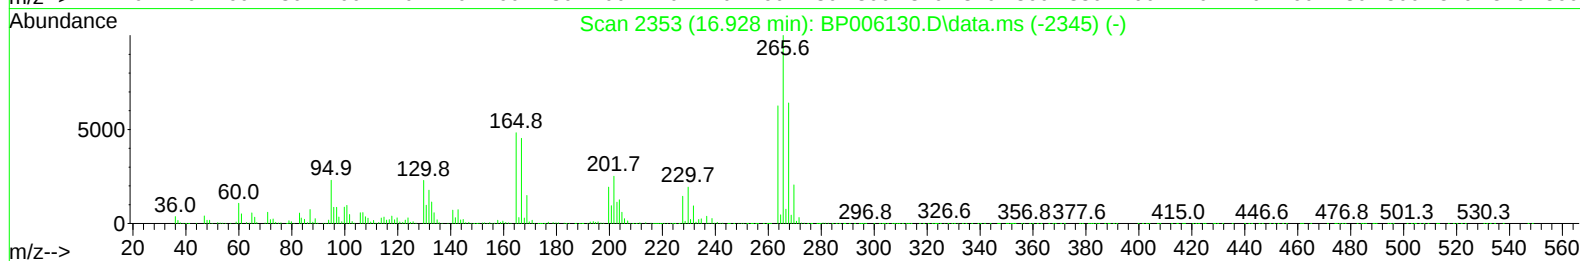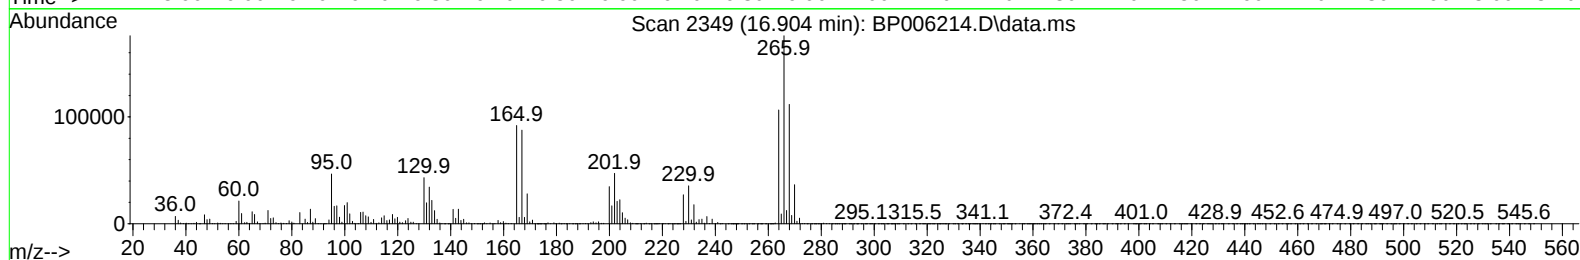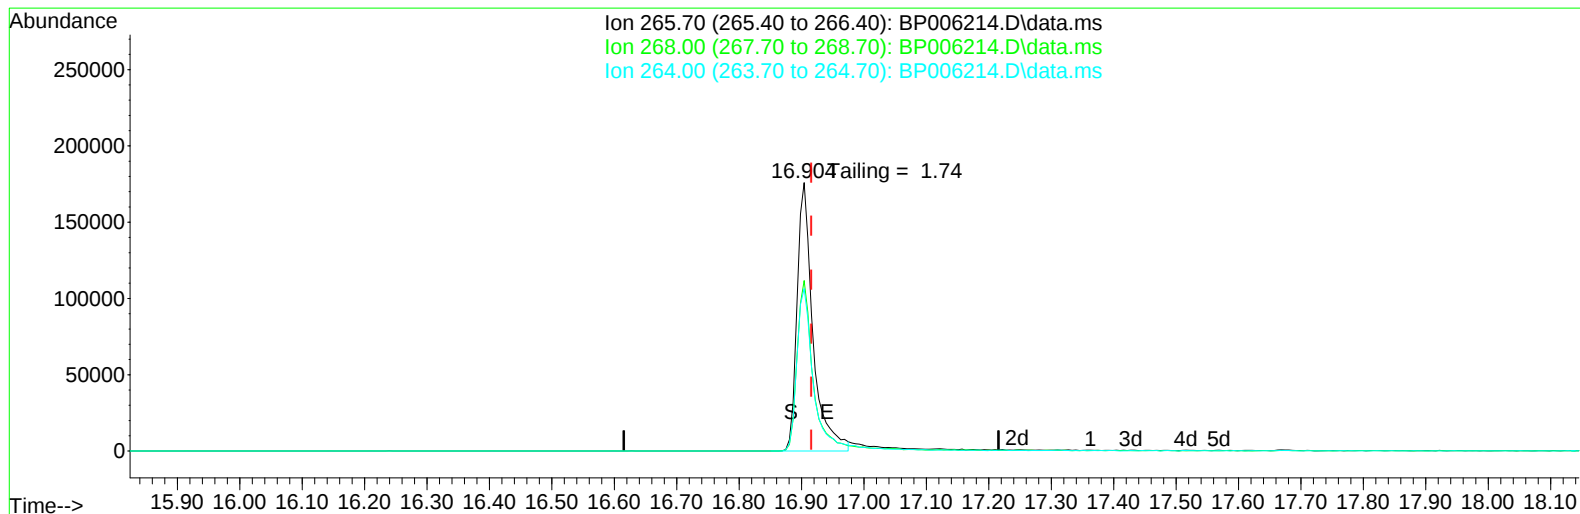

TIC: BP006214.D\data.ms

(70) Pentachlorophenol (C)

16.904min (-0.011) 36105.73 ng m

response 333437

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.51
264.00	62.90	60.53
0.00	0.00	0.00