

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071421\
 Data File : BP006226.D
 Acq On : 14 Jul 2021 19:35
 Operator : CG/JU
 Sample : M3015-01RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 RED-FRAC-TANKRE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006226.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.622	254	261	278	rBV7	26155	154154	2.32%	0.495%
2	4.964	315	319	326	rBV	60210	92306	1.39%	0.296%
3	5.440	393	400	419	rBV	222303	469003	7.07%	1.505%
4	7.058	668	675	688	rBV2	126939	298753	4.51%	0.959%
5	7.852	800	810	819	rBV	592945	1012025	15.26%	3.248%
6	8.116	849	855	878	rBV	250620	669250	10.09%	2.148%
7	8.952	990	997	1002	rBV	44701	69681	1.05%	0.224%
8	9.022	1002	1009	1027	rBV	1173261	2228757	33.61%	7.153%
9	10.440	1242	1250	1275	rBV	634688	1666500	25.13%	5.349%
10	10.651	1279	1286	1290	rVV	780707	1329928	20.06%	4.268%
11	10.704	1290	1295	1303	rVB	649093	1173906	17.70%	3.768%
12	13.110	1697	1704	1720	rBV	3037434	4580988	69.08%	14.703%
13	14.487	1931	1938	1946	rBV	954730	1463718	22.07%	4.698%
14	15.987	2187	2193	2208	rBV	708496	1285742	19.39%	4.127%
15	17.239	2400	2406	2412	rBV	987107	1533236	23.12%	4.921%
16	17.898	2514	2518	2523	rVB	108664	127432	1.92%	0.409%
17	18.122	2551	2556	2564	rBV	454093	680188	10.26%	2.183%
18	19.233	2739	2745	2751	rBV10	35410	95463	1.44%	0.306%
19	19.345	2761	2764	2773	rBV	207628	340214	5.13%	1.092%
20	19.616	2806	2810	2817	rVV	244078	356751	5.38%	1.145%
21	19.675	2817	2820	2824	rVB	71625	88103	1.33%	0.283%
22	19.786	2834	2839	2846	rBV	5522524	6631022	100.00%	21.283%
23	20.216	2909	2912	2916	rVB	77801	82098	1.24%	0.263%
24	21.016	3044	3048	3056	rBV2	358583	571574	8.62%	1.835%
25	21.316	3094	3099	3110	rBV	1396672	1838380	27.72%	5.900%
26	22.521	3301	3304	3311	rVB	189450	261298	3.94%	0.839%
27	23.692	3497	3503	3515	rVB2	957539	2056449	31.01%	6.600%




Sum of corrected areas: 31156919

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071421\
Data File : BP006226.D
Acq On : 14 Jul 2021 19:35
Operator : CG/JU
Sample : M3015-01RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RED-FRAC-TANKRE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

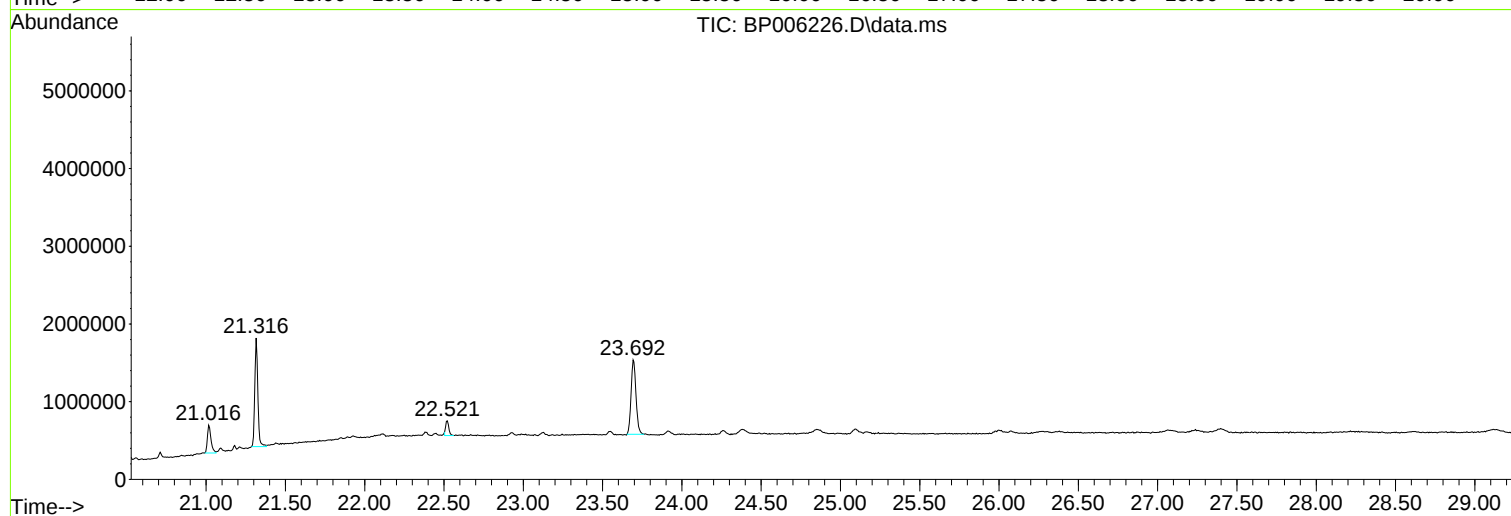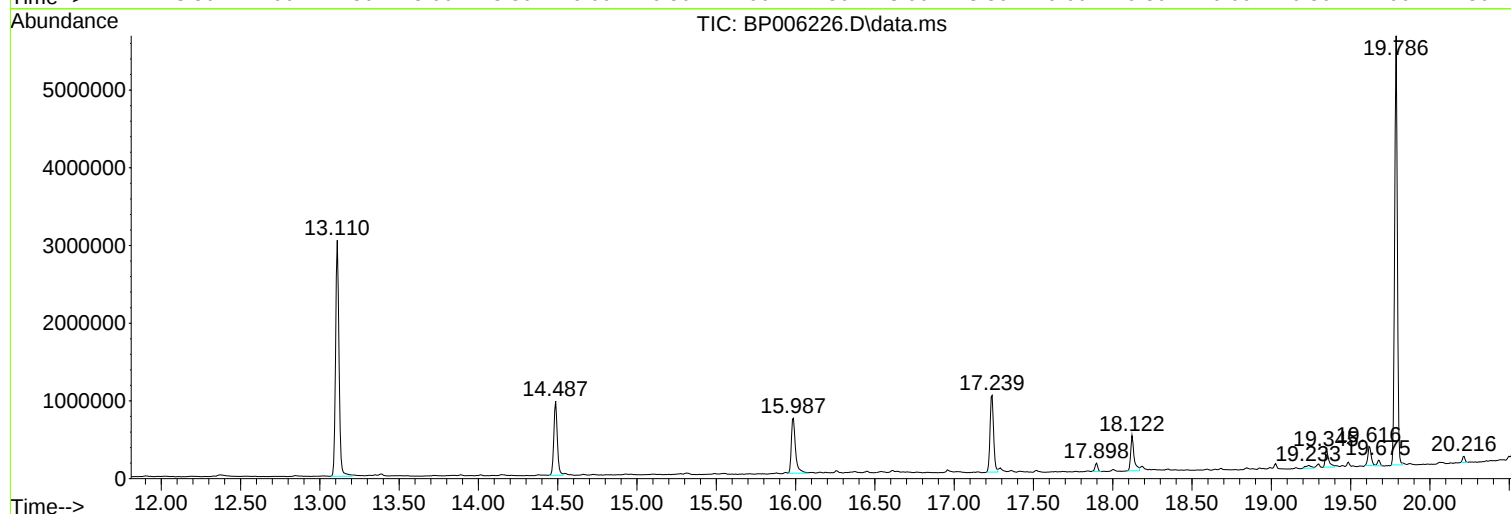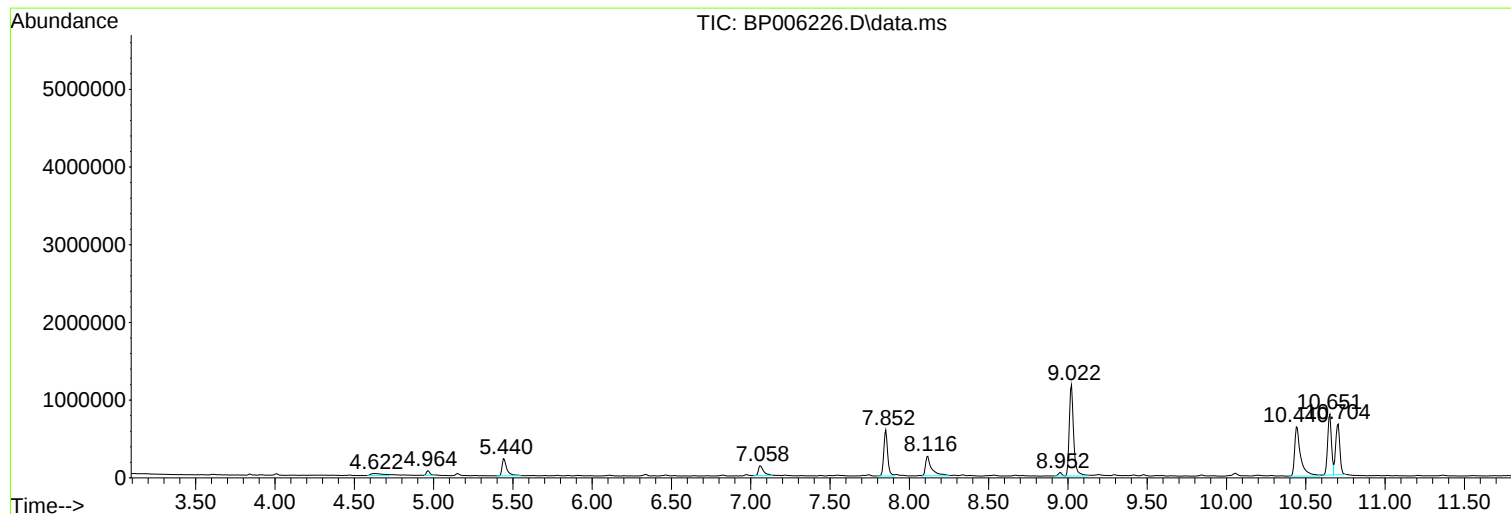

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071421\
Data File : BP006226.D
Acq On : 14 Jul 2021 19:35
Operator : CG/JU
Sample : M3015-01RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RED-FRAC-TANKRE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071421\
Data File : BP006226.D
Acq On : 14 Jul 2021 19:35
Operator : CG/JU
Sample : M3015-01RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
RED-FRAC-TANKRE

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------