
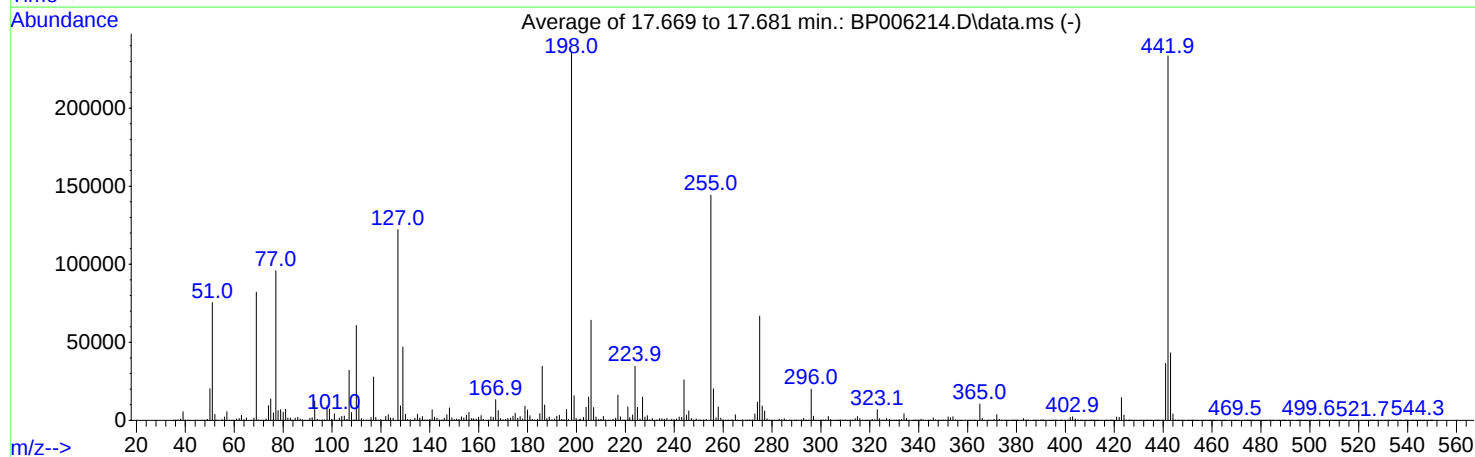


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071421\
 Data File : BP006214.D
 Acq On : 14 Jul 2021 12:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 15 13:37:02 2021

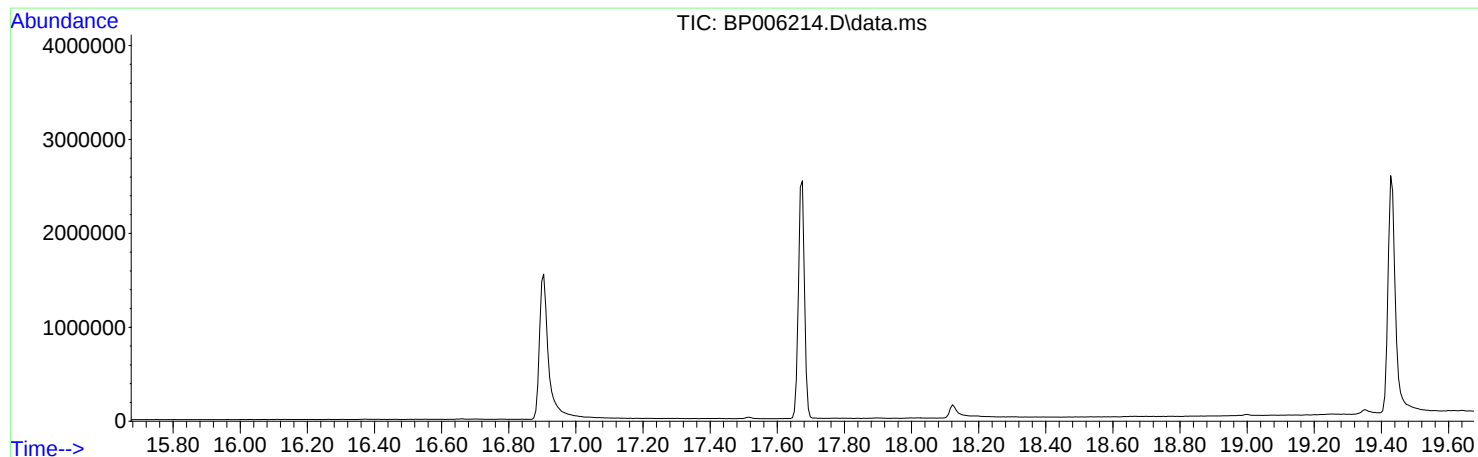




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.0	75469	PASS
68	69	0.00	2	1.8	1515	PASS
69	198	0.00	100	34.9	82133	PASS
70	69	0.00	2	0.4	313	PASS
127	198	10	80	51.8	122159	PASS
197	198	0.00	2	0.2	472	PASS
198	198	100	100	100.0	235669	PASS
199	198	5	9	6.7	15784	PASS
275	198	10	60	28.3	66799	PASS
365	198	1	100	4.4	10469	PASS
441	198	0.01	100	15.5	36531	PASS
442	442	100	100	100.0	233527	PASS
443	442	15	24	18.5	43299	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071421\
 Data File : BP006214.D
 Acq On : 14 Jul 2021 12:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 14 13:59:18 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 14:59:51 2021
 Response via : Initial Calibration

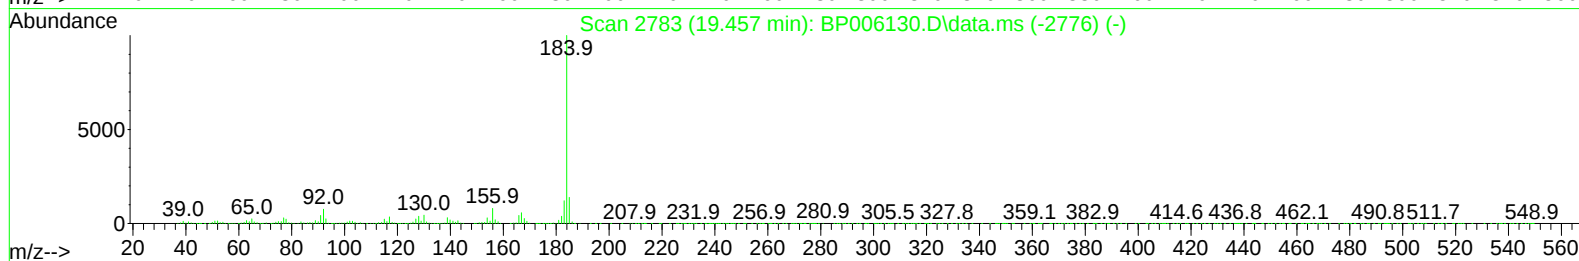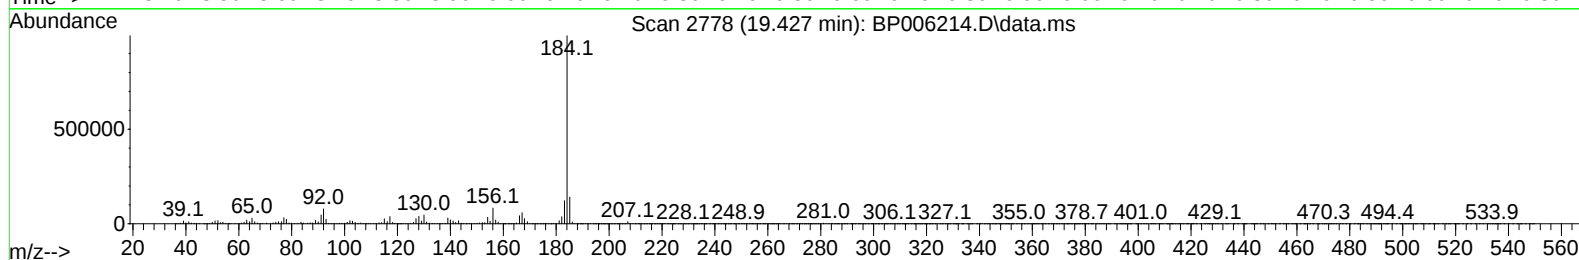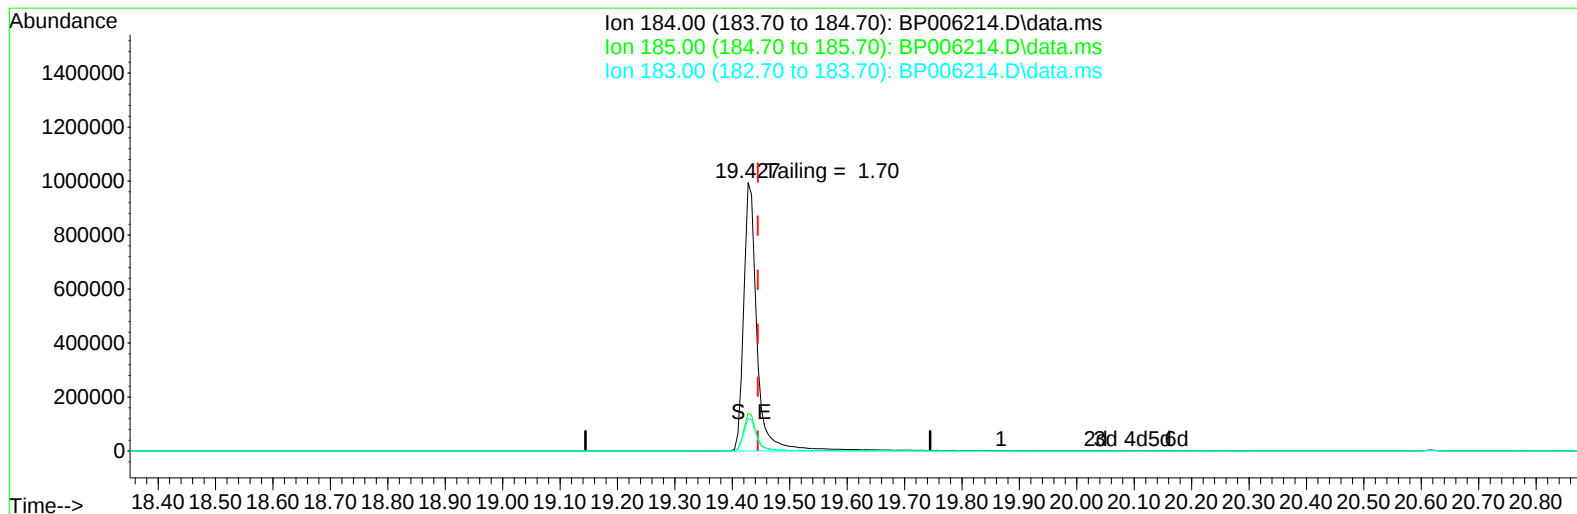

TIC: BP006214.D\data.ms

(77) Benzidine

19.427min (-0.017) 367945.30 ng m




response 1549292

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.16
183.00	11.90	12.26
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071421\
Data File : BP006214.D
Acq On : 14 Jul 2021 12:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 14 13:59:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 12 14:59:51 2021
Response via : Initial Calibration

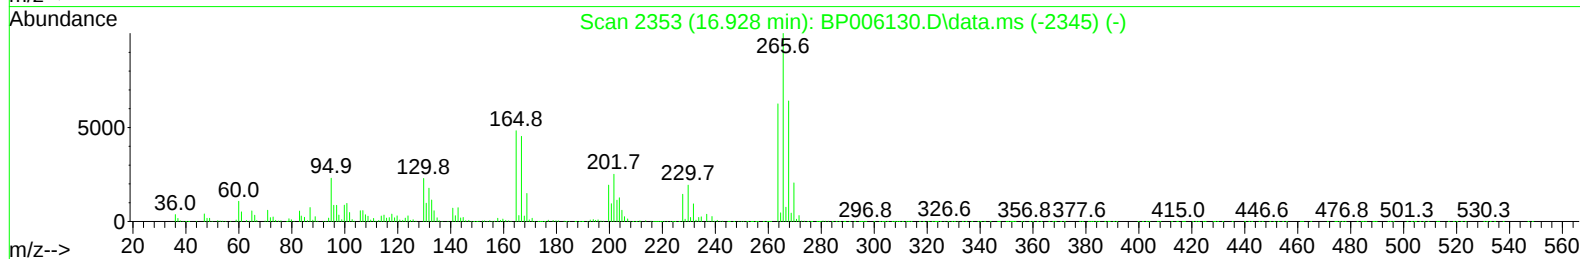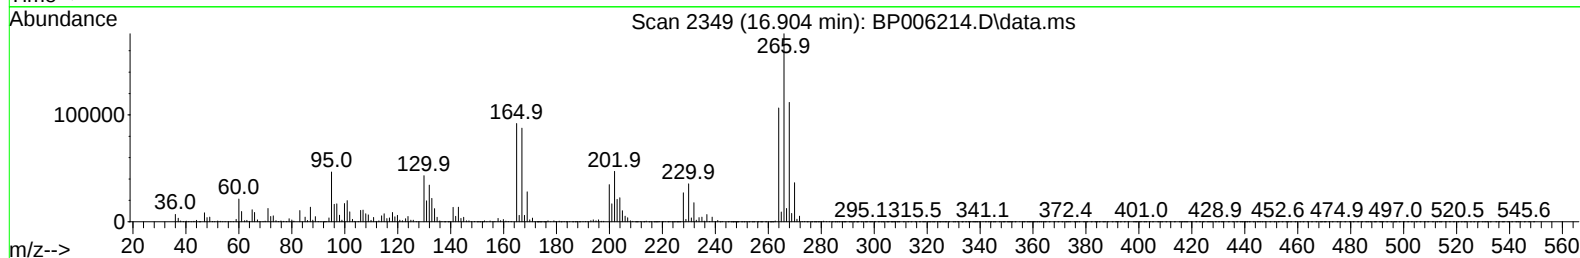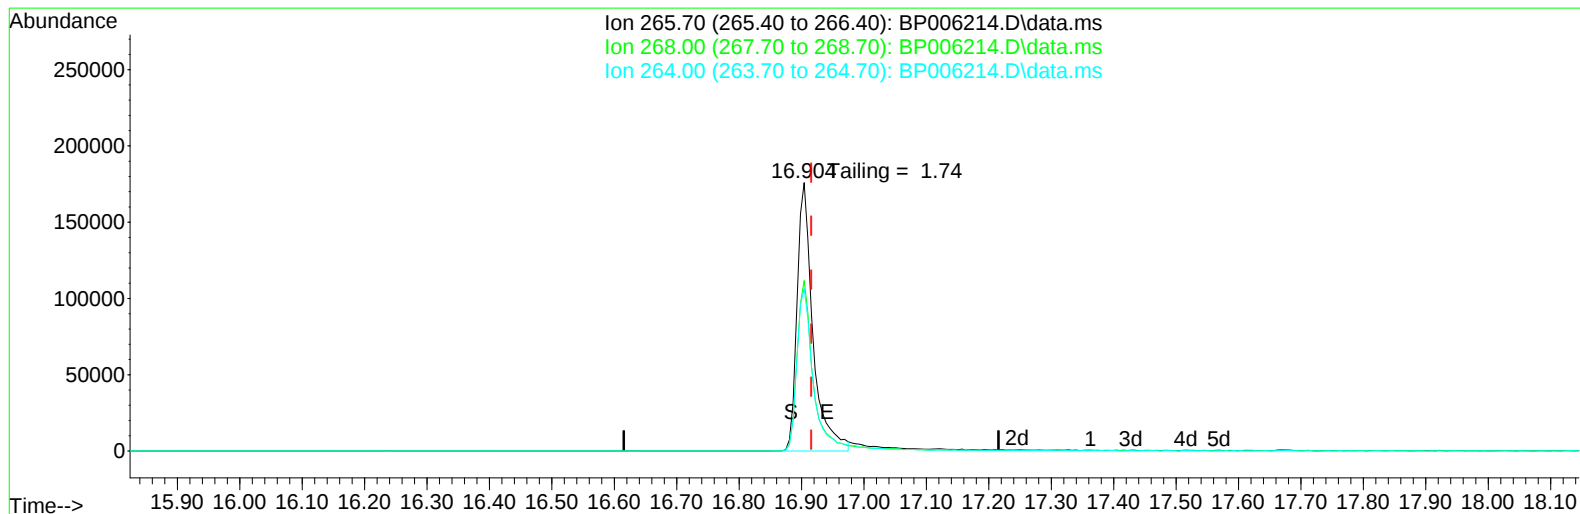

TIC: BP006214.D\data.ms

(70) Pentachlorophenol (C)

16.904min (-0.011) 36105.73 ng m

response 333437

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.51
264.00	62.90	60.53
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/14/2021	BNA_P	BP006214.D
Compound Name	Response	Retention Time
DDT	795424	20.61
DDD	6119	20.19
DDE	2706	19.69
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8825	804249	1.10