
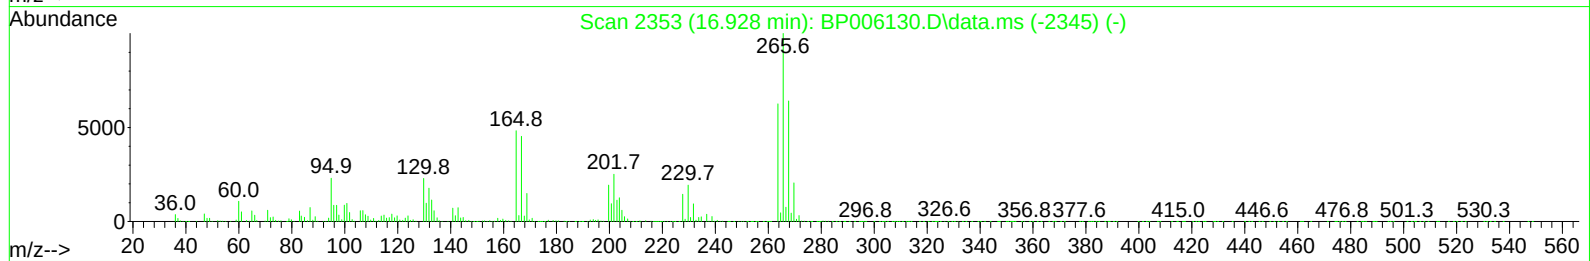
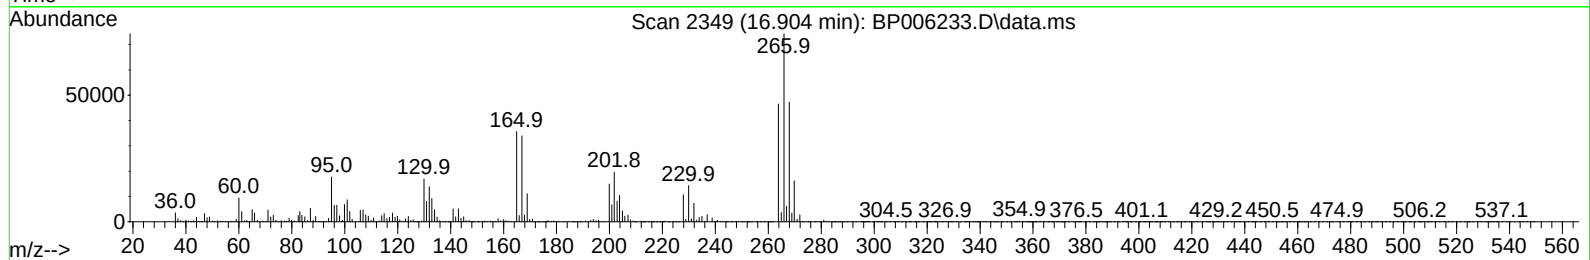


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071521\
Data File : BP006233.D
Acq On : 15 Jul 2021 11:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 13:31:32 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 12 14:59:51 2021
Response via : Initial Calibration

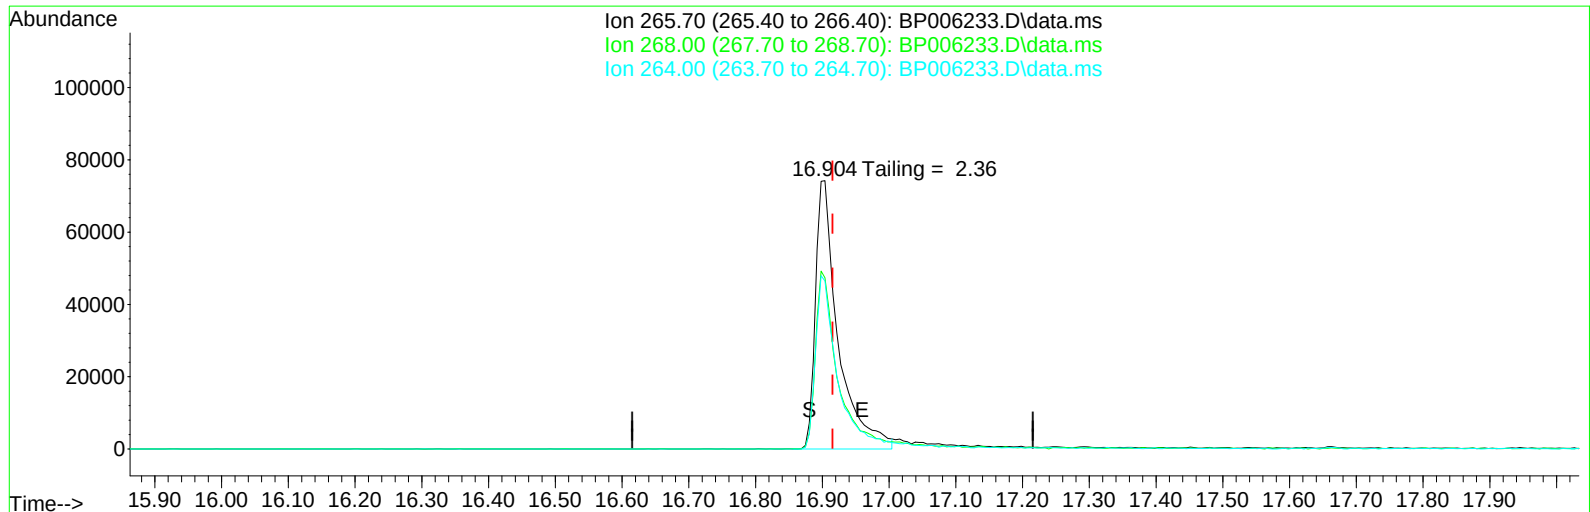

TIC: BP006233.D\data.ms

(70) Pentachlorophenol (C)




16.904min (-0.011) 636767.51 ng

response 178824

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.78
264.00	62.90	62.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071521\
 Data File : BP006233.D
 Acq On : 15 Jul 2021 11:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 13:31:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 14:59:51 2021
 Response via : Initial Calibration

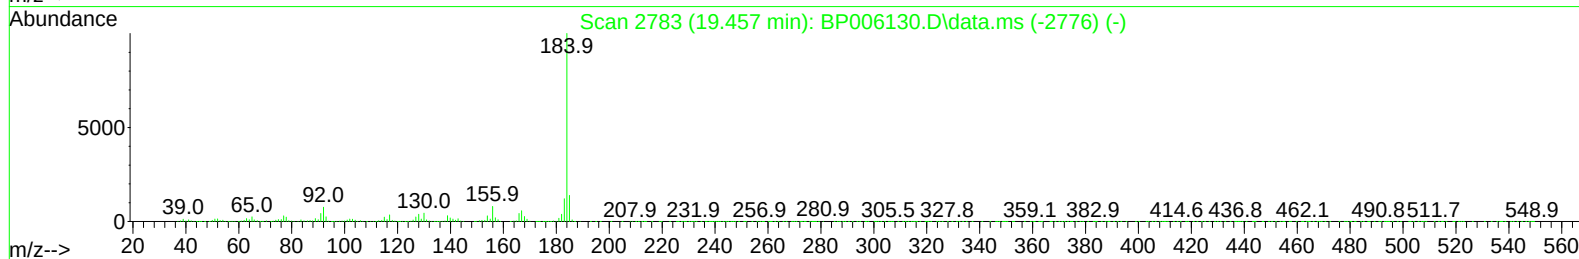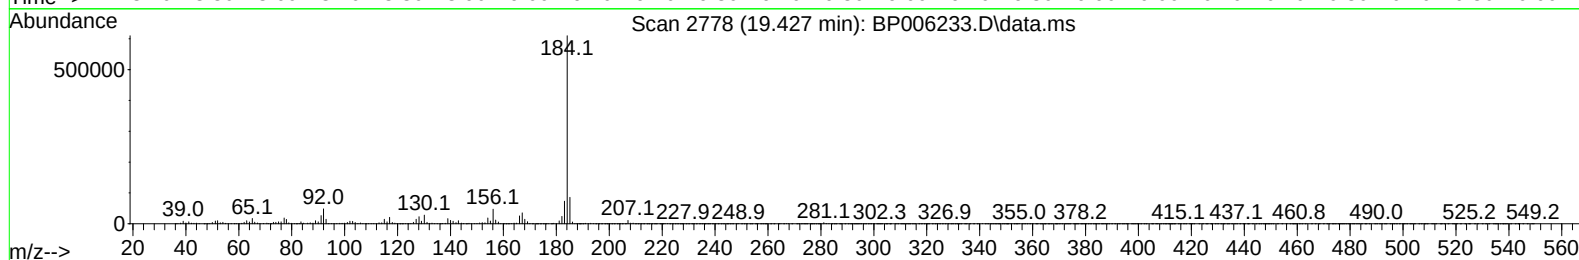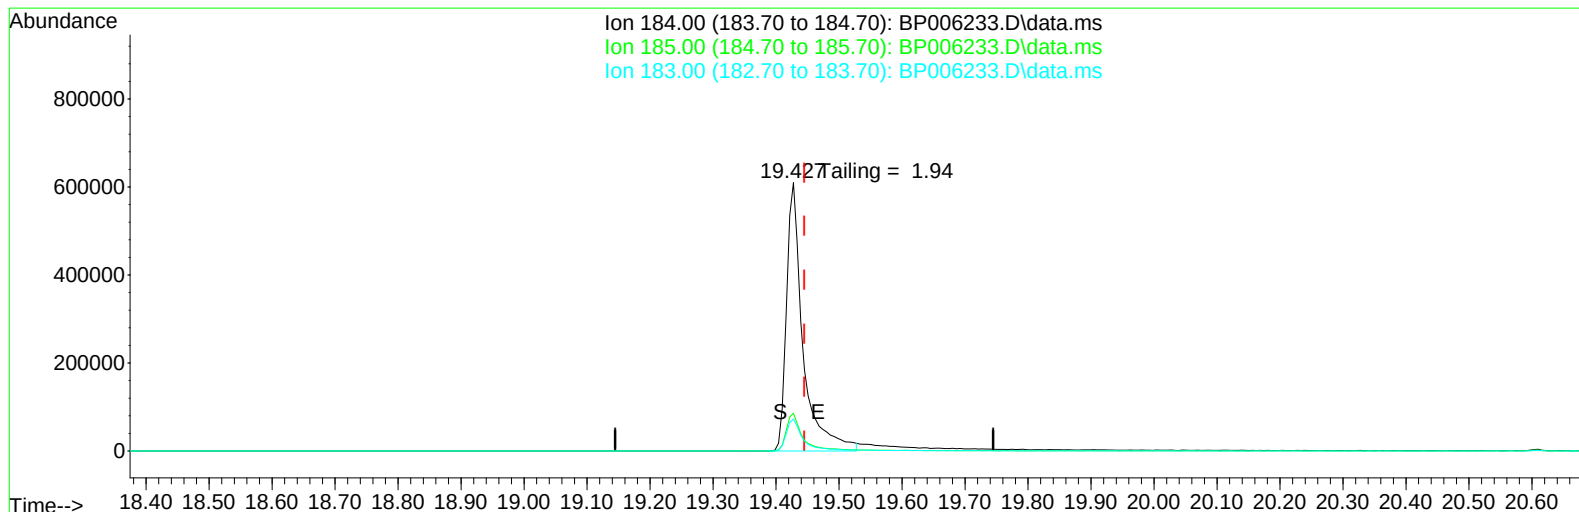

TIC: BP006233.D\data.ms

(77) Benzidine

19.427min (-0.017) 283980.76 ng

response 1195746

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.08
183.00	11.90	11.97
0.00	0.00	0.00