

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071521\
 Data File : BP006243.D
 Acq On : 15 Jul 2021 17:46
 Operator : CG/JU
 Sample : M3038-10
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SB-10-COMP

Quant Time: Jul 16 03:20:19 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 15 13:37:02 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	147001	20.000	ng	0.00
21) Naphthalene-d8	10.646	136	593285	20.000	ng	0.00
39) Acenaphthene-d10	14.481	164	319740	20.000	ng	0.00
64) Phenanthrene-d10	17.234	188	627631	20.000	ng	# 0.00
76) Chrysene-d12	21.310	240	628461	20.000	ng	# 0.00
86) Perylene-d12	23.686	264	734834	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.423	112	883867	103.456	ng	0.00
7) Phenol-d6	7.034	99	1075123	95.139	ng	0.00
23) Nitrobenzene-d5	9.016	82	606779	64.602	ng	0.00
42) 2,4,6-Tribromophenol	15.975	330	369433	97.048	ng	0.00
45) 2-Fluorobiphenyl	13.104	172	1354845	62.642	ng	0.00
79) Terphenyl-d14	19.781	244	2007394	62.976	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071521\
Data File : BP006243.D
Acq On : 15 Jul 2021 17:46
Operator : CG/JU
Sample : M3038-10
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SB-10-COMP

Quant Time: Jul 16 03:20:19 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 15 13:37:02 2021
Response via : Initial Calibration




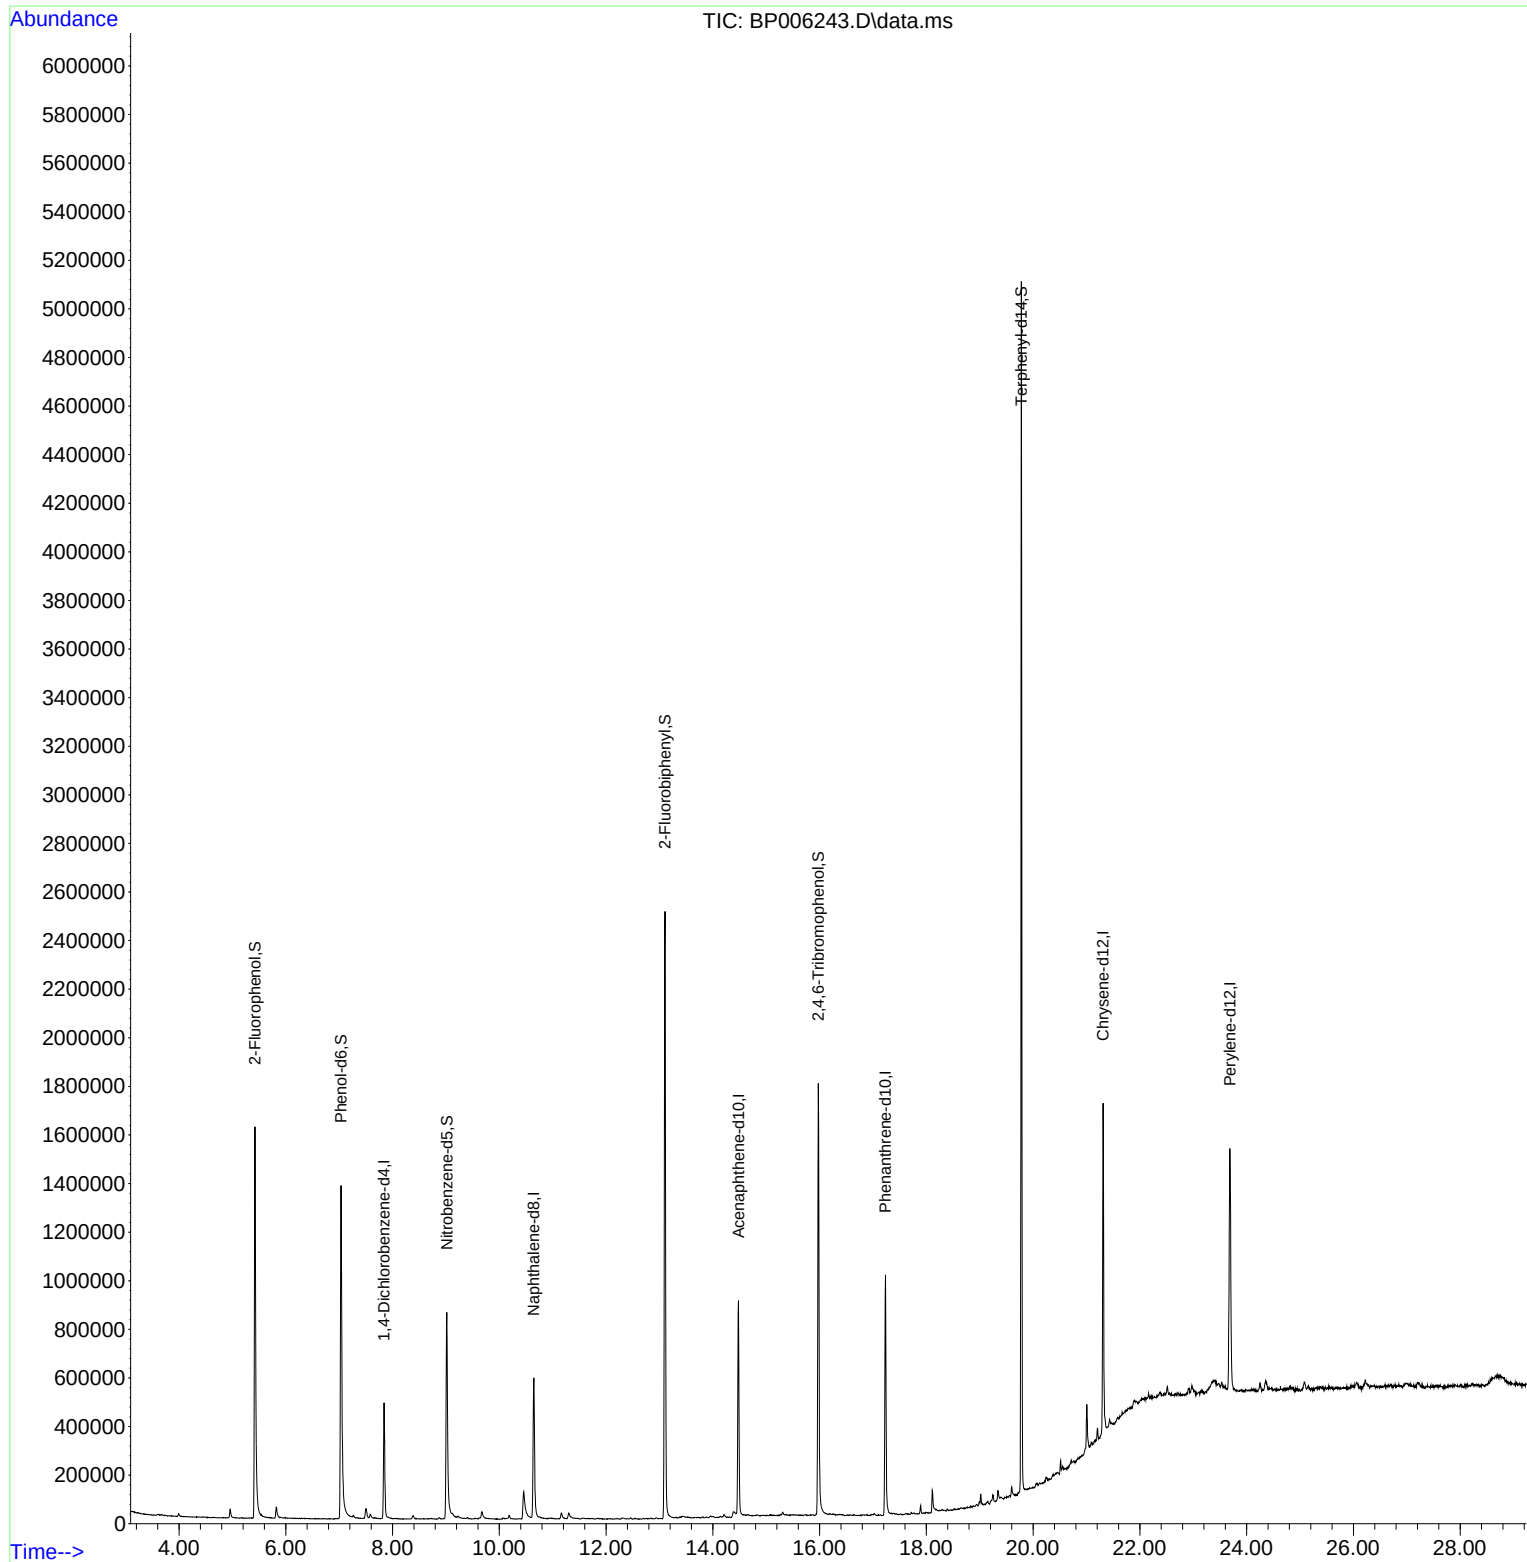


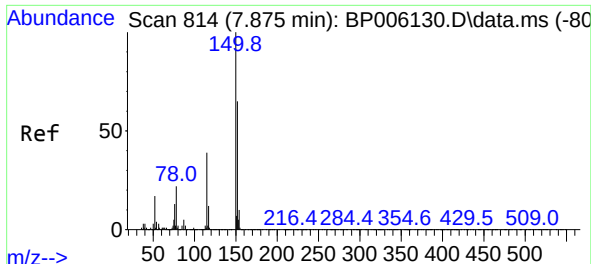

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.840 min Scan# 808
Delta R.T. 0.000 min
Lab File: BP006243.D
Acq: 15 Jul 2021 17:46




Instrument :
BNA_P
ClientSampleId :
SB-10-COMP


Tgt Ion:152 Resp: 147001
Ion Ratio Lower Upper
152 100
150 158.8 125.6 188.4
115 60.6 48.5 72.7

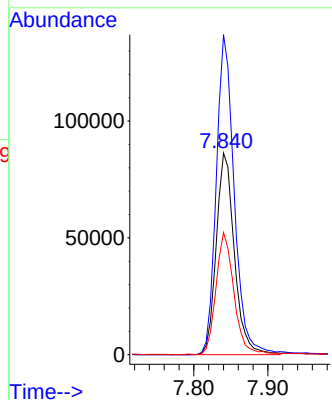

#5
2-Fluorophenol
Concen: 103.456 ng
RT: 5.423 min Scan# 397
Delta R.T. 0.000 min
Lab File: BP006243.D
Acq: 15 Jul 2021 17:46

Tgt Ion:112 Resp: 883867
Ion Ratio Lower Upper
112 100
64 50.3 41.4 62.2
63 25.5 23.8 35.8

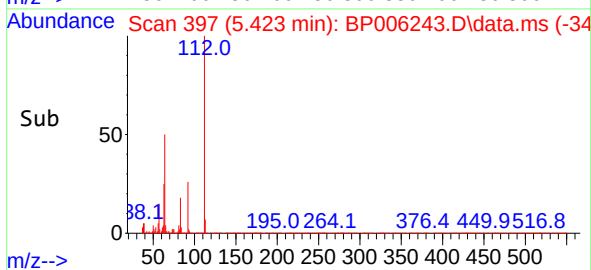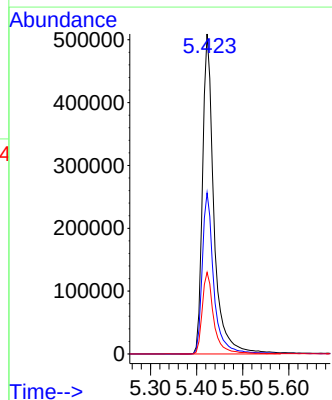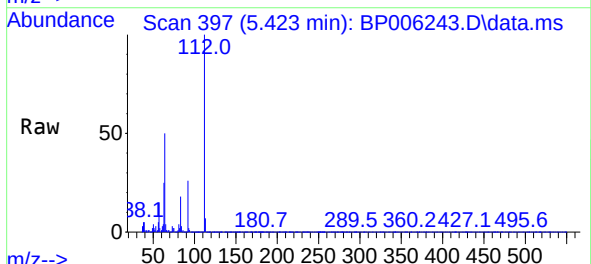




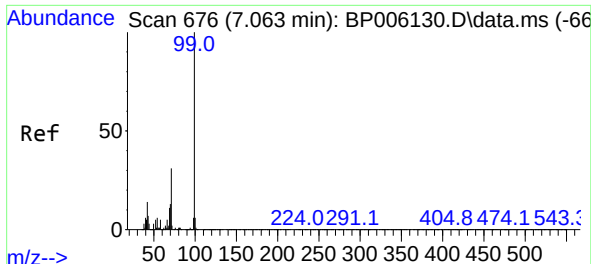


#7
Phenol-d6
Concen: 95.139 ng
RT: 7.034 min Scan# 671
Delta R.T. 0.000 min
Lab File: BP006243.D
Acq: 15 Jul 2021 17:46

Instrument :
BNA_P
ClientSampleId :
SB-10-COMP

Tgt Ion: 99 Resp: 1075123




Ion	Ratio	Lower	Upper
99	100		
42	15.4	13.4	20.0
71	32.0	30.6	46.0

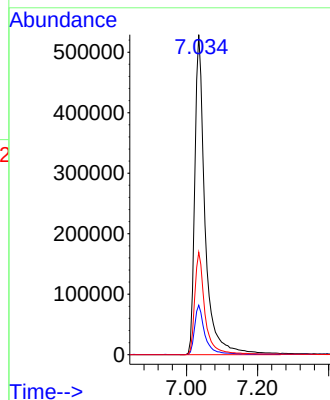


#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.646 min Scan# 1285
Delta R.T. 0.006 min
Lab File: BP006243.D
Acq: 15 Jul 2021 17:46

Tgt Ion: 136 Resp: 593285

Ion	Ratio	Lower	Upper
136	100		
137	10.8	8.6	12.8
54	6.7	4.6	6.8
68	5.3	3.6	5.4


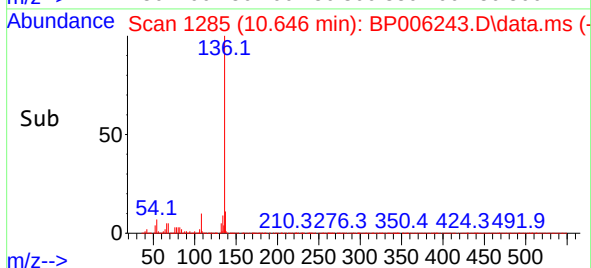
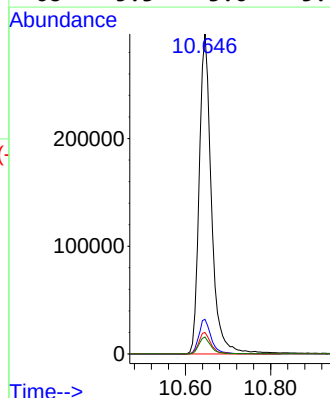
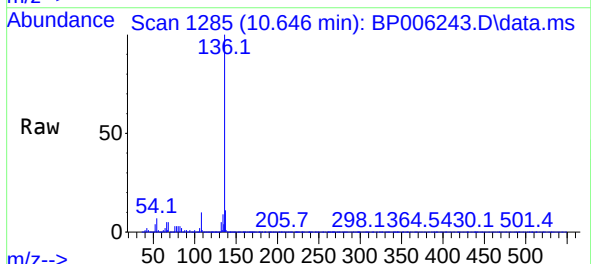


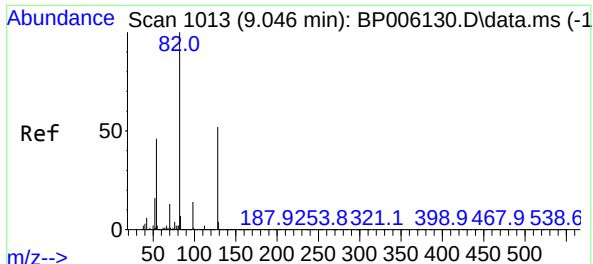

#23
Nitrobenzene-d5
Concen: 64.602 ng
RT: 9.016 min Scan# 1008
Delta R.T. 0.006 min
Lab File: BP006243.D
Acq: 15 Jul 2021 17:46




Instrument :
BNA_P
ClientSampleId :
SB-10-COMP


Tgt Ion: 82 Resp: 606779
Ion Ratio Lower Upper
82 100
128 49.9 35.7 53.5
54 45.2 35.0 52.4

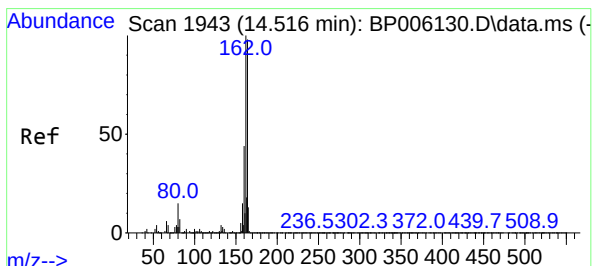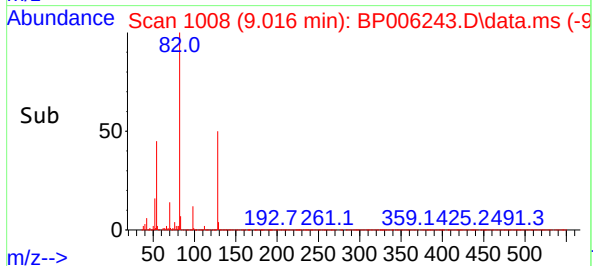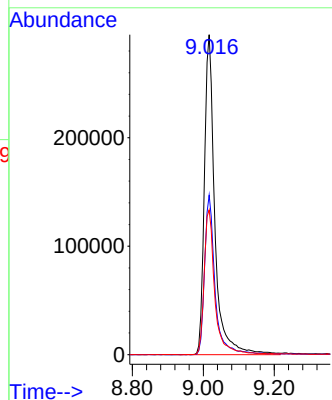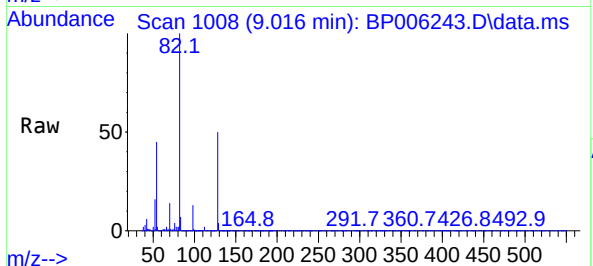

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.481 min Scan# 1937
Delta R.T. 0.000 min
Lab File: BP006243.D
Acq: 15 Jul 2021 17:46

Tgt Ion: 164 Resp: 319740
Ion Ratio Lower Upper
164 100
162 103.6 80.2 120.2
160 45.8 34.5 51.7


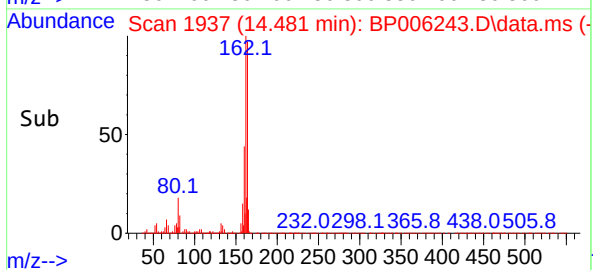
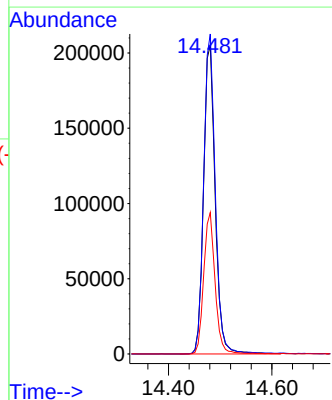
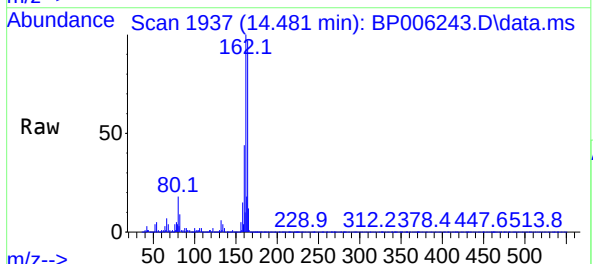




#42
2,4,6-Tribromophenol
Concen: 97.048 ng
RT: 15.975 min Scan# 2191
Delta R.T. 0.000 min
Lab File: BP006243.D
Acq: 15 Jul 2021 17:46




Instrument :
BNA_P
ClientSampleId :
SB-10-COMP


Tgt Ion:330 Resp: 369433
Ion Ratio Lower Upper
330 100
332 97.9 77.8 116.8
141 39.7 25.4 38.2#

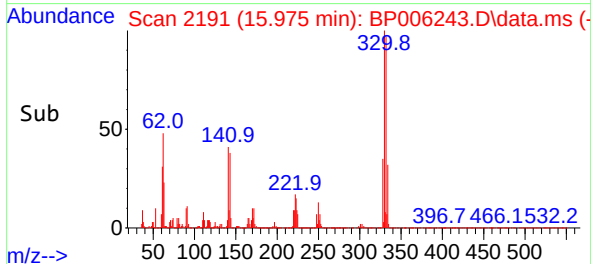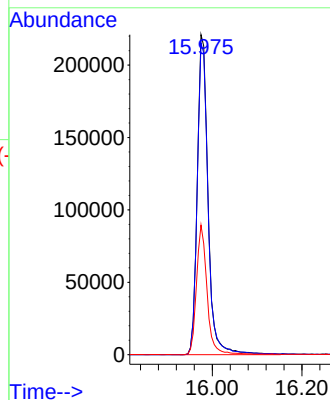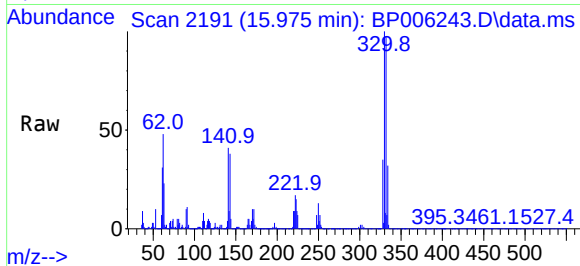

#45
2-Fluorobiphenyl
Concen: 62.642 ng
RT: 13.104 min Scan# 1703
Delta R.T. 0.000 min
Lab File: BP006243.D
Acq: 15 Jul 2021 17:46

Tgt Ion:172 Resp: 1354845
Ion Ratio Lower Upper
172 100
171 36.6 27.9 41.9
170 23.5 18.6 27.8


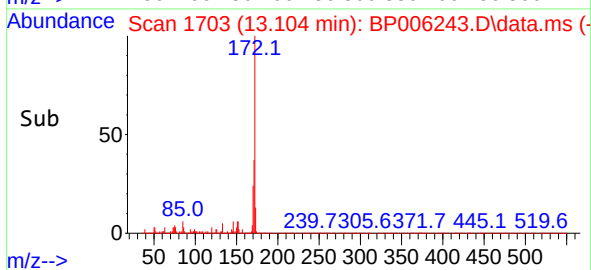
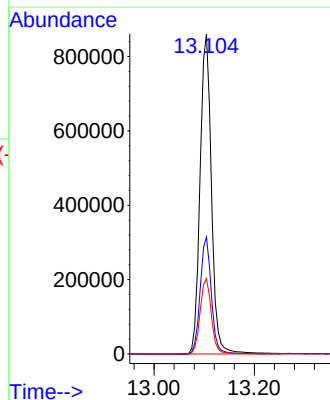
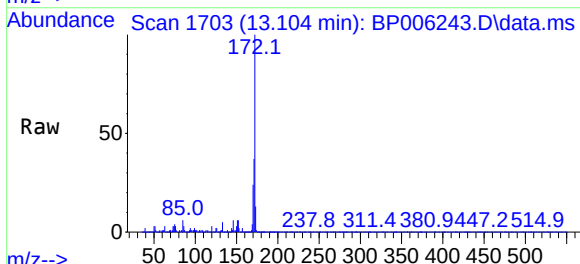


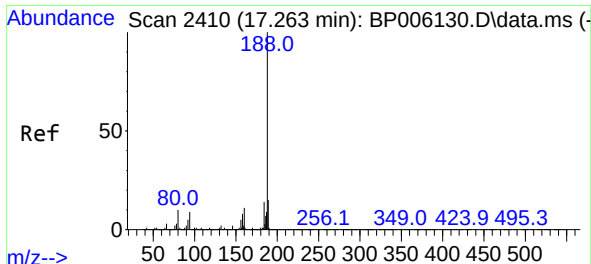

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.234 min Scan# 2405
Delta R.T. 0.006 min
Lab File: BP006243.D
Acq: 15 Jul 2021 17:46




Instrument :
BNA_P
ClientSampleId :
SB-10-COMP


Tgt Ion:188 Resp: 627631
Ion Ratio Lower Upper
188 100
94 9.1 5.6 8.4#
80 10.0 6.3 9.5#

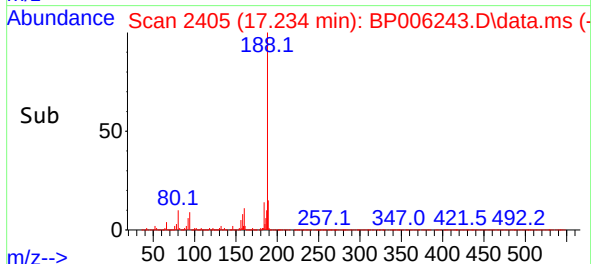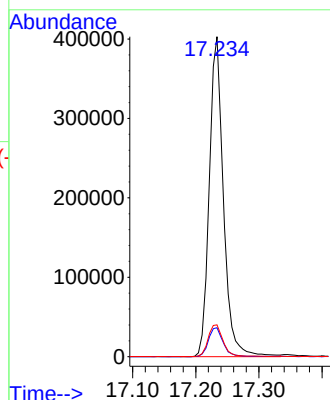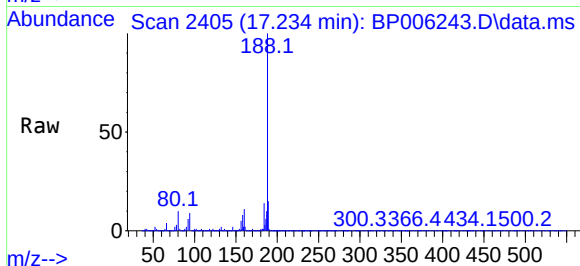

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.310 min Scan# 3098
Delta R.T. 0.000 min
Lab File: BP006243.D
Acq: 15 Jul 2021 17:46

Tgt Ion:240 Resp: 628461
Ion Ratio Lower Upper
240 100
120 13.8 6.5 9.7#
236 25.6 20.6 31.0


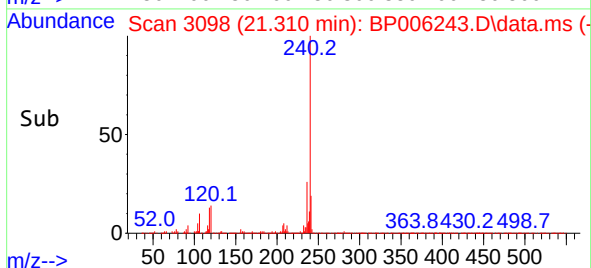
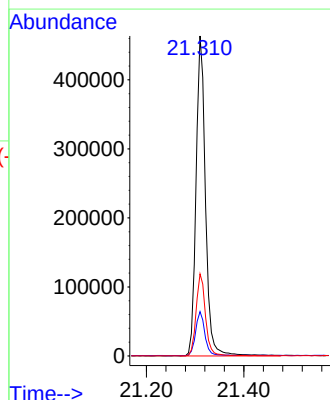
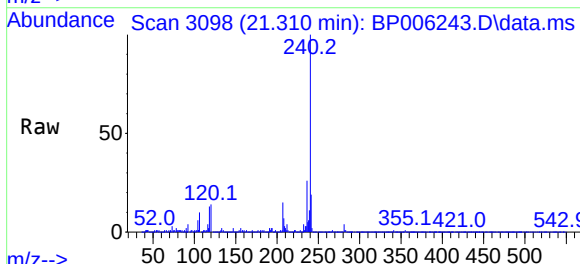




#79
Terphenyl-d14
Concen: 62.976 ng
RT: 19.781 min Scan# 2838
Delta R.T. 0.000 min
Lab File: BP006243.D
Acq: 15 Jul 2021 17:46

Instrument :
BNA_P
ClientSampleId :
SB-10-COMP

Tgt Ion:244 Resp: 2007394
Ion Ratio Lower Upper
244 100
212 7.6 6.0 9.0
122 13.1 7.1 10.7#

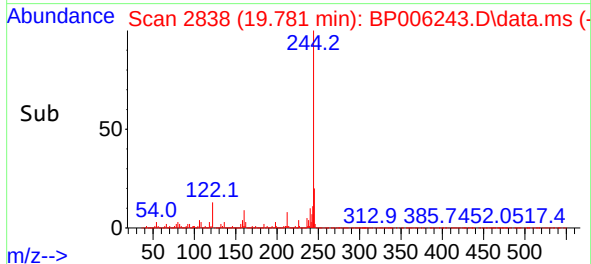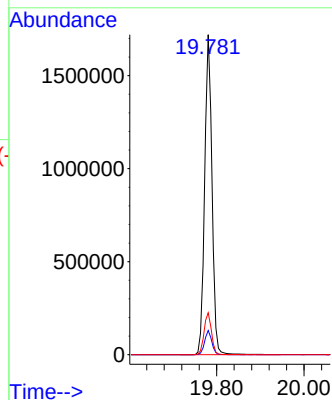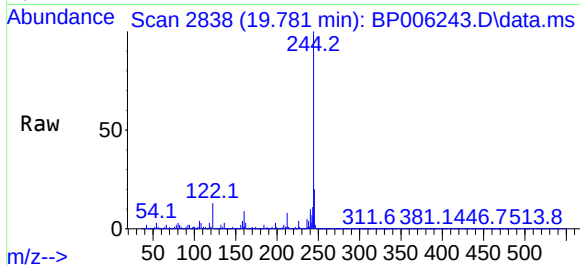

#86
Perylene-d12
Concen: 20.000 ng
RT: 23.686 min Scan# 3502
Delta R.T. -0.006 min
Lab File: BP006243.D
Acq: 15 Jul 2021 17:46

Tgt Ion:264 Resp: 734834
Ion Ratio Lower Upper
264 100
260 23.7 18.6 28.0
265 22.2 17.6 26.4

