
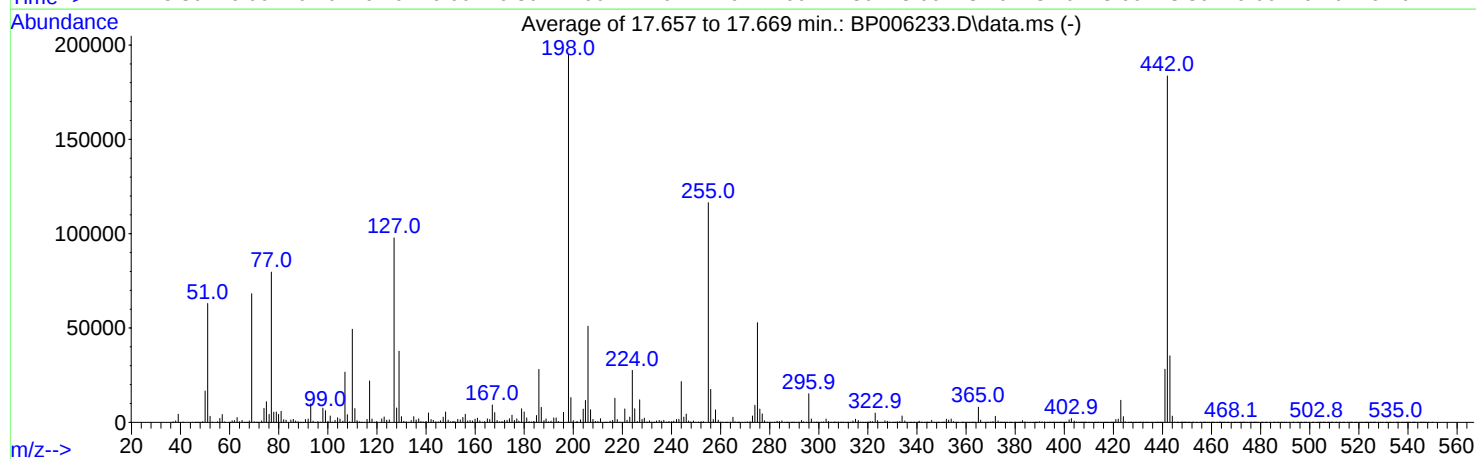


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071521\
 Data File : BP006233.D
 Acq On : 15 Jul 2021 11:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 15 13:37:02 2021

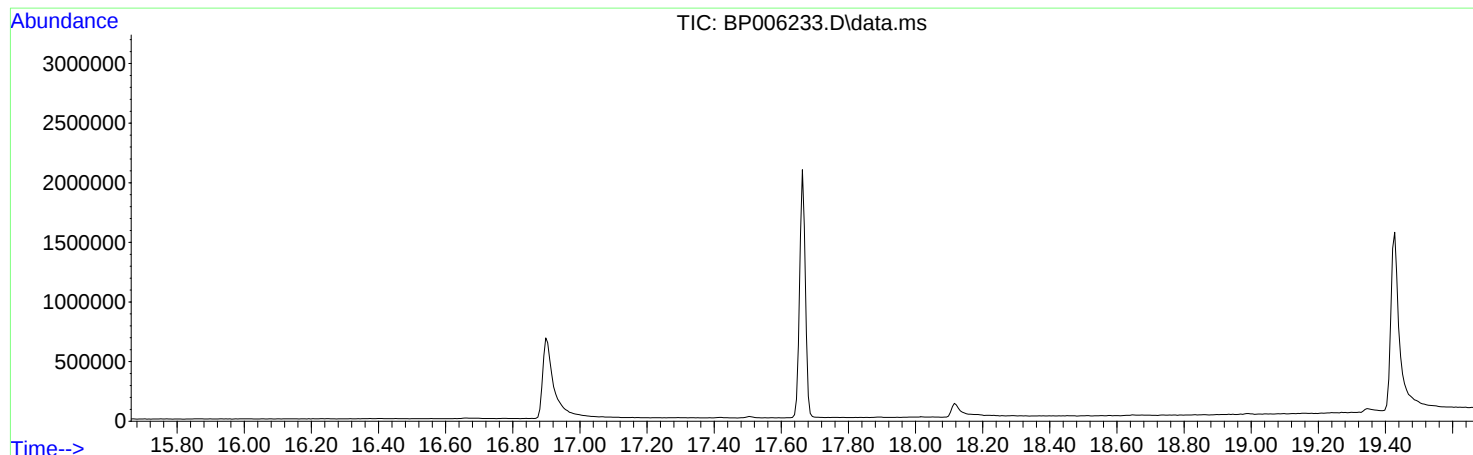


AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.3	63035	PASS
68	69	0.00	2	1.1	733	PASS
69	198	0.00	100	35.0	68195	PASS
70	69	0.00	2	0.5	374	PASS
127	198	10	80	50.2	97779	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	194968	PASS
199	198	5	9	6.7	13116	PASS
275	198	10	60	27.1	52815	PASS
365	198	1	100	4.1	8080	PASS
441	198	0.01	100	14.4	28133	PASS
442	442	100	100	100.0	183617	PASS
443	442	15	24	19.2	35243	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071521\
 Data File : BP006233.D
 Acq On : 15 Jul 2021 11:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 15 13:31:32 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 12 14:59:51 2021
 Response via : Initial Calibration

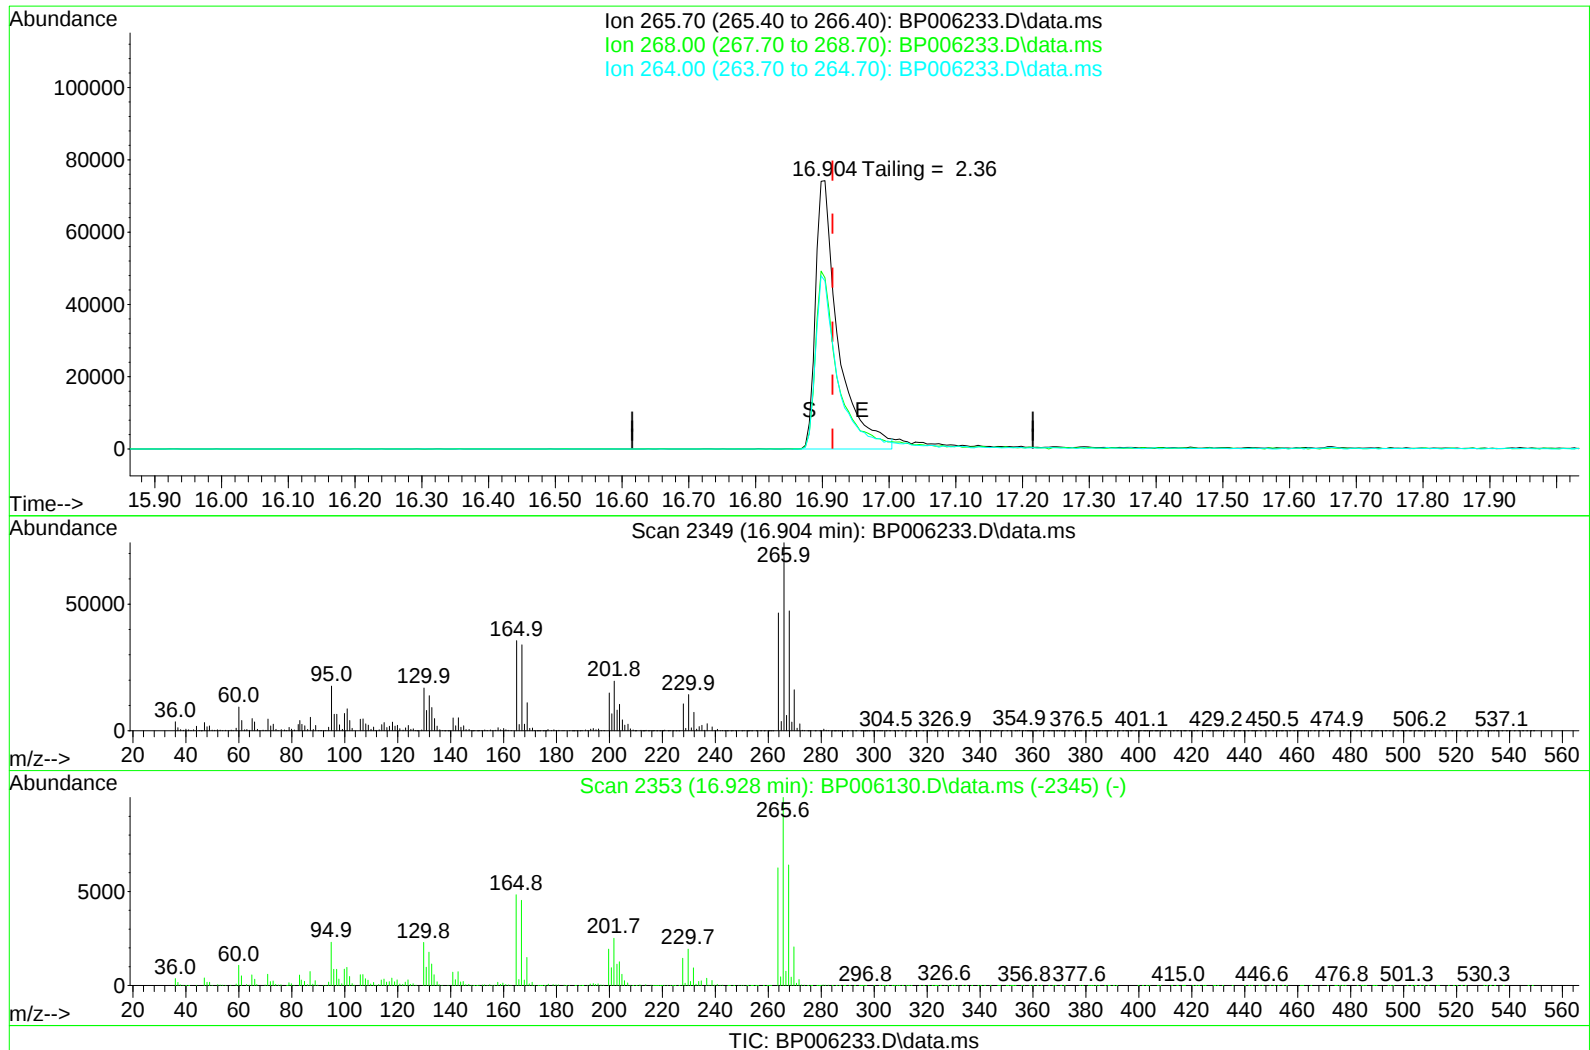

TIC: BP006233.D\data.ms

(70) Pentachlorophenol (C)

16.904min (-0.011) 636767.51 ng




response 178824

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.78
264.00	62.90	62.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071521\
Data File : BP006233.D
Acq On : 15 Jul 2021 11:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 15 13:31:32 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 12 14:59:51 2021
Response via : Initial Calibration

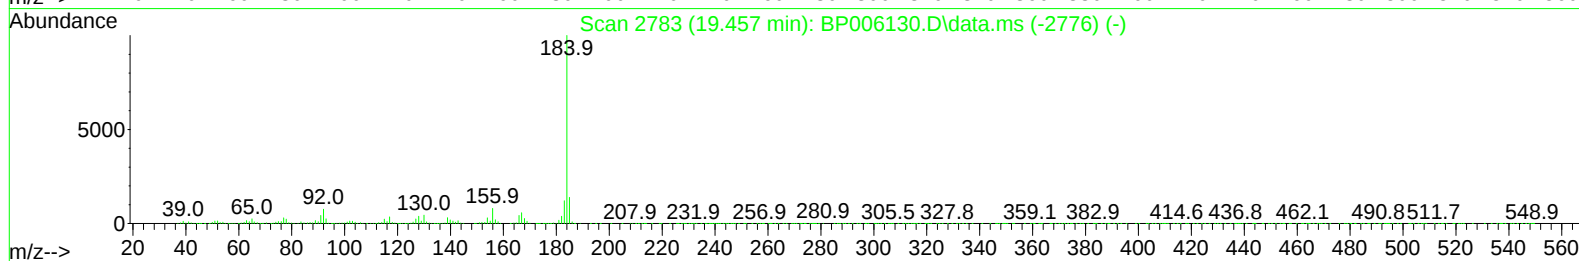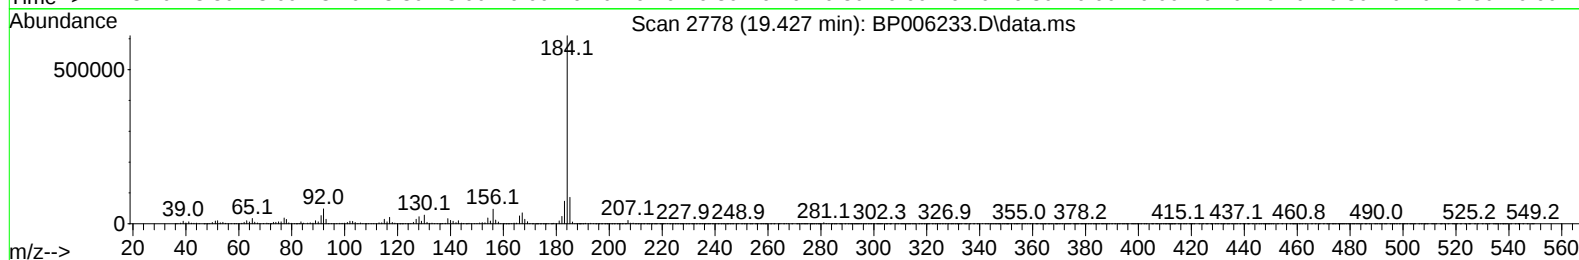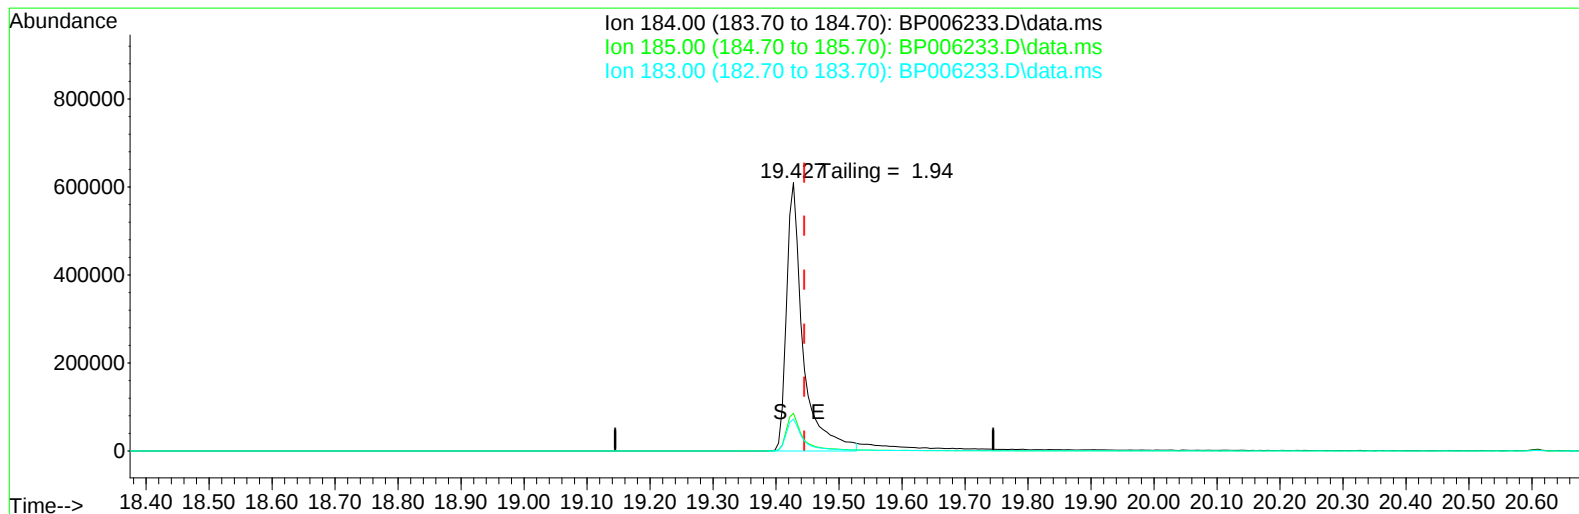

TIC: BP006233.D\data.ms

(77) Benzidine

19.427min (-0.017) 283980.76 ng

response 1195746

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.08
183.00	11.90	11.97
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/15/2021	BNA_P	BP006233.D
Compound Name	Response	Retention Time
DDT	640397	20.61
DDD	5863	20.18
DDE	3140	19.69
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9003	649400	1.39

Instrument :
BNA_P
ClientSampleId :
DFTPP