


4-Chloroaniline

Response Ratio

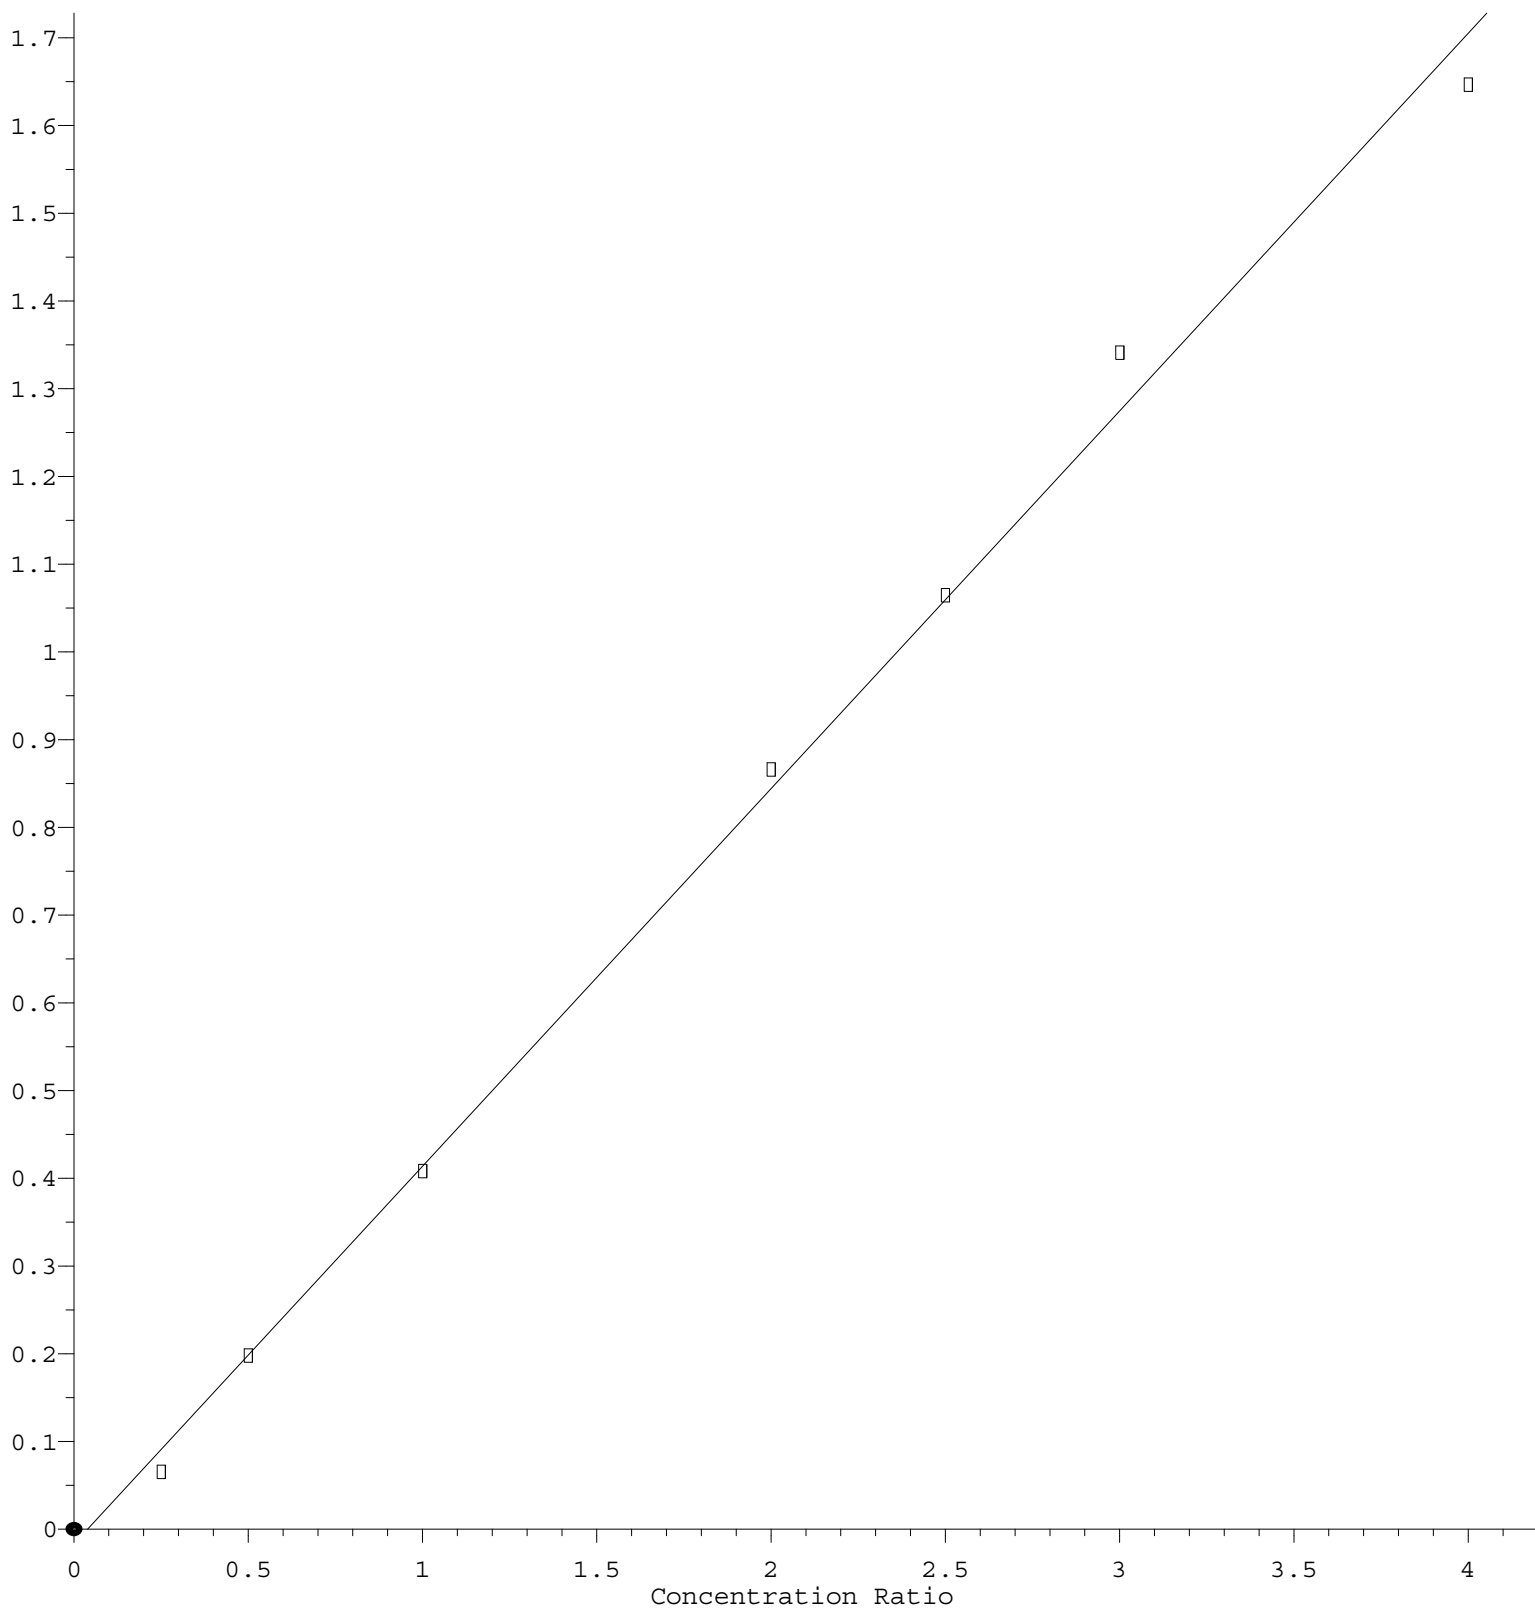

$$\text{Response} = 4.307\text{e-}001 * \text{Amt} - 1.688\text{e-}002$$


Coef of Det (r^2) = 0.995777 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP071522.M

Calibration Table Last Updated: Fri Jul 15 13:54:34 2022

3-Nitroaniline

Response Ratio

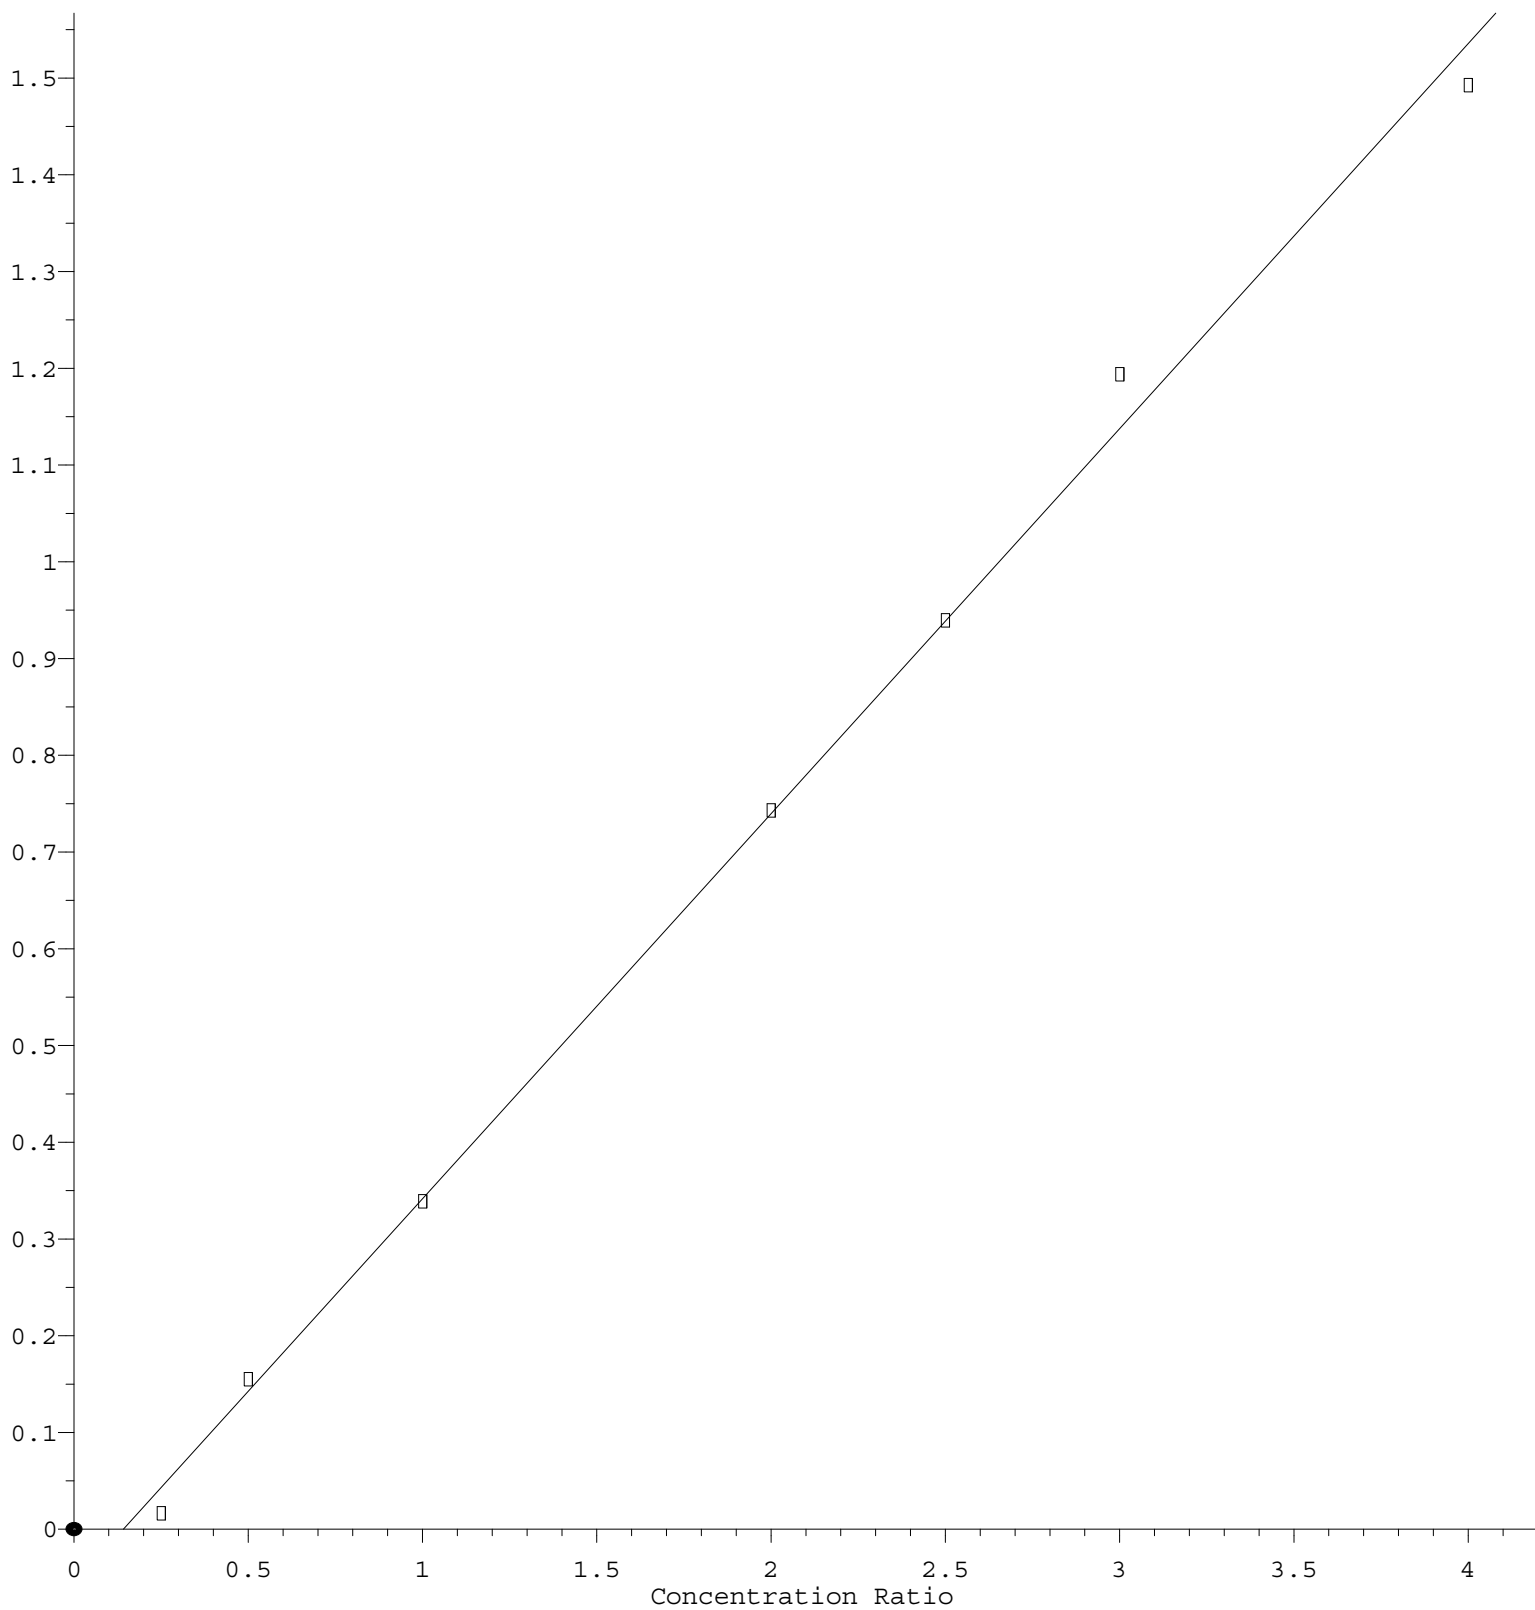

$$\text{Response} = 3.981\text{e-}001 * \text{Amt} - 5.660\text{e-}002$$


Coef of Det (r^2) = 0.996769 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP071522.M

Calibration Table Last Updated: Fri Jul 15 13:54:34 2022

4-Nitroaniline

Response Ratio

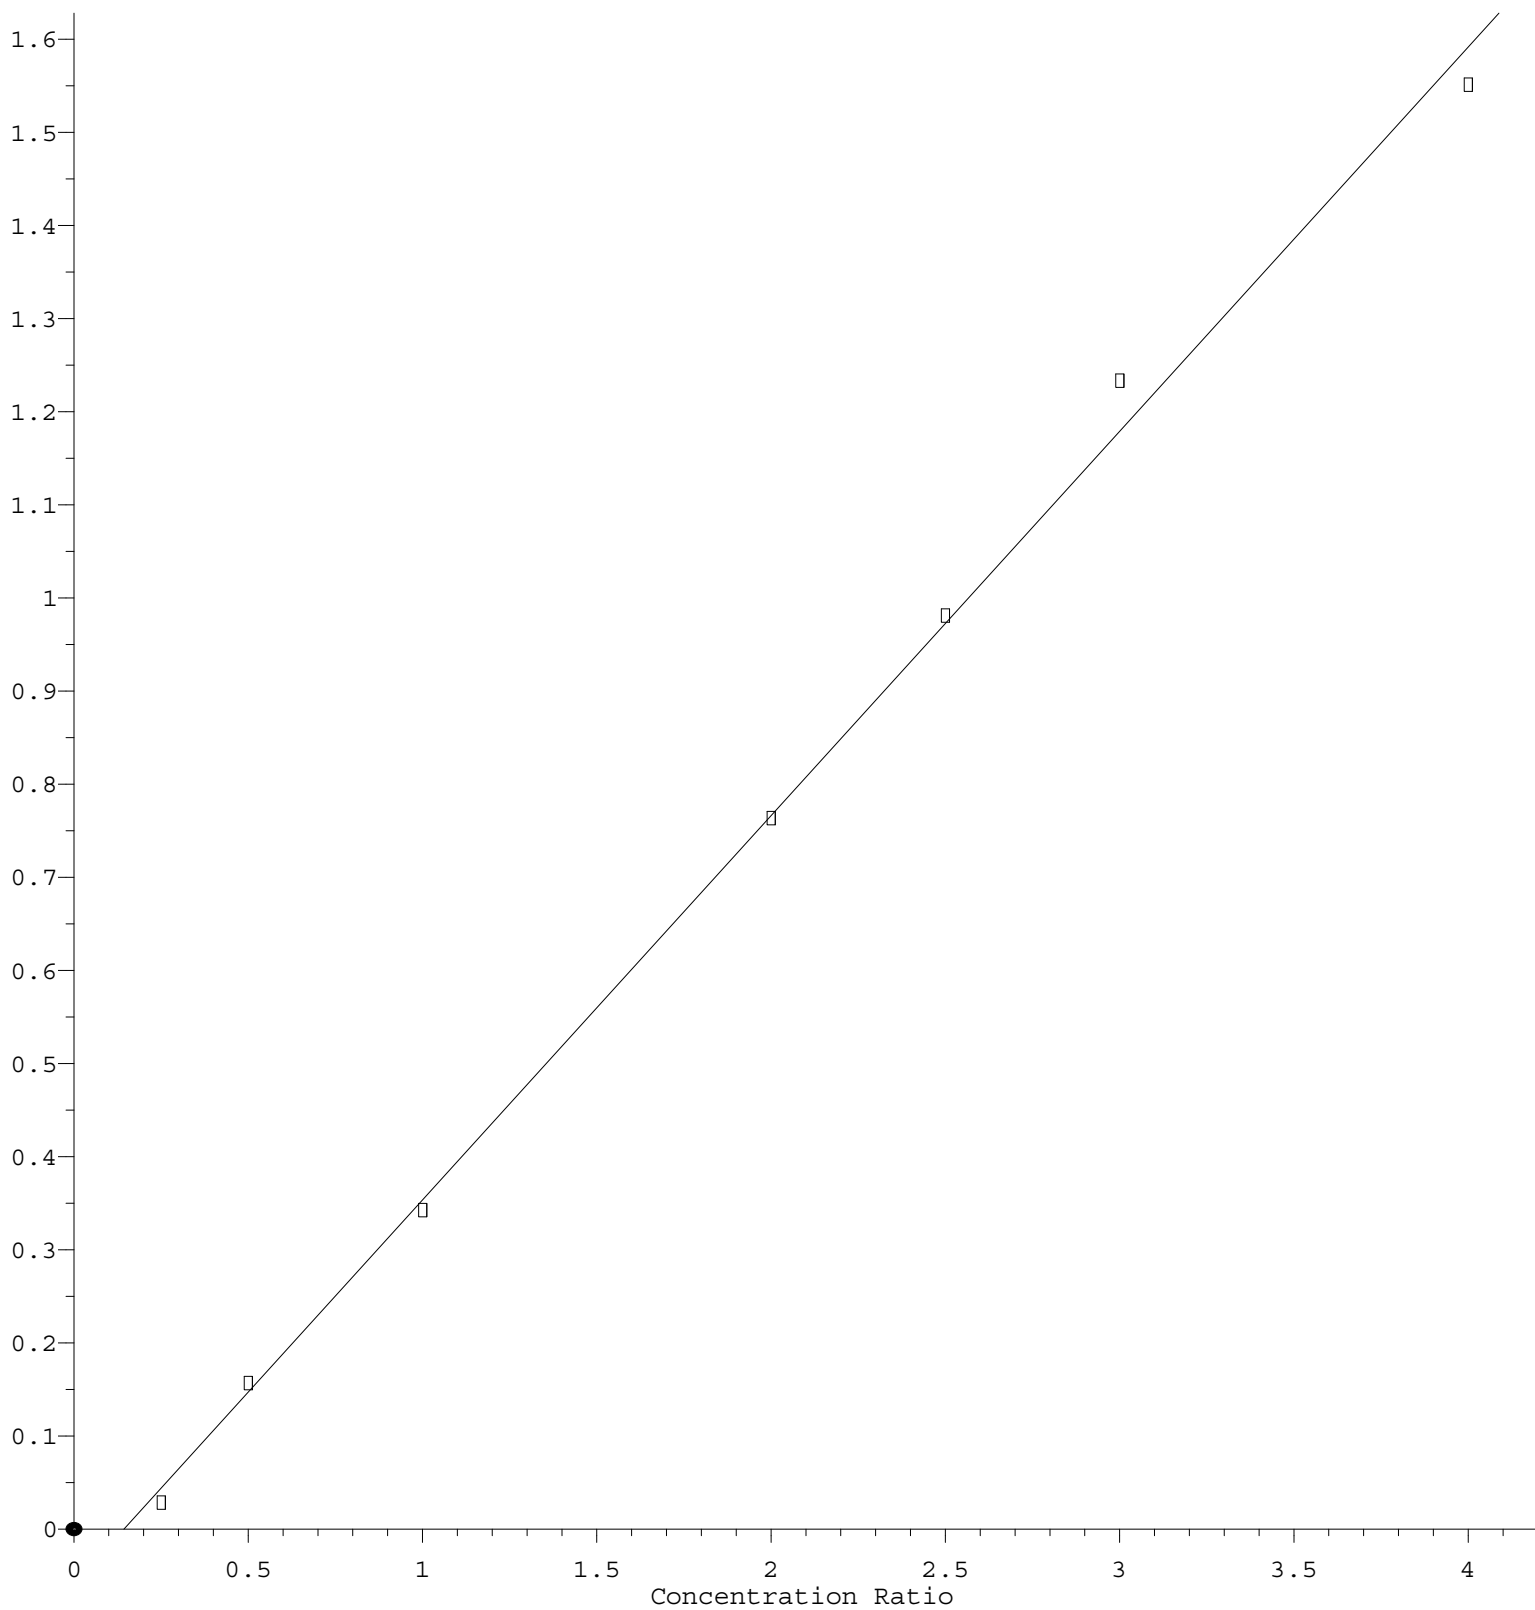

$$\text{Response} = 4.128\text{e-}001 * \text{Amt} - 5.897\text{e-}002$$


Coef of Det (r^2) = 0.997394 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP071522.M

Calibration Table Last Updated: Fri Jul 15 13:54:34 2022

Benzidine

Response Ratio

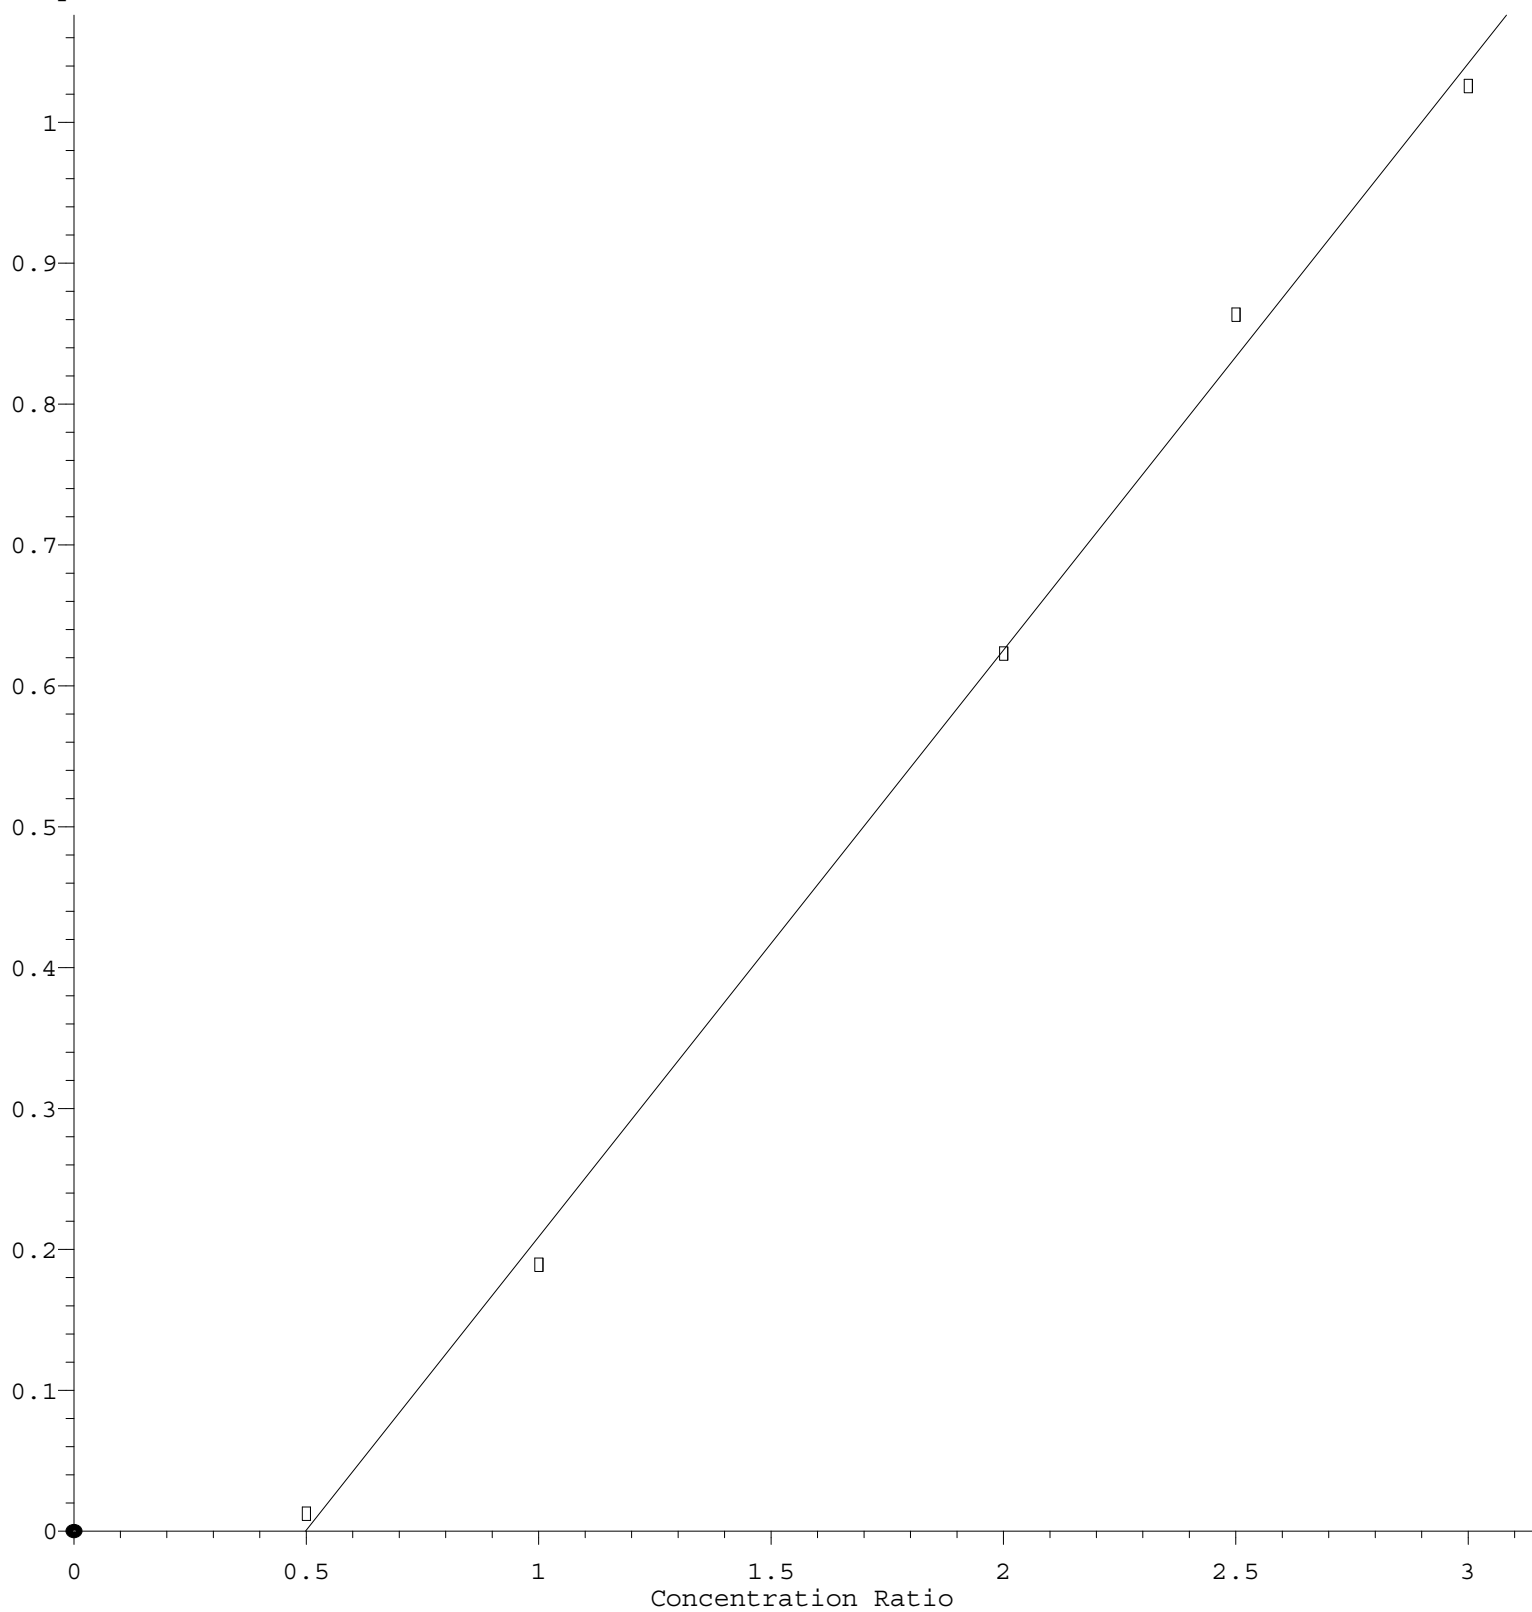

$$\text{Response} = 4.168\text{e-}001 * \text{Amt} - 2.076\text{e-}001$$

Coef of Det (r^2) = 0.997753 Curve Fit: Linear

Method Name: Z:\svoasrv\HPCHEM1\BNA P\Methods\8270E-BP071522.M

Calibration Table Last Updated: Fri Jul 15 13:54:34 2022