
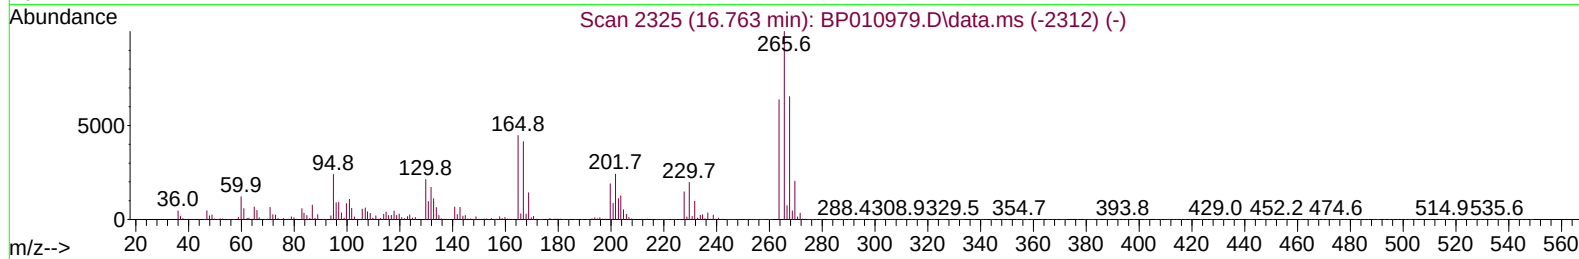
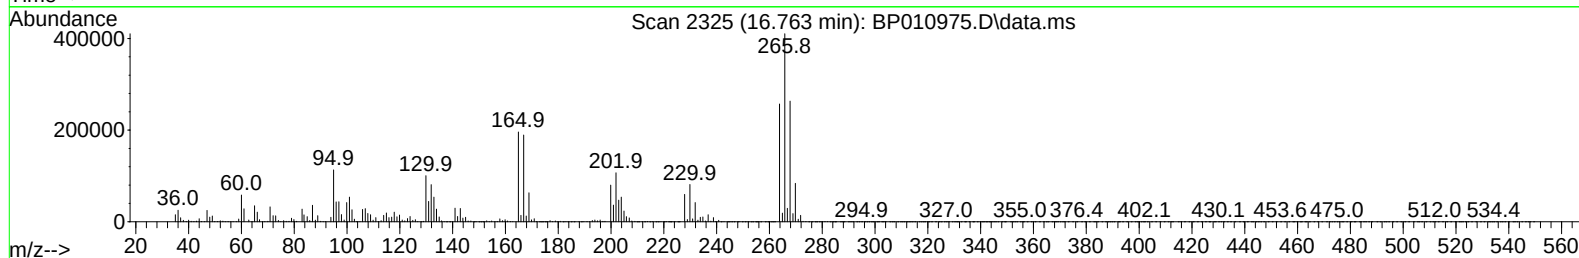


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071522\
Data File : BP010975.D
Acq On : 15 Jul 2022 08:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 13:55:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 13:54:34 2022
Response via : Initial Calibration

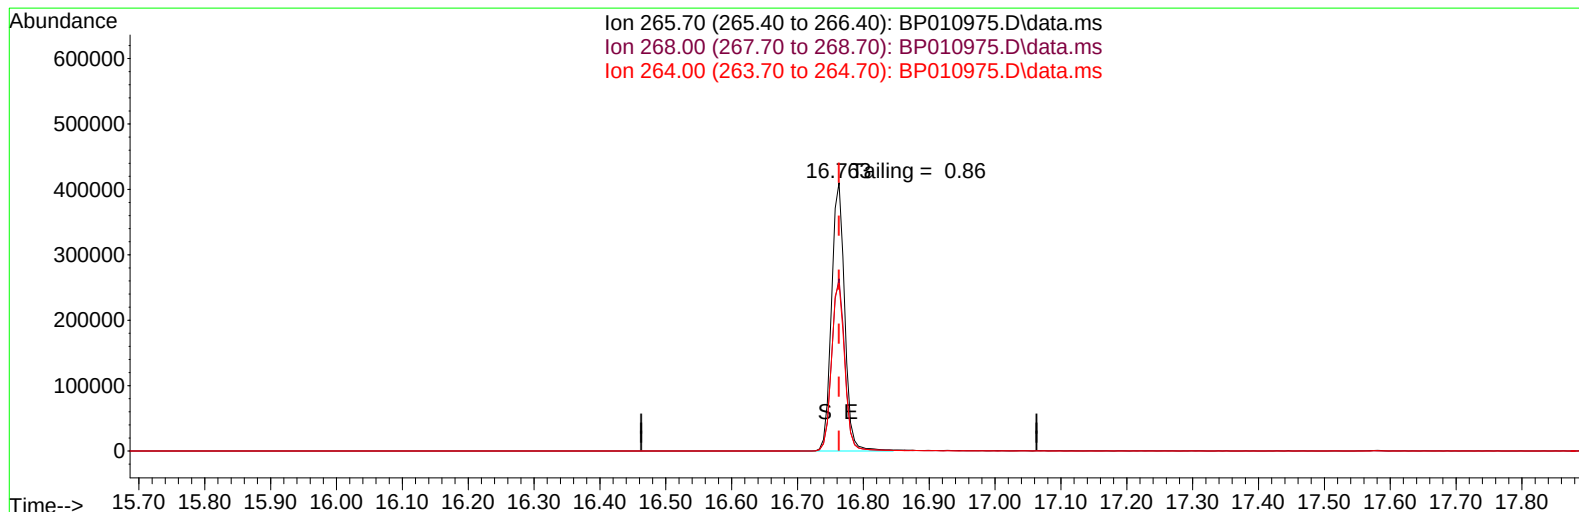

TIC: BP010975.D\data.ms

(70) Pentachlorophenol (C)




16.763min (+ 0.000) 70333.18 ng

response 573563

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.18
264.00	63.00	62.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071522\
Data File : BP010975.D
Acq On : 15 Jul 2022 08:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 15 13:55:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 13:54:34 2022
Response via : Initial Calibration

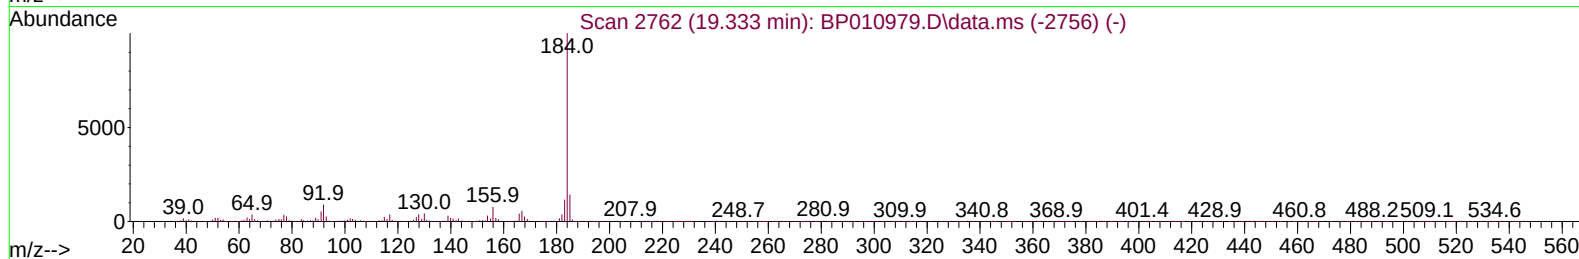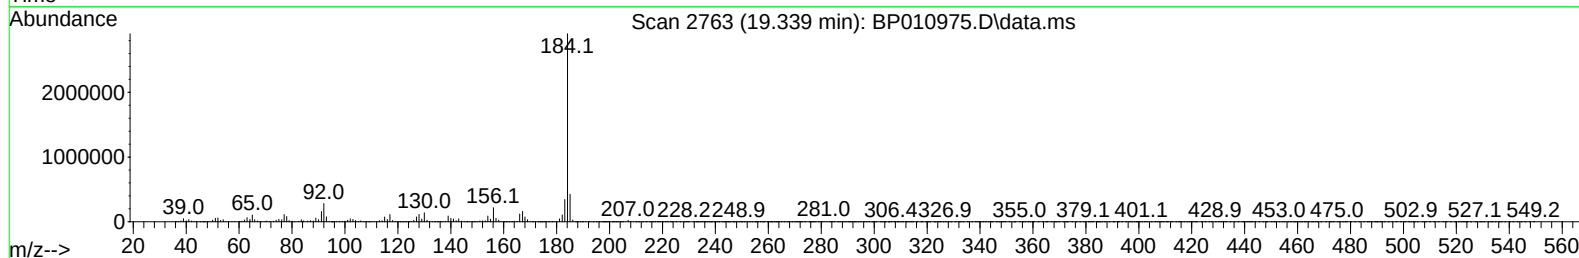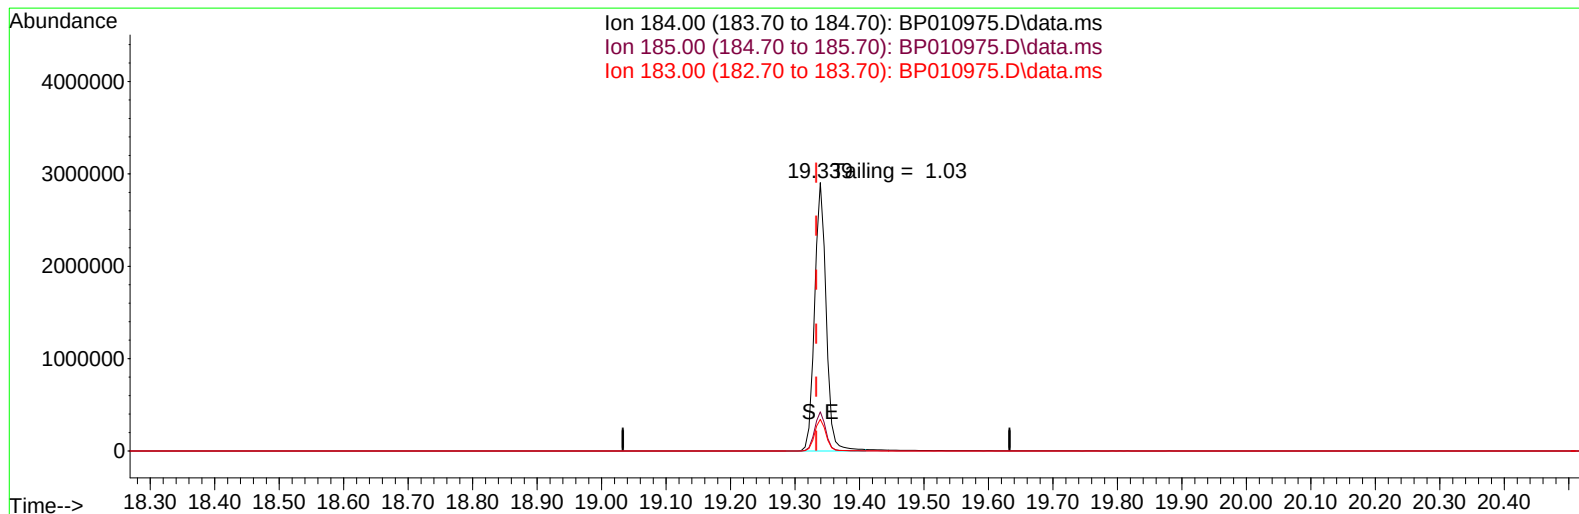

TIC: BP010975.D\data.ms

(77) Benzidine

19.339min (+ 0.006) 27166.97 ng

response 3686904

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.62
183.00	11.30	11.80
0.00	0.00	0.00