
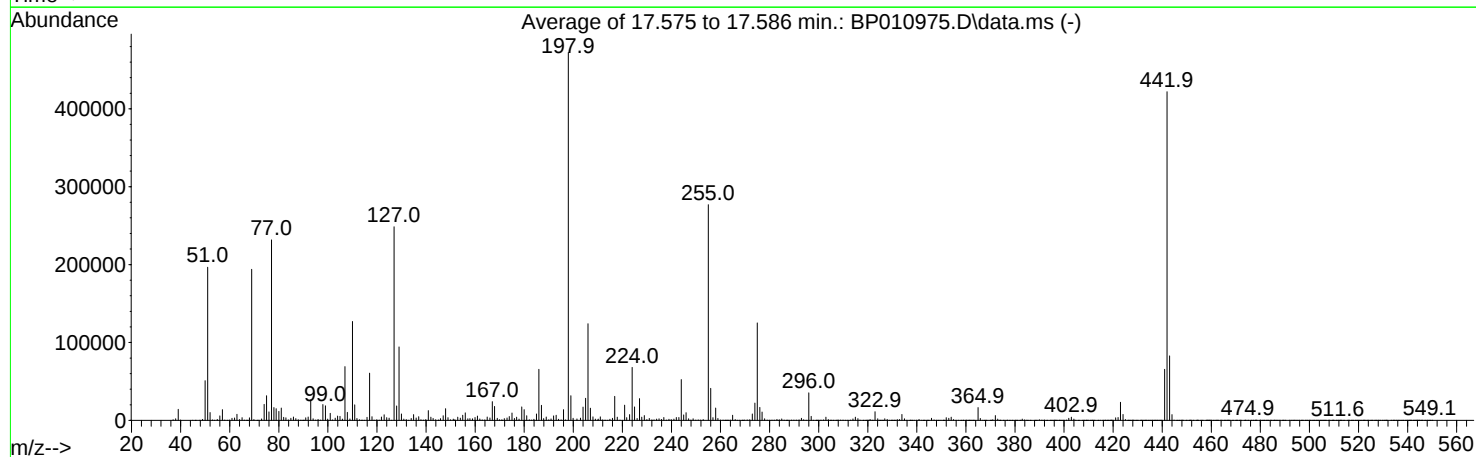


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071522\
 Data File : BP010975.D
 Acq On : 15 Jul 2022 08:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP071522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 15 13:54:34 2022

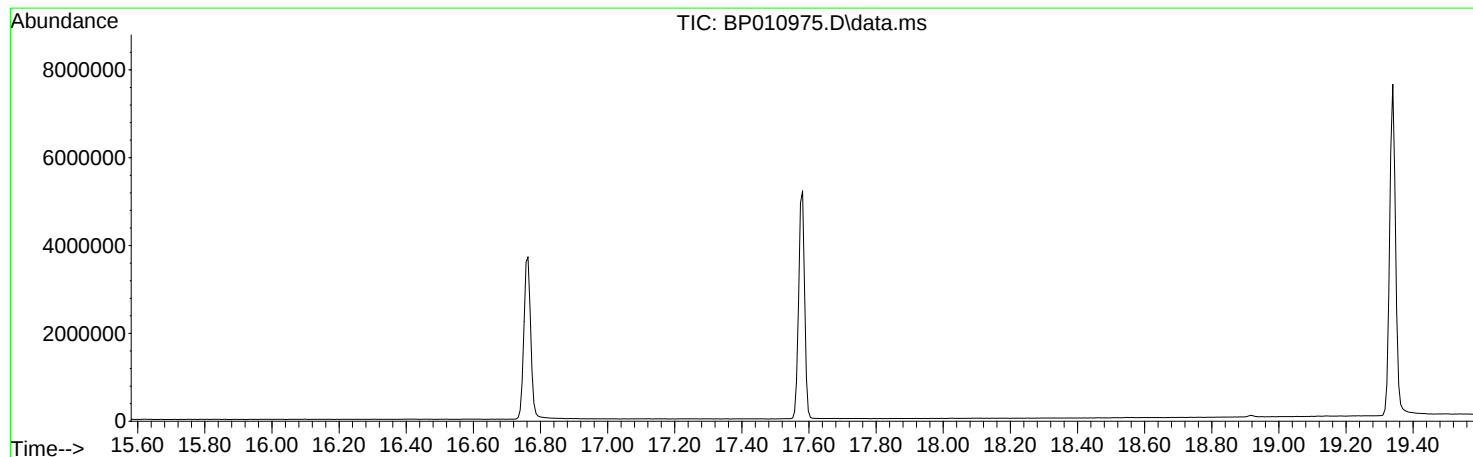

AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.6	196616	PASS
68	69	0.00	2	1.7	3258	PASS
69	198	0.00	100	41.1	193940	PASS
70	69	0.00	2	0.6	1083	PASS
127	198	10	80	52.6	248516	PASS
197	198	0.00	2	0.1	656	PASS
198	198	100	100	100.0	472320	PASS
199	198	5	9	6.7	31659	PASS
275	198	10	60	26.5	125141	PASS
365	198	1	100	3.5	16507	PASS
441	198	0.01	100	13.9	65494	PASS
442	442	100	100	100.0	422035	PASS
443	442	15	24	19.6	82763	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/15/2022	BNA_P	<u>BP010975.D</u>
Compound Name	Response	Retention Time
DDT	1718653	20.55
DDD	11430	20.11
DDE	1317	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12747	1731400	0.74

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071522\
Data File : BP010975.D
Acq On : 15 Jul 2022 08:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 15 13:55:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 13:54:34 2022
Response via : Initial Calibration

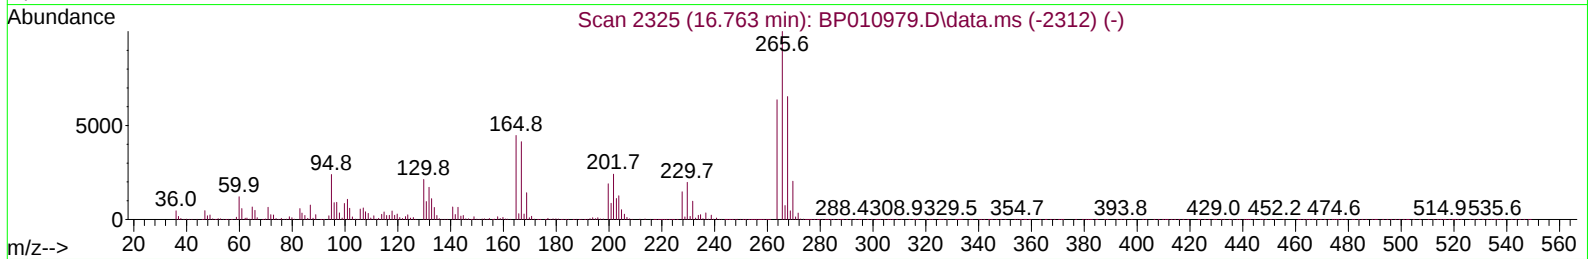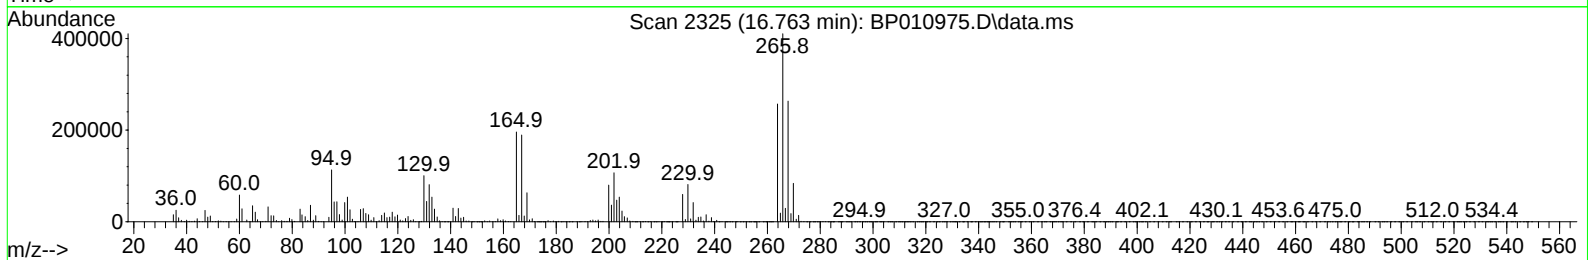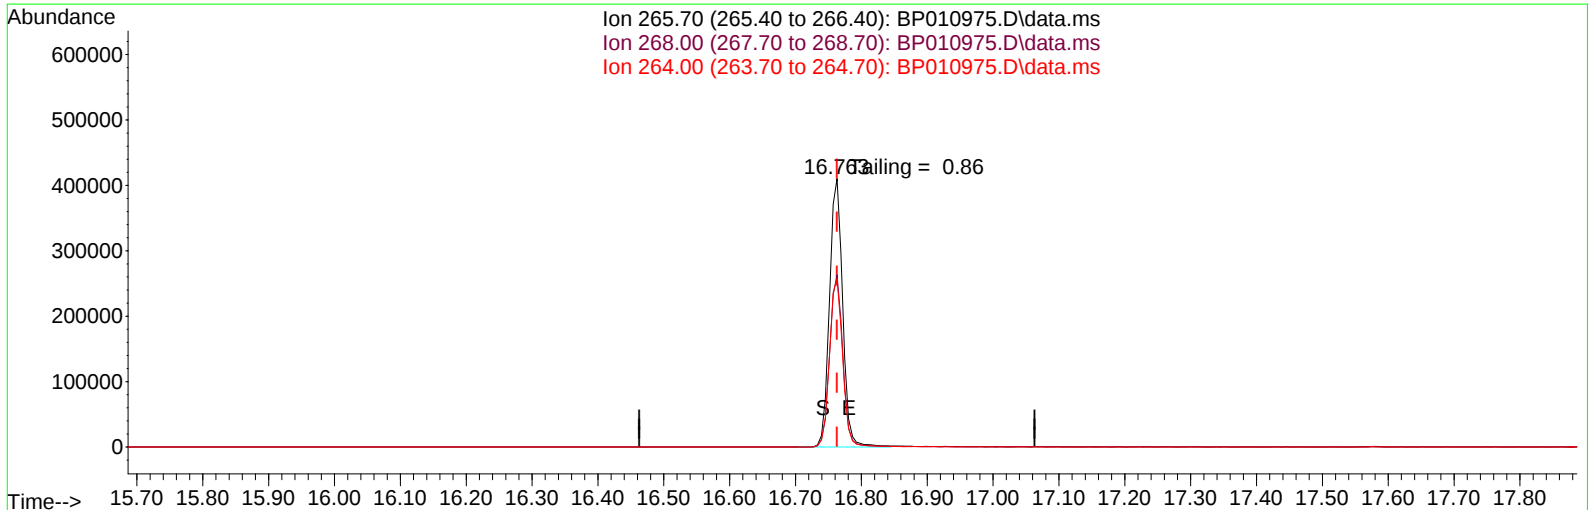

TIC: BP010975.D\data.ms

(70) Pentachlorophenol (C)

16.763min (+ 0.000) 70333.18 ng




response 573563

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.18
264.00	63.00	62.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071522\
Data File : BP010975.D
Acq On : 15 Jul 2022 08:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 15 13:55:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP071522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 15 13:54:34 2022
Response via : Initial Calibration

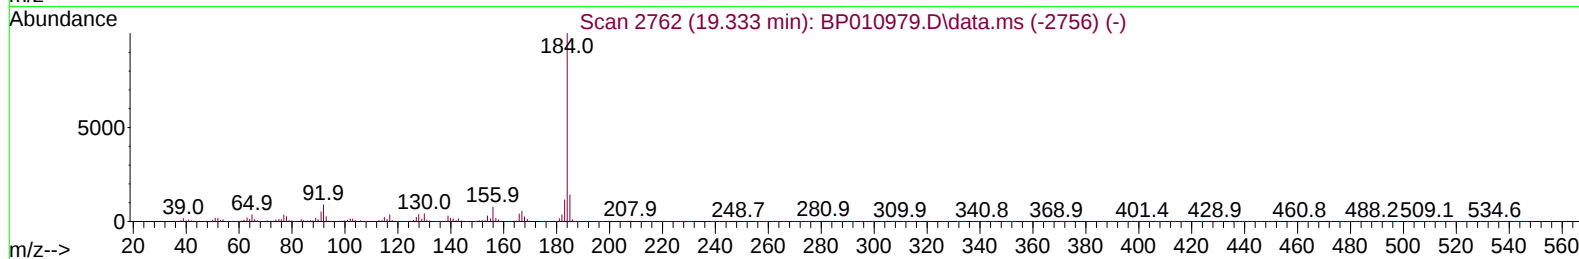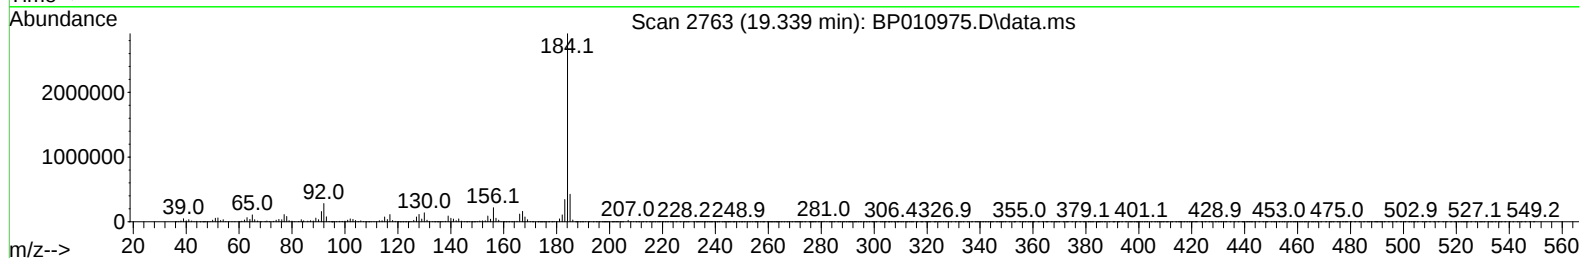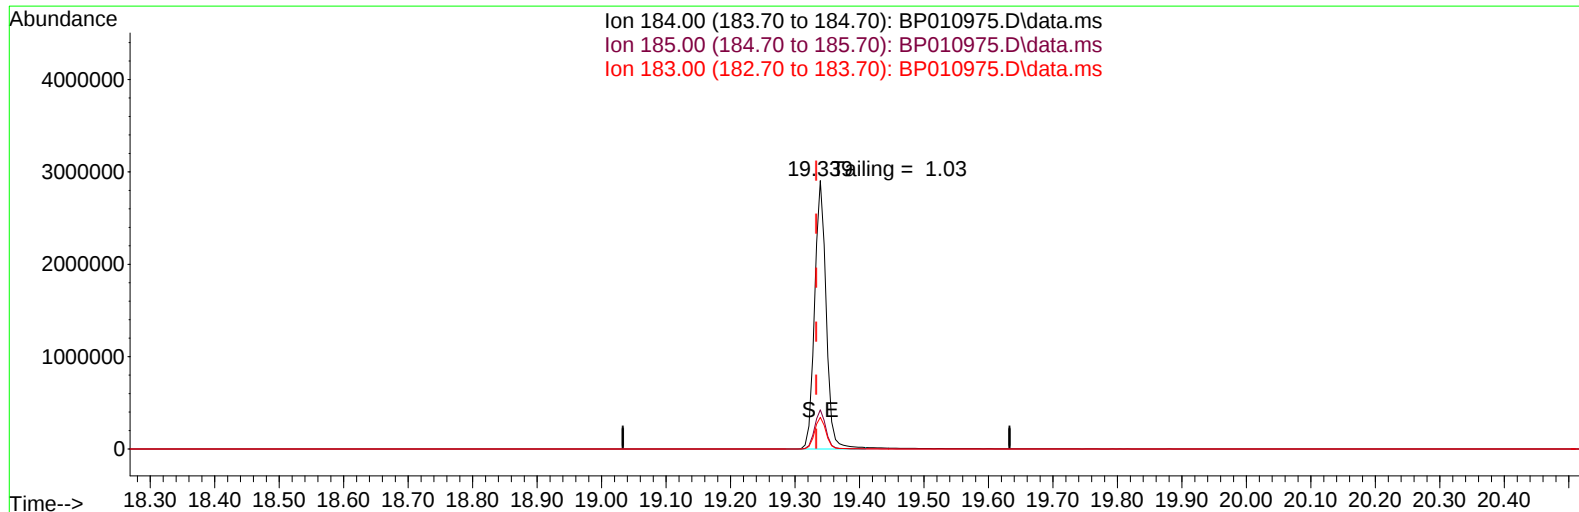

TIC: BP010975.D\data.ms

(77) Benzidine

19.339min (+ 0.006) 27166.97 ng

response 3686904

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.62
183.00	11.30	11.80
0.00	0.00	0.00