
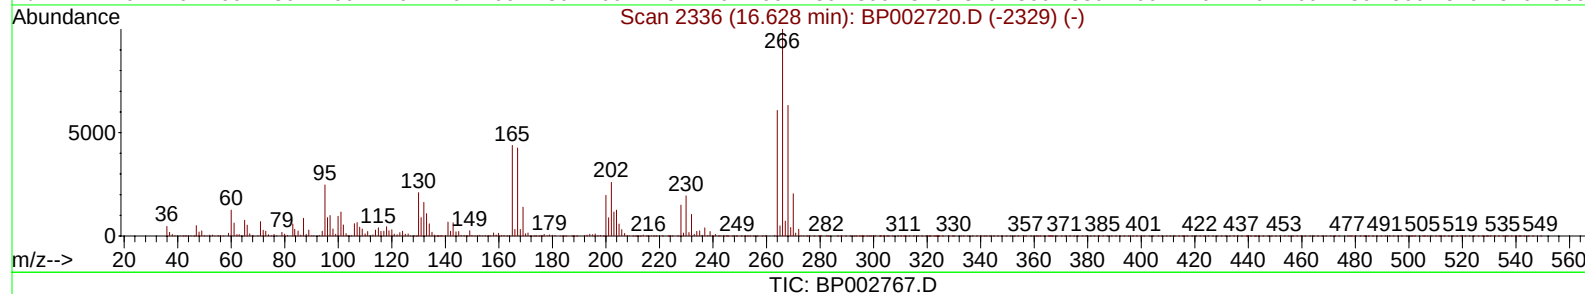
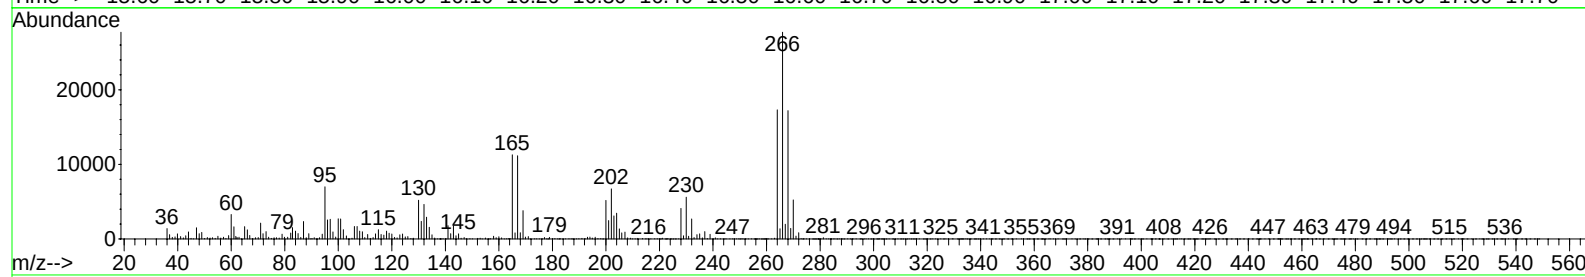


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP071620\
Data File : BP002767.D
Acq On : 16 Jul 2020 11:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 17:21:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 13 10:54:03 2020
Response via : Initial Calibration

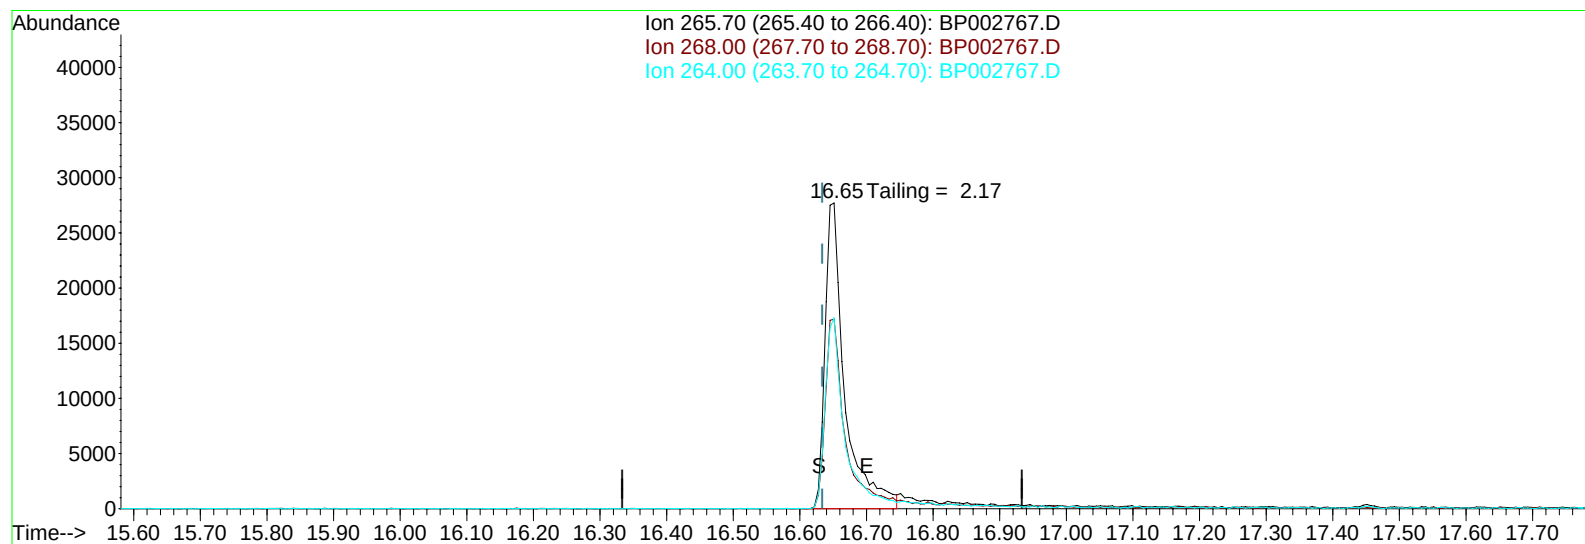

(70) Pentachlorophenol (C)




16.651min (+0.018) 332582.30ng

response 59027

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	62.04
264.00	60.70	62.44
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP071620\
 Data File : BP002767.D
 Acq On : 16 Jul 2020 11:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 17:21:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 13 10:54:03 2020
 Response via : Initial Calibration

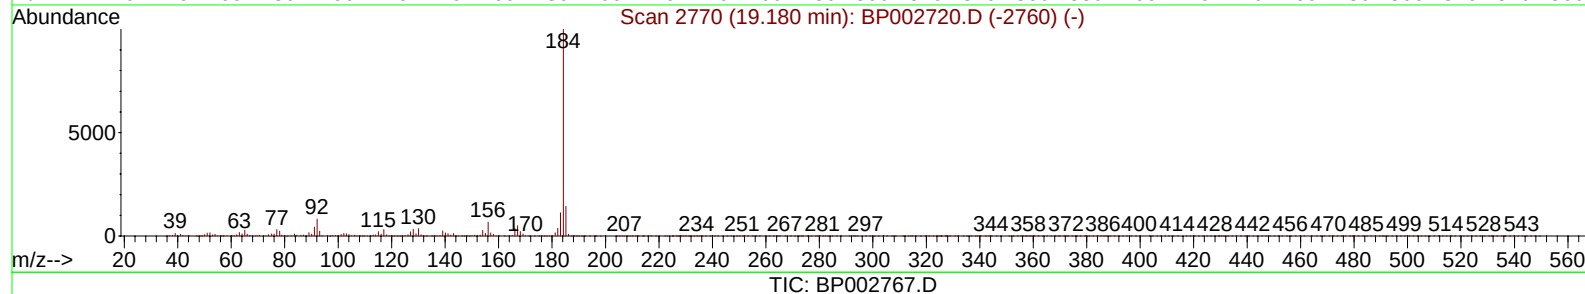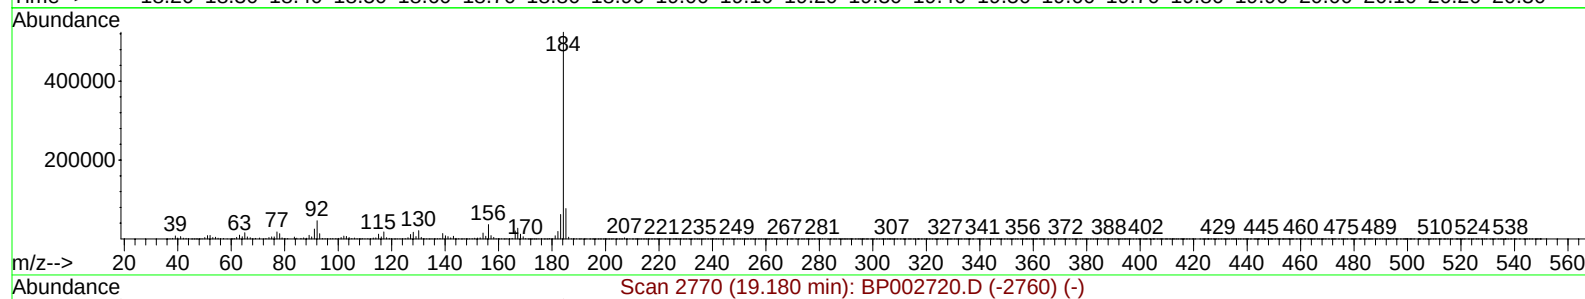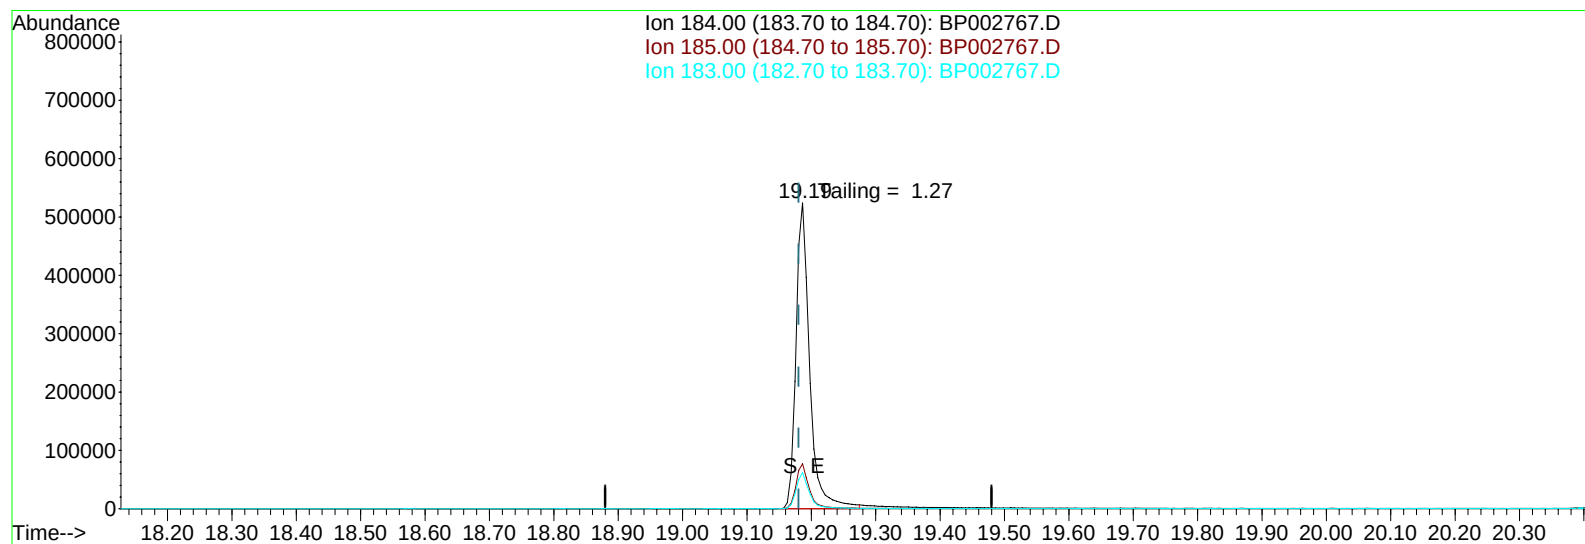

(77) Benzidine

19.186min (+0.006) 121092.55ng

response 669337

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	14.71
183.00	11.20	11.84
0.00	0.00	0.00