

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP071620\
 Data File : BP002773.D
 Acq On : 16 Jul 2020 15:40
 Operator : CG/JU
 Sample : L3308-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 1

Quant Time: Jul 17 02:09:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 13 10:54:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	225019	20.00	ng	0.00
21) Naphthalene-d8	10.33	136	971845	20.00	ng	0.00
39) Acenaphthene-d10	14.21	164	584689	20.00	ng	0.00
64) Phenanthrene-d10	16.97	188	1125758	20.00	ng	0.00
76) Chrysene-d12	21.08	240	766555	20.00	ng	0.00
86) Perylene-d12	23.27	264	660033	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.19	112	1092589	81.92	ng	0.00
7) Phenol-d6	6.76	99	1529713	80.37	ng	0.00
23) Nitrobenzene-d5	8.70	82	995144	54.77	ng	0.00
42) 2,4,6-Tribromophenol	15.72	330	478722	78.44	ng	0.00
45) 2-Fluorobiphenyl	12.82	172	1927613	51.00	ng	0.00
79) Terphenyl-d14	19.56	244	1994622	59.66	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.67	163	413329	9.269	ng	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP071620\
Data File : BP002773.D
Acq On : 16 Jul 2020 15:40
Operator : CG/JU
Sample : L3308-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
1

Quant Time: Jul 17 02:09:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 13 10:54:03 2020
Response via : Initial Calibration

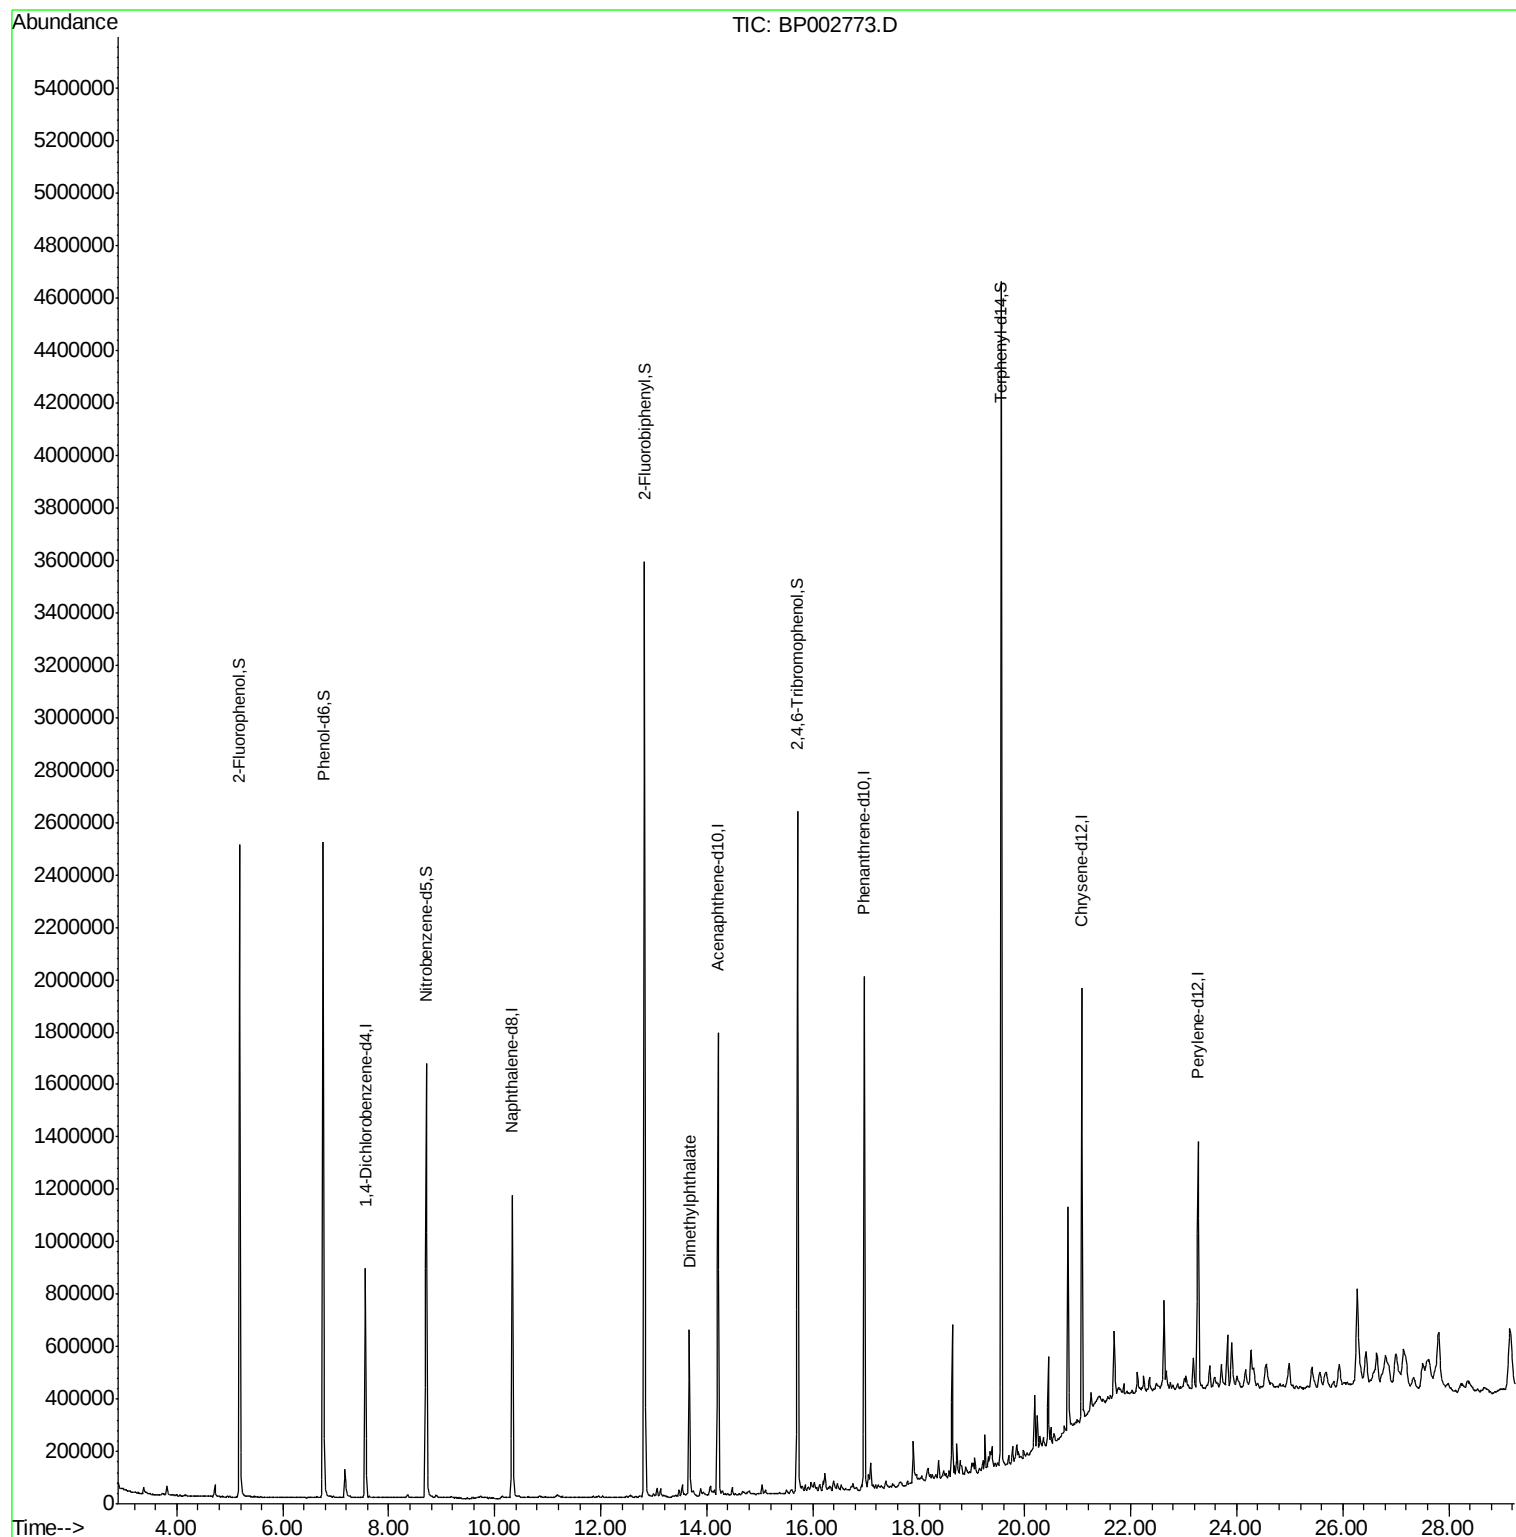




#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.56 min Scan# 794
Delta R.T. 0.01 min
Lab File: BP002773.D
Acq: 16 Jul 2020 15:40

Instrument :
BNA_P
ClientSampleId :
1

Tot Ion	Ratio	Lower	Upper
152	100		
150	158.0	123.7	185.5
115	59.1	47.2	70.8

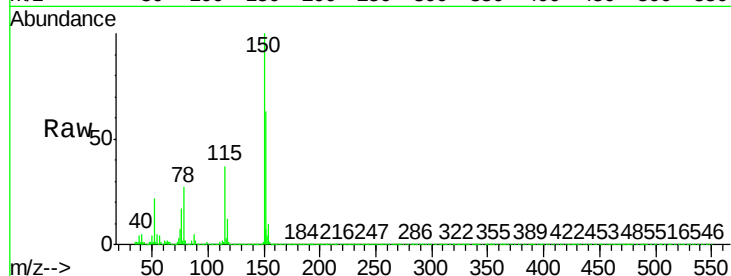


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

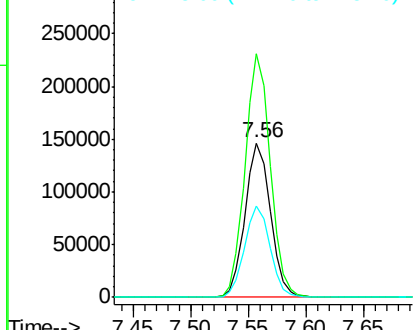



#5


2-Fluorophenol
Concen: 81.922 ng
RT: 5.19 min Scan# 391
Delta R.T. 0.01 min
Lab File: BP002773.D
Acq: 16 Jul 2020 15:40

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.3	45.6	68.4
63	31.6	23.5	35.3



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BP0
Ion 63.00 (62.70 to 63.70): BP0

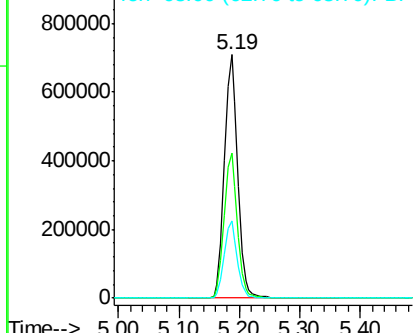

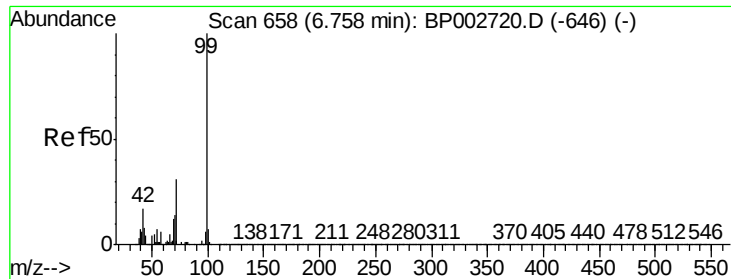

#7

Phenol-d6

Concen: 80.367 ng

RT: 6.76 min Scan# 659

Delta R.T. 0.01 min

Lab File: BP002773.D

Acq: 16 Jul 2020 15:40

Instrument :


BNA_P

ClientSampleId :

1

Tot Ion: 99 Resp: 1529713

Ion	Ratio	Lower	Upper
99	100		
42	18.0	13.4	20.2
71	33.3	24.6	36.8






Abundance

Ion 99.00 (98.70 to 99.70): BP0

Ion 42.00 (41.70 to 42.70): BP0

Ion 71.00 (70.70 to 71.70): BP0

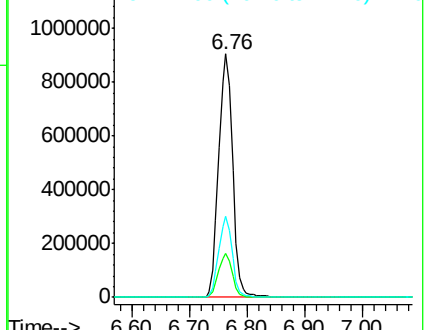

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.33 min Scan# 1265


Delta R.T. -0.00 min

Lab File: BP002773.D

Acq: 16 Jul 2020 15:40

Tgt Ion: 136 Resp: 971845

Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.6	13.0
54	9.1	6.9	10.3
68	7.5	5.7	8.5





Abundance


Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BP0

Ion 68.00 (67.70 to 68.70): BP0




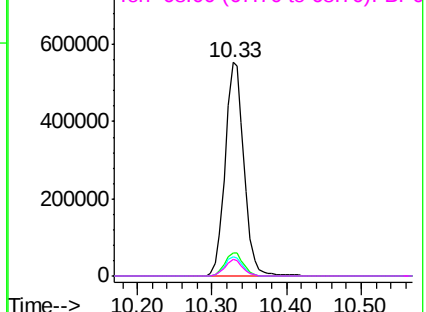


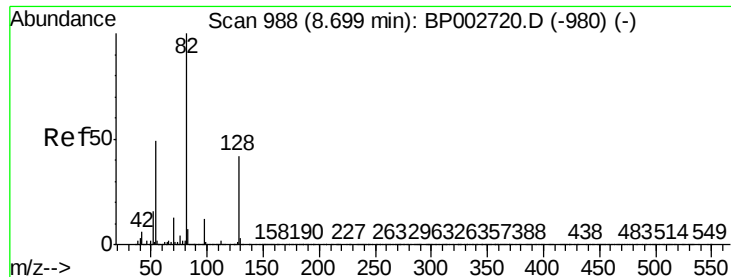

#23
 Nitrobenzene-d5
 Concen: 54.766 ng
 RT: 8.70 min Scan# 989
 Delta R.T. -0.00 min
 Lab File: BP002773.D
 Acq: 16 Jul 2020 15:40




Instrument :
 BNA_P
 ClientSampleId :
 1


Tot Ion	82	Resp	995144
Ion Ratio	Lower	Upper	
82	100		
128	40.4	33.8	50.8
54	49.0	38.8	58.2

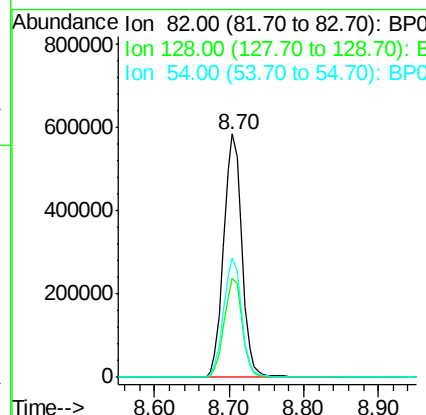

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.21 min Scan# 1925
 Delta R.T. -0.00 min
 Lab File: BP002773.D
 Acq: 16 Jul 2020 15:40

Tgt Ion	164	Resp	584689
Ion Ratio	Lower	Upper	
164	100		
162	99.1	80.6	121.0
160	45.4	36.4	54.6

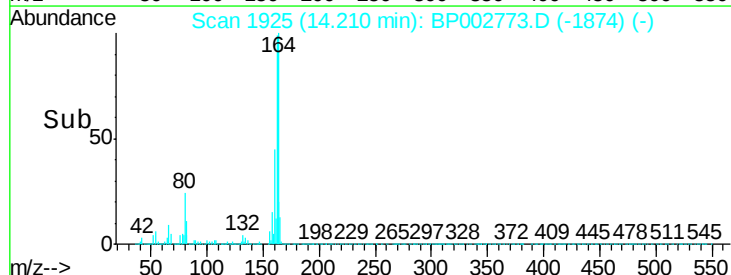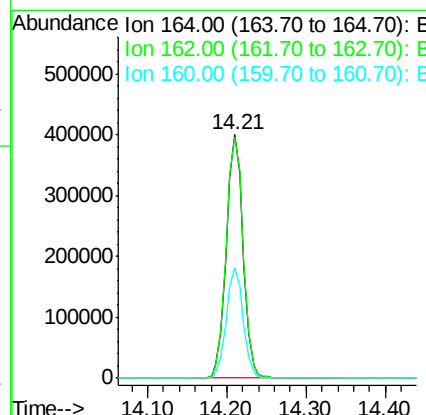







#42
2,4,6-Tribromophenol
Concen: 78.438 ng
RT: 15.72 min Scan# 2181
Delta R.T. 0.01 min
Lab File: BP002773.D
Acq: 16 Jul 2020 15:40

Instrument :
BNA_P
ClientSampleId :
1

Tot Ion:330 Resp: 478722
Ion Ratio Lower Upper
330 100
332 96.4 76.5 114.7
141 35.3 28.8 43.2




Abundance Ion 329.80 (329.50 to 330.50): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E


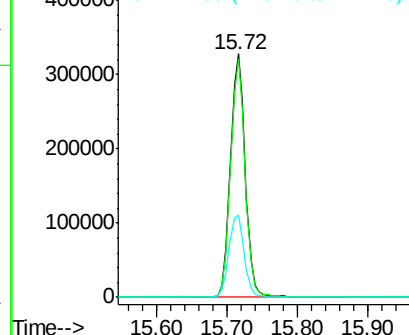



#45
2-Fluorobiphenyl
Concen: 51.001 ng
RT: 12.82 min Scan# 1689
Delta R.T. -0.00 min
Lab File: BP002773.D
Acq: 16 Jul 2020 15:40

Tgt Ion:172 Resp: 1927613
Ion Ratio Lower Upper
172 100
171 35.5 28.1 42.1
170 23.9 19.3 28.9



Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

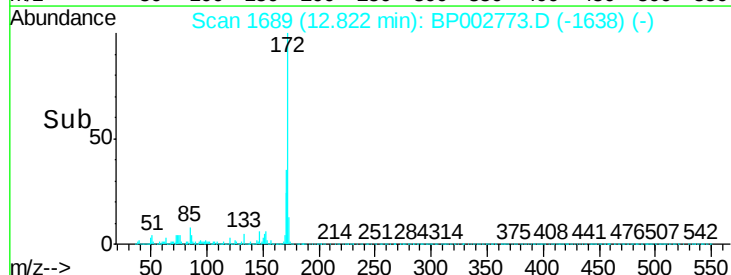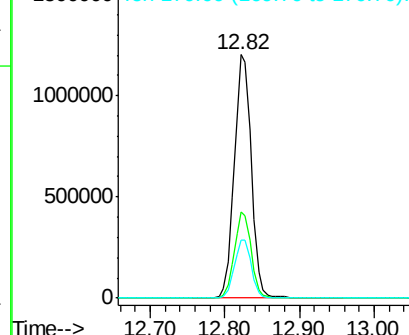



#50

Dimethylphthalate

Concen: 9.269 ng

RT: 13.67 min Scan# 1833

Delta R.T. -0.01 min

Lab File: BP002773.D

Acq: 16 Jul 2020 15:40

Instrument :

BNA_P

ClientSampleId :

1


Tot Ion:163 Resp: 413329

Ion Ratio Lower Upper

163 100

194 4.1 3.4 5.2




164 10.7 7.8 11.8



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

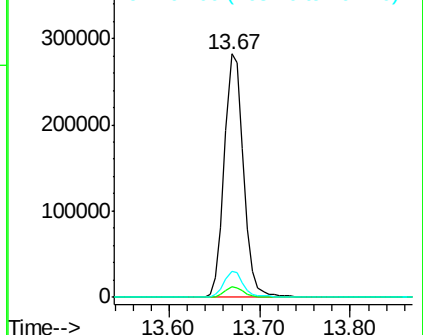

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.97 min Scan# 2394

Delta R.T. -0.00 min

Lab File: BP002773.D

Acq: 16 Jul 2020 15:40


Tgt Ion:188 Resp: 1125758

Ion Ratio Lower Upper

188 100

94 11.0 8.1 12.1



80 12.0 8.9 13.3




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0



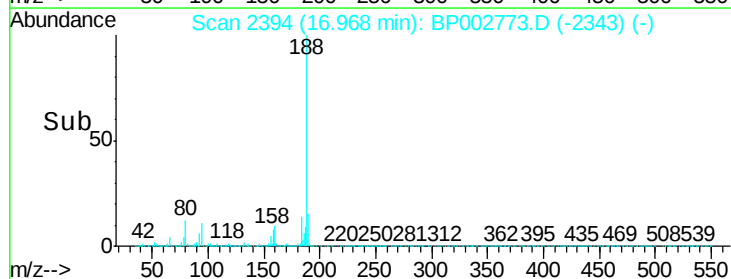
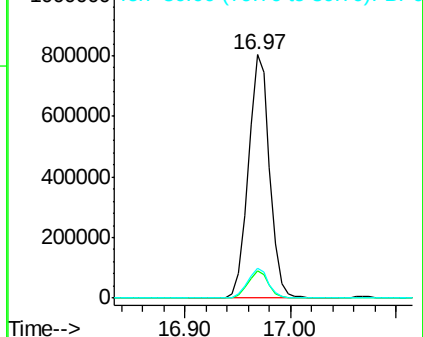


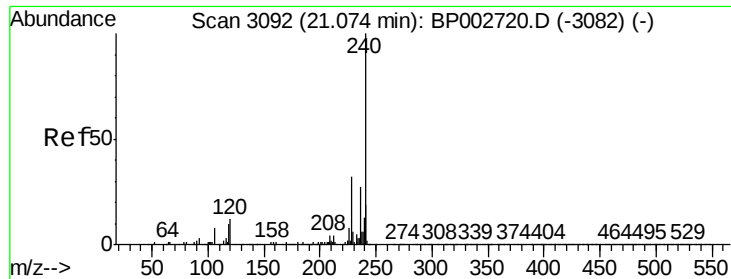

#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 21.08 min Scan# 3093
 Delta R.T. 0.01 min
 Lab File: BP002773.D
 Acq: 16 Jul 2020 15:40




Instrument :
 BNA_P
 ClientSampleId :
 1


Tot Ion:240 Resp: 766555
 Ion Ratio Lower Upper
 240 100
 120 11.6 9.4 14.2
 236 26.9 21.3 31.9

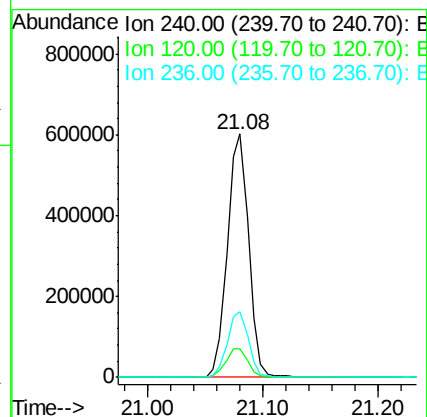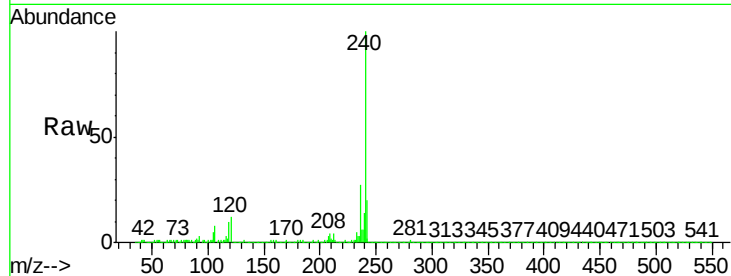

#79
 Terphenyl-d14
 Concen: 59.658 ng
 RT: 19.56 min Scan# 2834
 Delta R.T. -0.00 min
 Lab File: BP002773.D
 Acq: 16 Jul 2020 15:40

Tgt Ion:244 Resp: 1994622
 Ion Ratio Lower Upper
 244 100
 212 7.8 6.0 9.0
 122 11.3 8.9 13.3

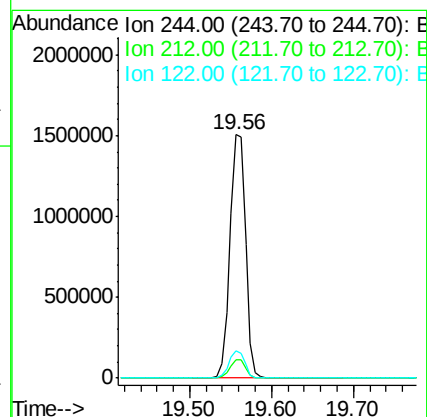


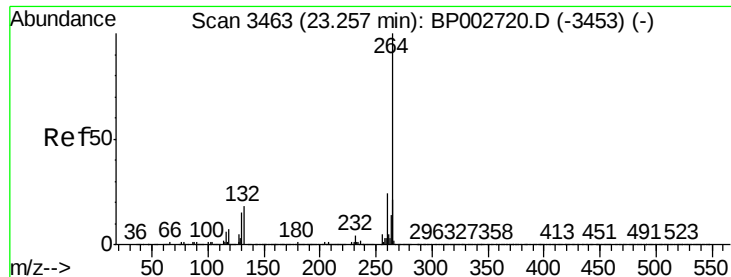

#86
 Pervlene-d12
 Concen: 20.000 ng
 RT: 23.27 min Scan# 3465
 Delta R.T. 0.01 min
 Lab File: BP002773.D
 Acq: 16 Jul 2020 15:40

Instrument :
 BNA_P
 ClientSampleId :
 1

Tot Ion	Ratio	Lower	Upper
264	100		
260	26.2	19.3	28.9
265	22.2	16.8	25.2



Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

