

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP071620\
 Data File : BP002778.D
 Acq On : 16 Jul 2020 18:29
 Operator : CG/JU
 Sample : L3308-08
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 8

Quant Time: Jul 17 02:18:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 13 10:54:03 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.56	152	222753	20.00	ng	0.00
21) Naphthalene-d8	10.33	136	951205	20.00	ng	0.00
39) Acenaphthene-d10	14.21	164	564694	20.00	ng	0.00
64) Phenanthrene-d10	16.97	188	1072330	20.00	ng	0.00
76) Chrysene-d12	21.08	240	744019	20.00	ng	0.00
86) Perylene-d12	23.27	264	653121	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.19	112	1044547	79.12	ng	0.00
7) Phenol-d6	6.76	99	1452985	77.11	ng	0.00
23) Nitrobenzene-d5	8.70	82	934401	52.54	ng	0.00
42) 2,4,6-Tribromophenol	15.72	330	448952	76.16	ng	0.00
45) 2-Fluorobiphenyl	12.82	172	1783013	48.85	ng	0.00
79) Terphenyl-d14	19.56	244	1919011	59.14	ng	0.00
Target Compounds						
50) Dimethylphthalate	13.67	163	307906	7.150	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP071620\
Data File : BP002778.D
Acq On : 16 Jul 2020 18:29
Operator : CG/JU
Sample : L3308-08
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
8

Quant Time: Jul 17 02:18:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 13 10:54:03 2020
Response via : Initial Calibration

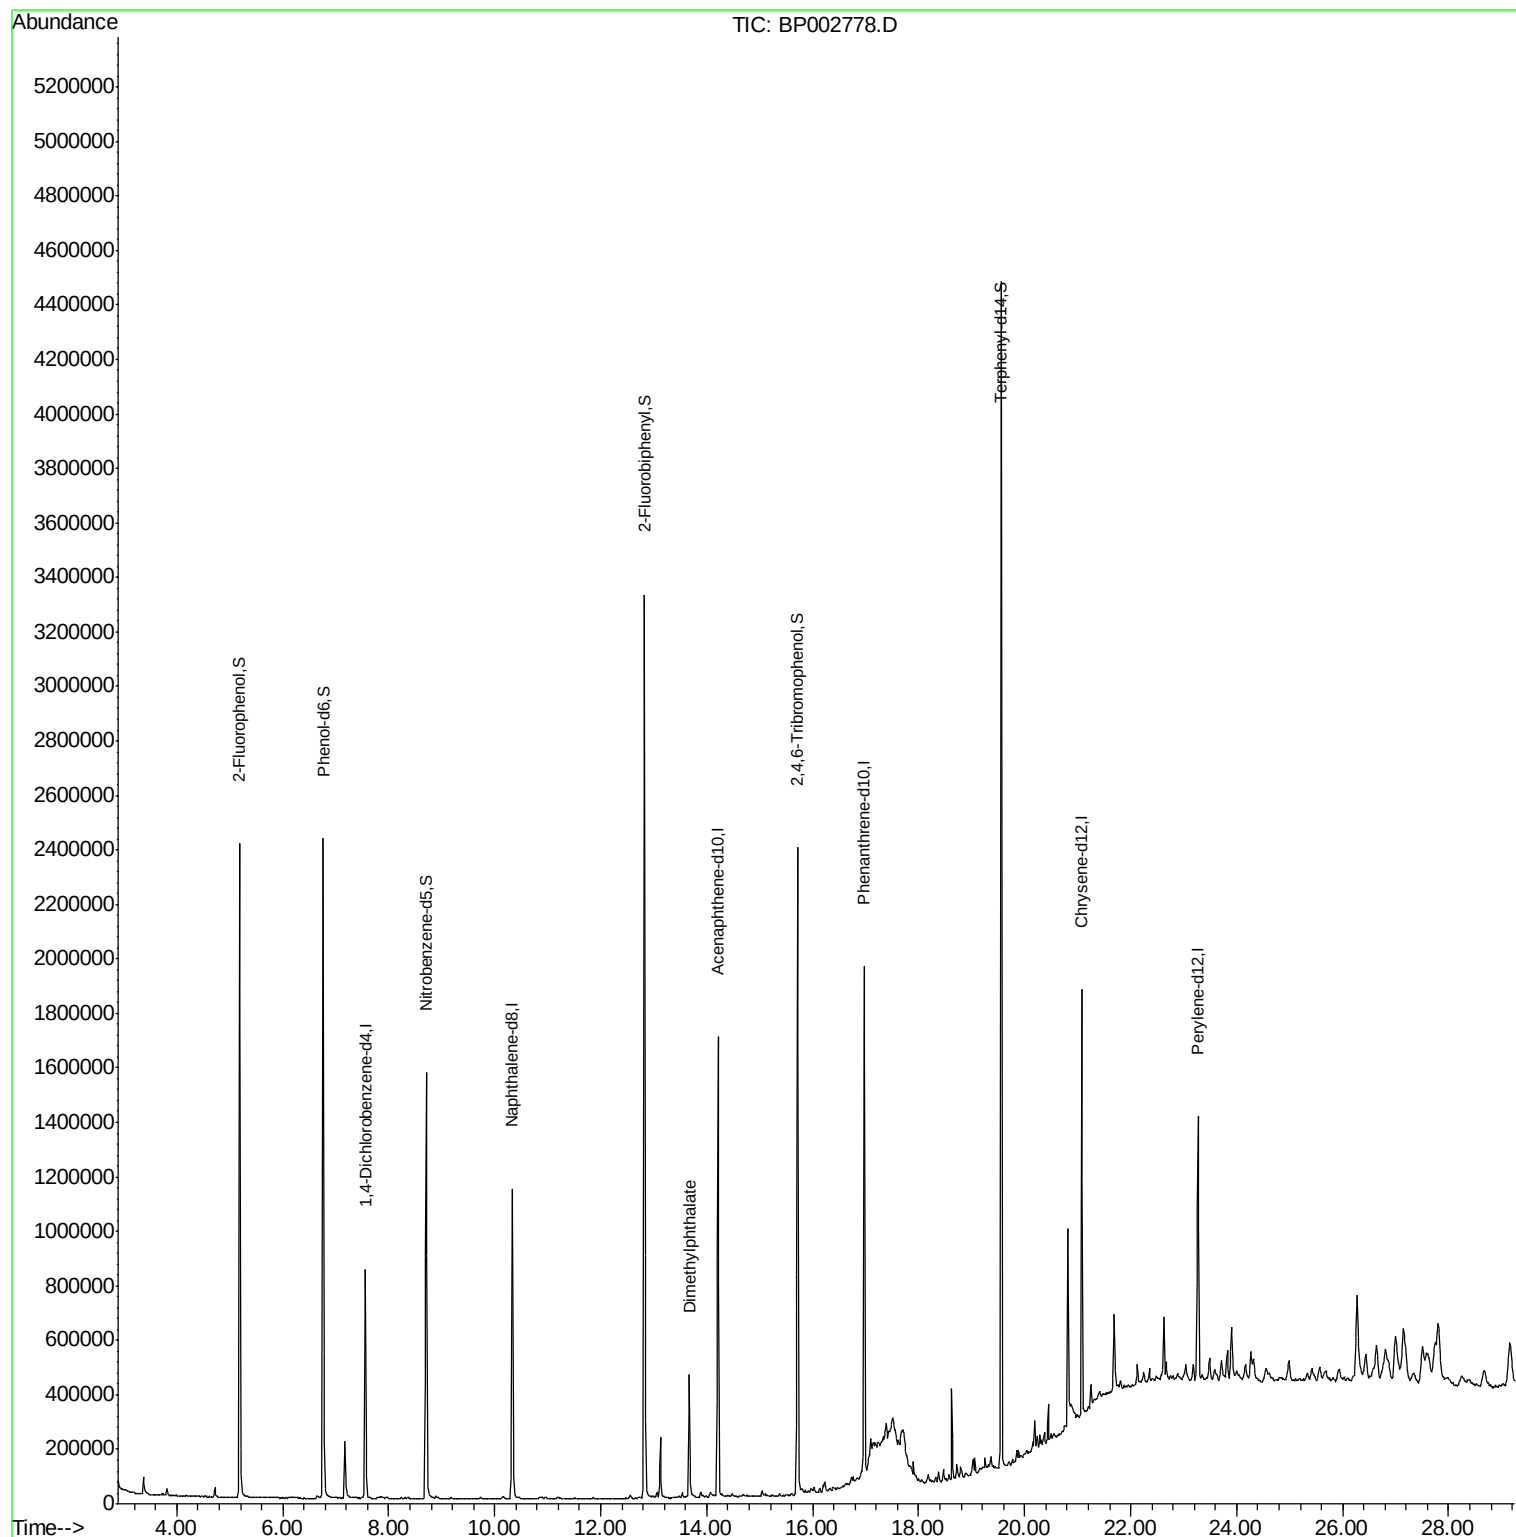

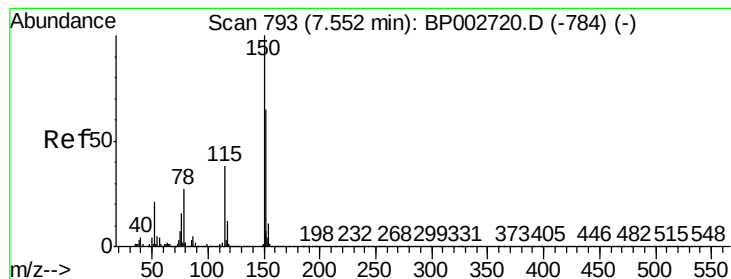


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.56 min Scan# 794
Delta R.T. 0.01 min
Lab File: BP002778.D
Acq: 16 Jul 2020 18:29

Instrument :
BNA_P
ClientSampled :
8

Tot Ion	Ratio	Lower	Upper
152	100		
150	156.5	123.7	185.5
115	59.0	47.2	70.8

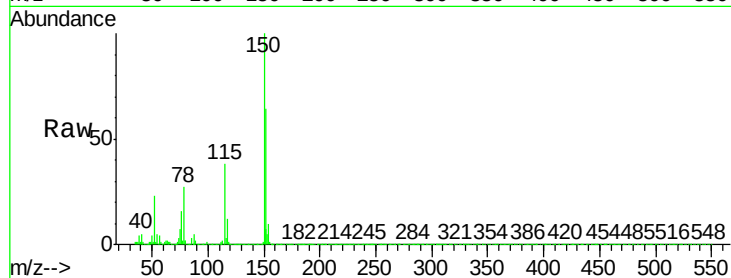


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

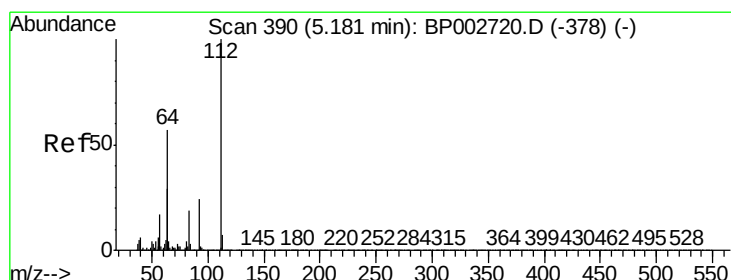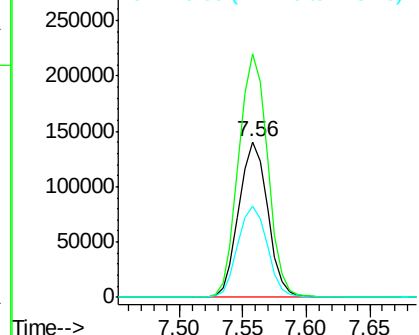



#5


2-Fluorophenol
Concen: 79.117 ng
RT: 5.19 min Scan# 391
Delta R.T. 0.01 min
Lab File: BP002778.D
Acq: 16 Jul 2020 18:29

Tgt Ion	Ratio	Lower	Upper
112	100		
64	59.1	45.6	68.4
63	30.6	23.5	35.3

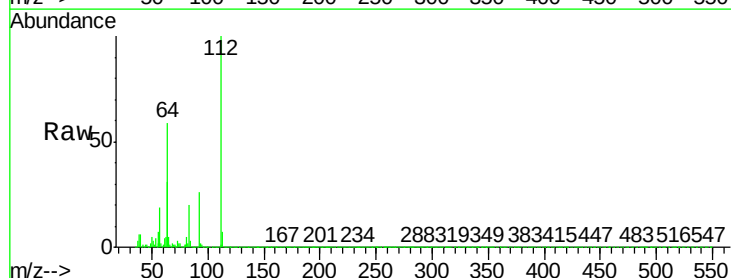

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BP0
Ion 63.00 (62.70 to 63.70): BP0

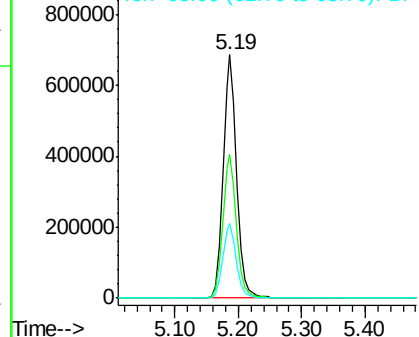

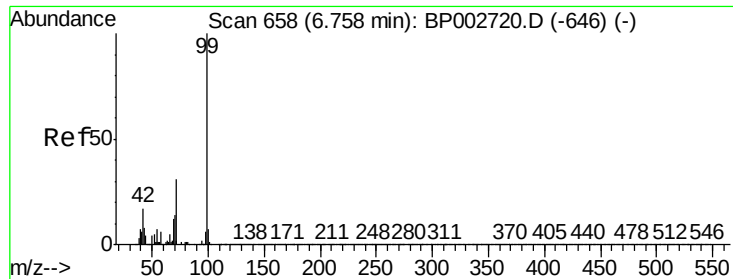

#7

Phenol-d6

Concen: 77.113 ng

RT: 6.76 min Scan# 659

Delta R.T. 0.01 min

Lab File: BP002778.D

Acq: 16 Jul 2020 18:29

Instrument :

BNA_P

ClientSampleId :

8





Tot Ion: 99 Resp: 1452985

Ion Ratio Lower Upper

99 100

42 17.8 13.4 20.2

71 32.4 24.6 36.8

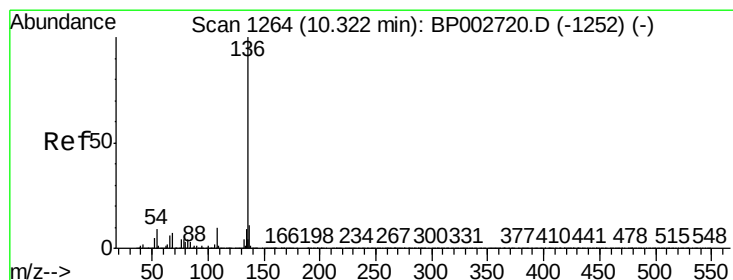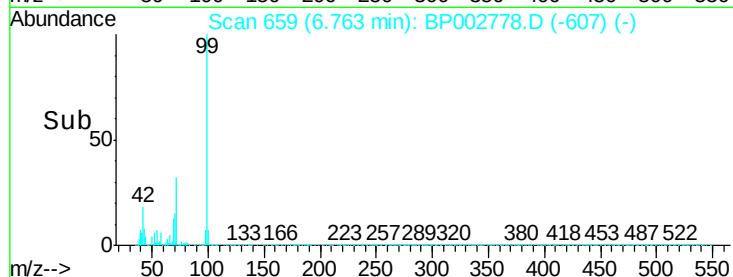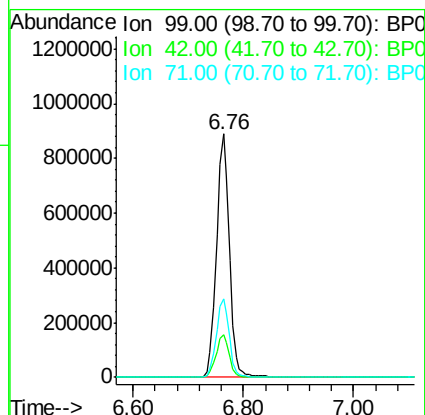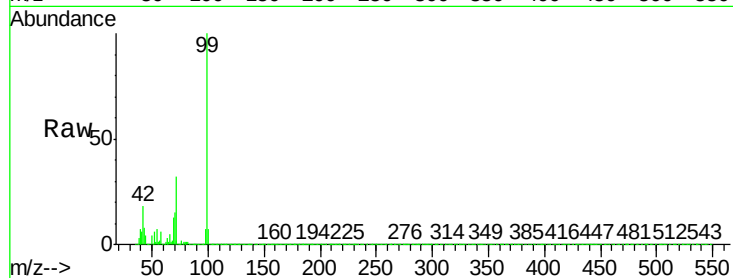

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.33 min Scan# 1265

Delta R.T. 0.00 min

Lab File: BP002778.D

Acq: 16 Jul 2020 18:29

Tgt Ion: 136 Resp: 951205




Ion Ratio Lower Upper


136 100

137 11.1 8.6 13.0

54 9.3 6.9 10.3

68 7.5 5.7 8.5


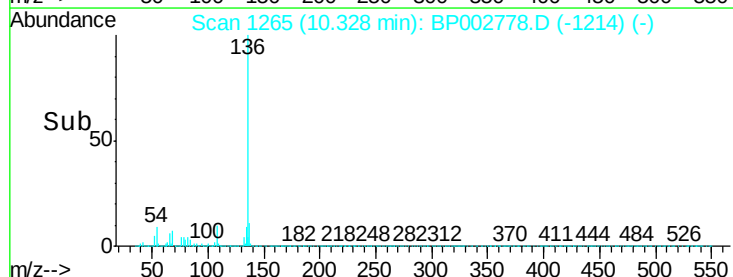
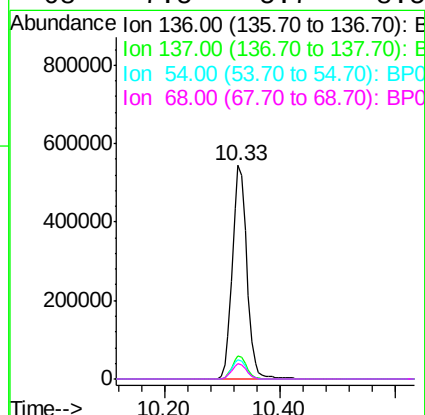
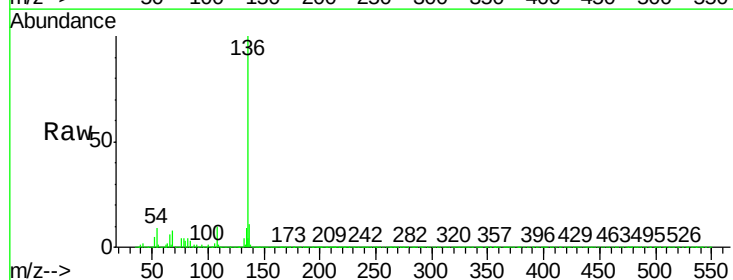




#23
 Nitrobenzene-d5
 Concen: 52.539 ng
 RT: 8.70 min Scan# 989
 Delta R.T. 0.00 min
 Lab File: BP002778.D
 Acq: 16 Jul 2020 18:29




Instrument :
 BNA_P
 ClientSampleId :
 8


Tot Ion	82	Resp	934401
Ion Ratio	Lower	Upper	
82	100		
128	40.7	33.8	50.8
54	48.1	38.8	58.2

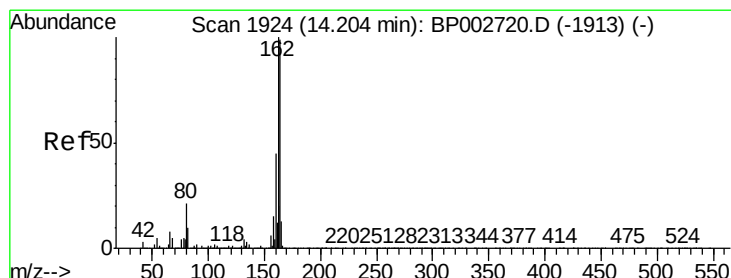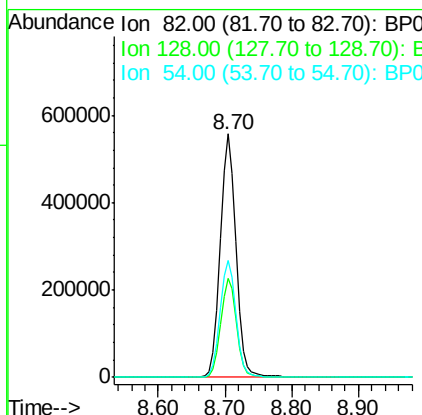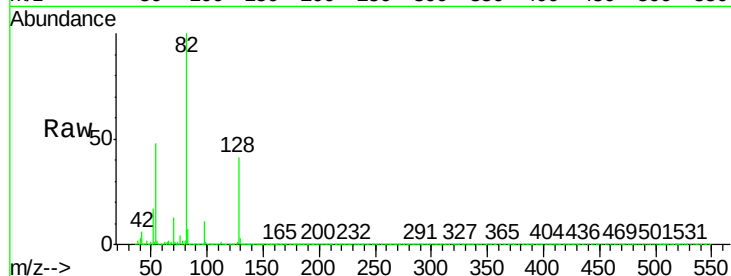

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.21 min Scan# 1925
 Delta R.T. 0.00 min
 Lab File: BP002778.D
 Acq: 16 Jul 2020 18:29

Tgt Ion	164	Resp	564694
Ion Ratio	Lower	Upper	
164	100		
162	99.9	80.6	121.0
160	45.6	36.4	54.6



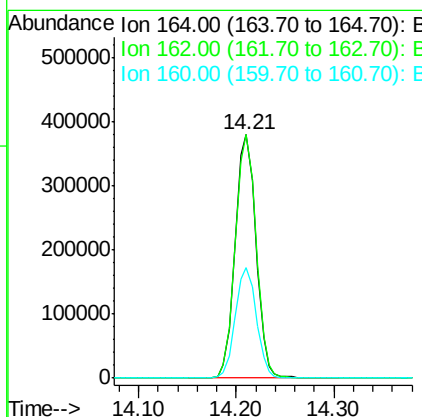
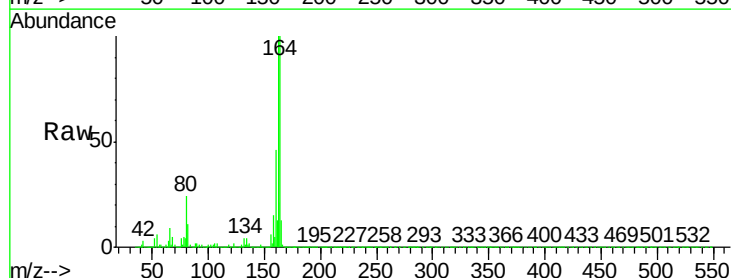


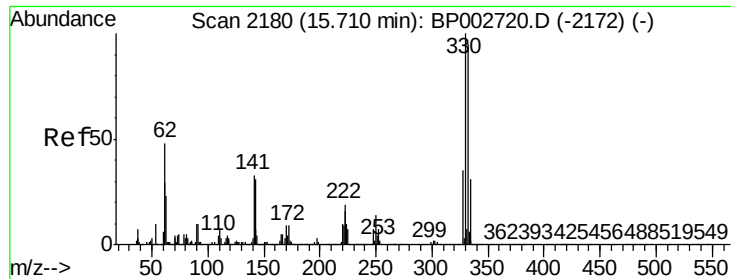

#42
2,4,6-Tribromophenol
Concen: 76.164 ng
RT: 15.72 min Scan# 2181
Delta R.T. 0.01 min
Lab File: BP002778.D
Acq: 16 Jul 2020 18:29




Instrument :
BNA_P
ClientSampleId :
8


Tot Ion:330 Resp: 448952
Ion Ratio Lower Upper
330 100
332 96.2 76.5 114.7
141 35.5 28.8 43.2

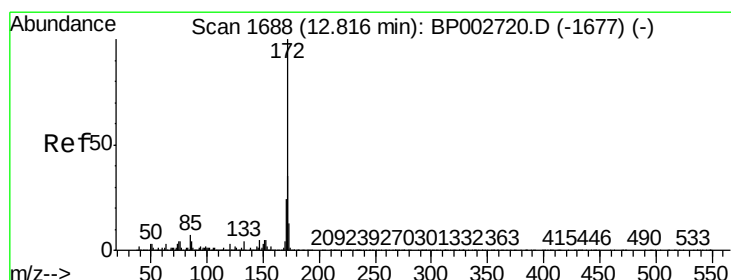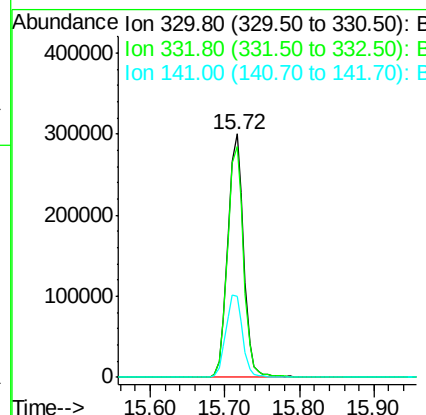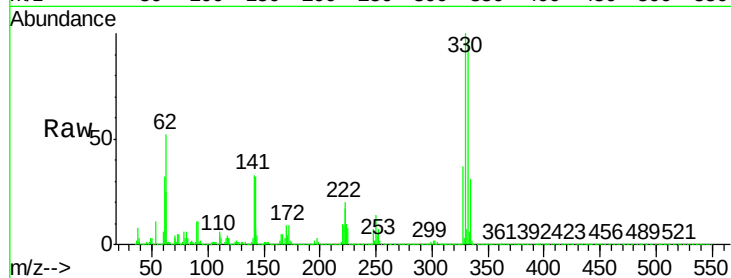

#45
2-Fluorobiphenyl
Concen: 48.846 ng
RT: 12.82 min Scan# 1689
Delta R.T. 0.00 min
Lab File: BP002778.D
Acq: 16 Jul 2020 18:29

Tgt Ion:172 Resp: 1783013
Ion Ratio Lower Upper
172 100
171 35.6 28.1 42.1
170 24.4 19.3 28.9

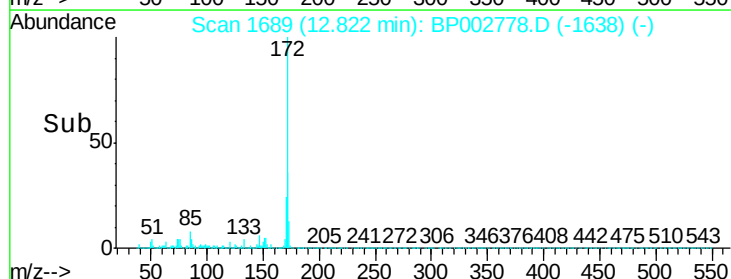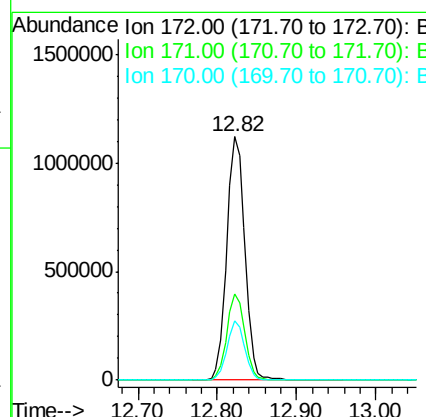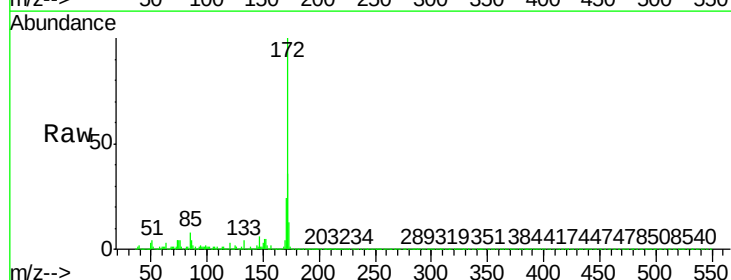



#50

Dimethylphthalate

Concen: 7.150 ng

RT: 13.67 min Scan# 1834

Delta R.T. 0.00 min

Lab File: BP002778.D

Acq: 16 Jul 2020 18:29

Instrument :

BNA_P

ClientSampleId :

8


Tot Ion:163 Resp: 307906

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2




164 9.6 7.8 11.8

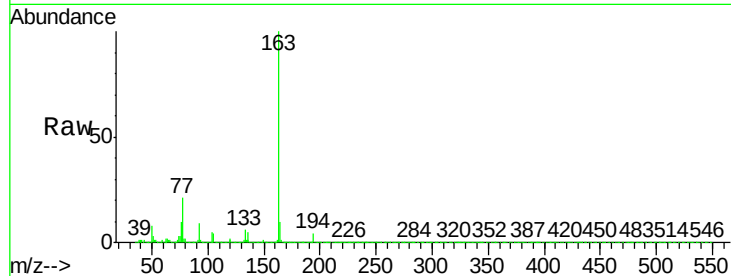

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

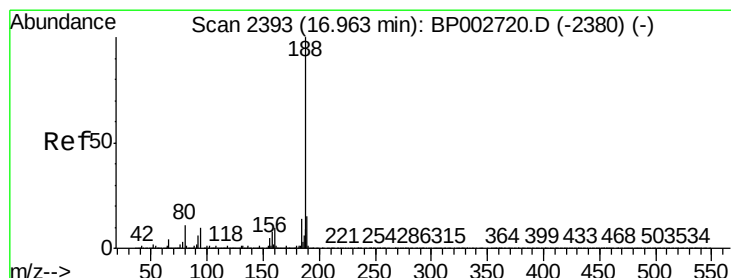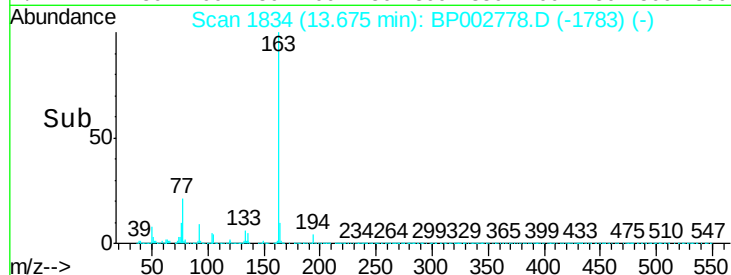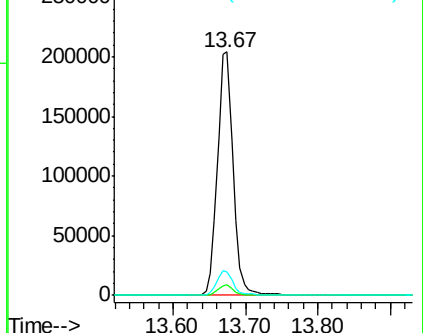

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 16.97 min Scan# 2394

Delta R.T. 0.00 min

Lab File: BP002778.D

Acq: 16 Jul 2020 18:29


Tgt Ion:188 Resp: 1072330

Ion Ratio Lower Upper

188 100

94 10.7 8.1 12.1



80 11.5 8.9 13.3

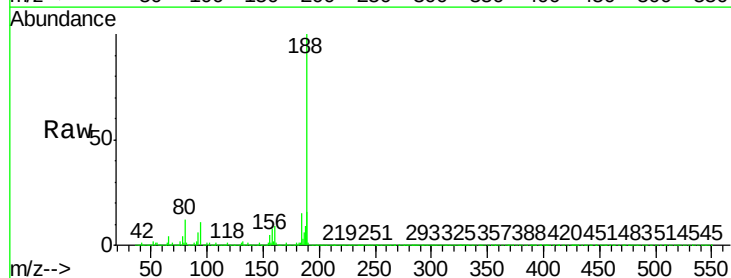


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BP0

Ion 80.00 (79.70 to 80.70): BP0



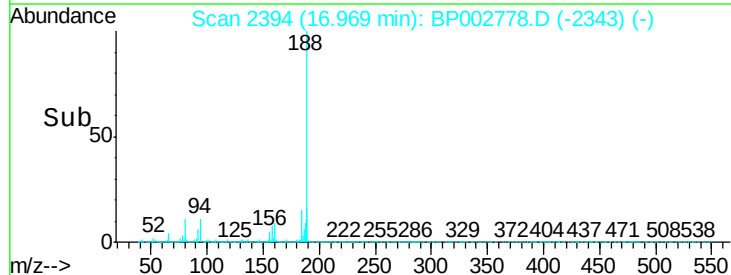
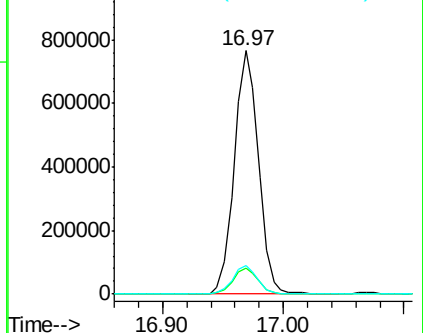


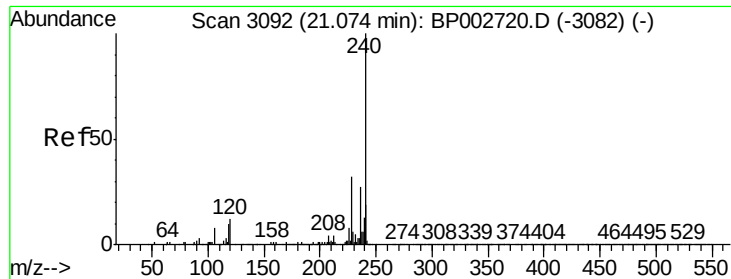

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.08 min Scan# 3093
Delta R.T. 0.01 min
Lab File: BP002778.D
Acq: 16 Jul 2020 18:29




Instrument :
BNA_P
ClientSampleId :
8


Tot Ion:240 Resp: 744019
Ion Ratio Lower Upper
240 100
120 10.6 9.4 14.2
236 24.7 21.3 31.9

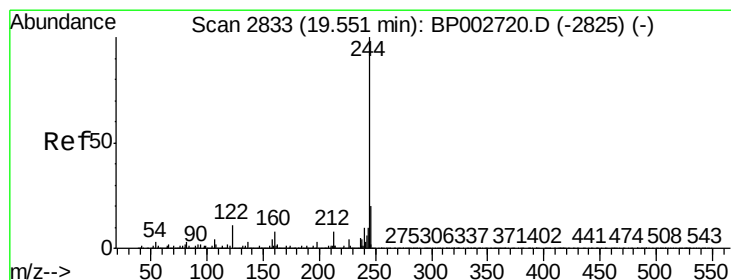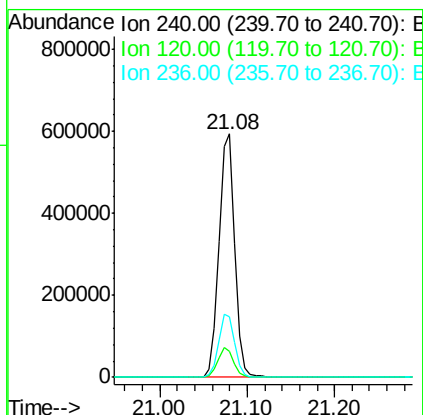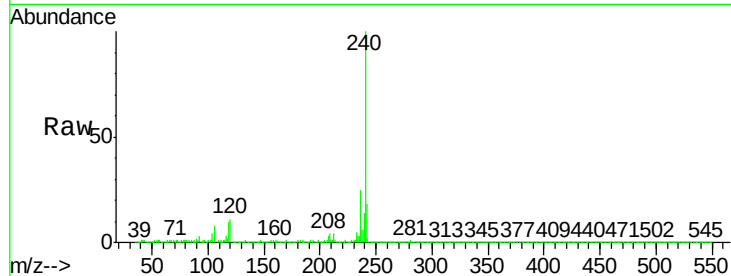

#79
Terphenyl-d14
Concen: 59.135 ng
RT: 19.56 min Scan# 2834
Delta R.T. 0.00 min
Lab File: BP002778.D
Acq: 16 Jul 2020 18:29

Tgt Ion:244 Resp: 1919011
Ion Ratio Lower Upper
244 100
212 8.0 6.0 9.0
122 11.5 8.9 13.3

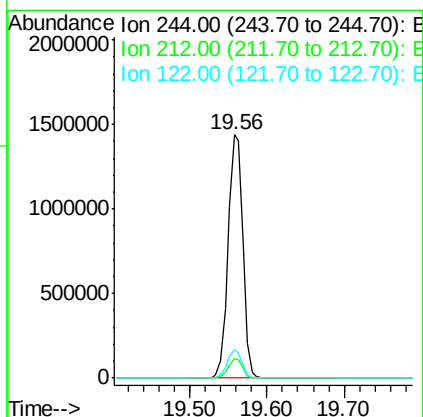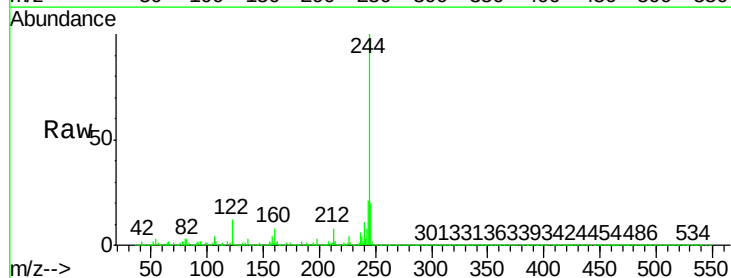




#86
Pervlene-d12
Concen: 20.000 ng
RT: 23.27 min Scan# 3465
Delta R.T. 0.01 min
Lab File: BP002778.D
Acq: 16 Jul 2020 18:29

Instrument :
BNA_P
ClientSampleId :
8

Tot Ion	Ratio	Lower	Upper
264	100		
260	25.4	19.3	28.9
265	22.4	16.8	25.2

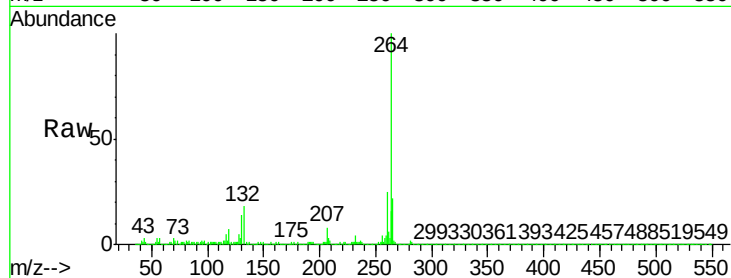

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

