


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071620\
 Data File : BP002767.D
 Acq On : 16 Jul 2020 11:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP071020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 13 10:54:03 2020

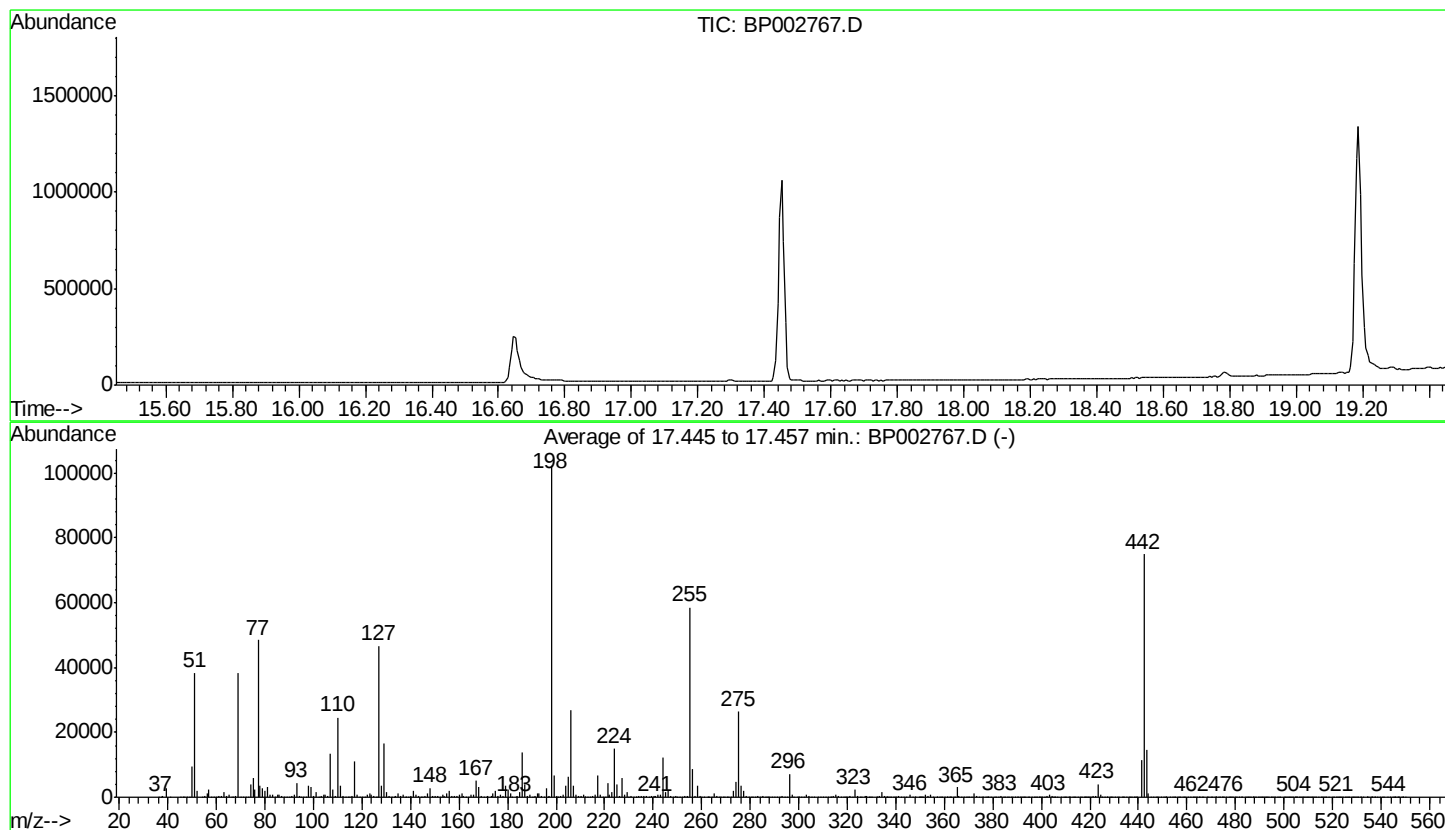

AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	38375	PASS
68	69	0.00	2	1.5	572	PASS
69	198	0.00	100	37.6	38472	PASS
70	69	0.00	2	0.5	176	PASS
127	198	10	80	45.6	46663	PASS
197	198	0.00	2	0.4	460	PASS
198	198	100	100	100.0	102271	PASS
199	198	5	9	6.7	6824	PASS
275	198	10	60	25.7	26301	PASS
365	198	1	100	3.1	3133	PASS
441	198	0.01	100	11.2	11502	PASS
442	198	50	100	73.3	74945	PASS
443	442	15	24	19.3	14452	PASS