
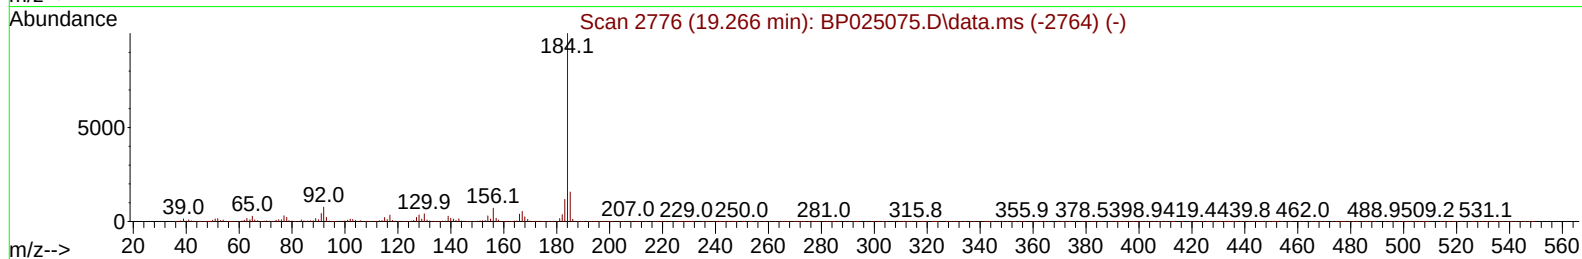
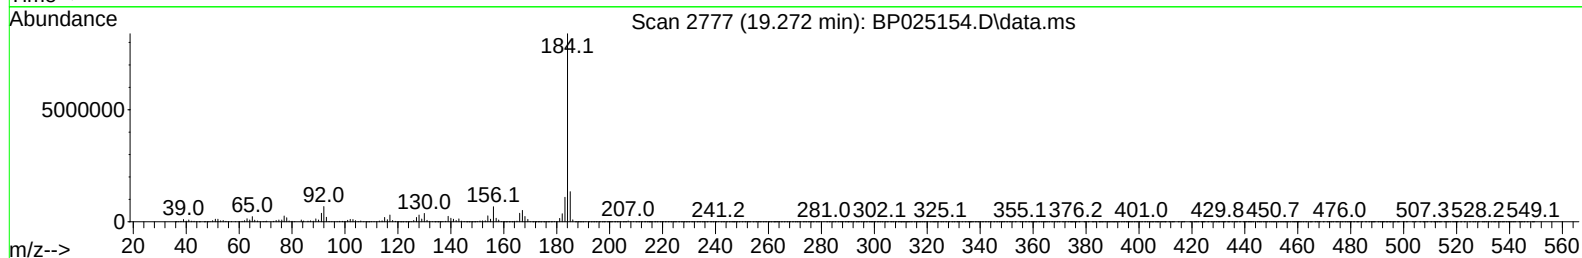


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071625\
Data File : BP025154.D
Acq On : 16 Jul 2025 11:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 14:37:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

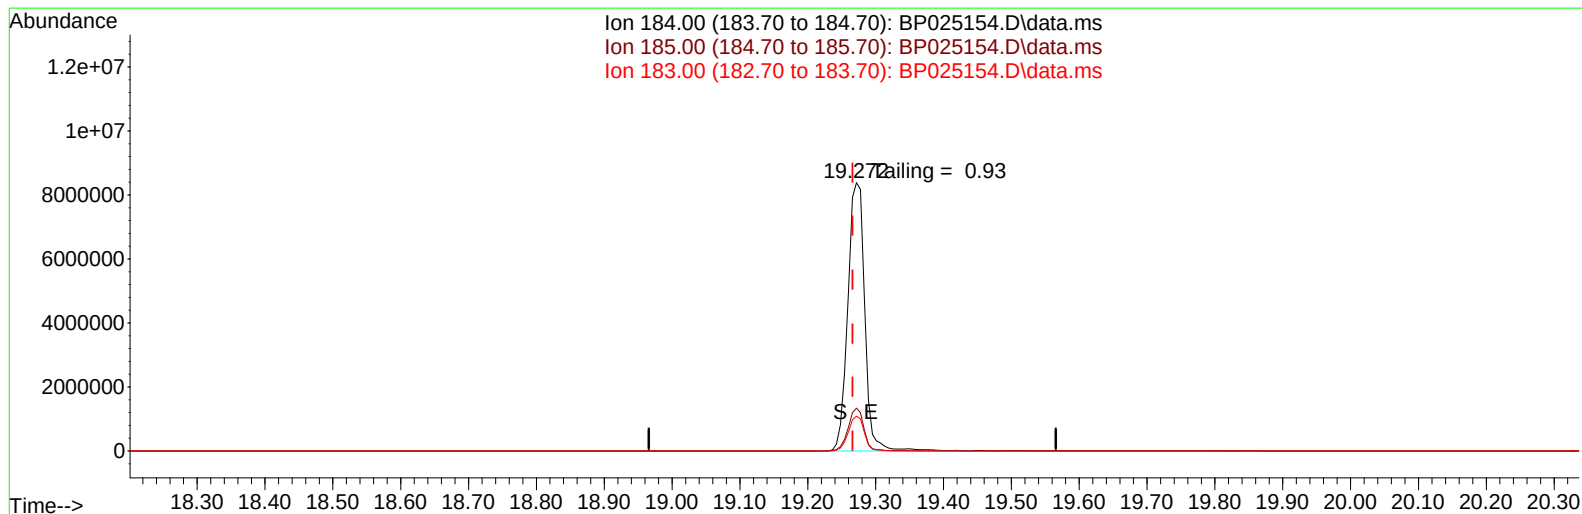




TIC: BP025154.D\data.ms

(77) Benzidine**19.272min (+ 0.006) 56461.29 ng****response 14377417**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	16.02
183.00	11.80	13.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071625\
Data File : BP025154.D
Acq On : 16 Jul 2025 11:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 16 14:37:58 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

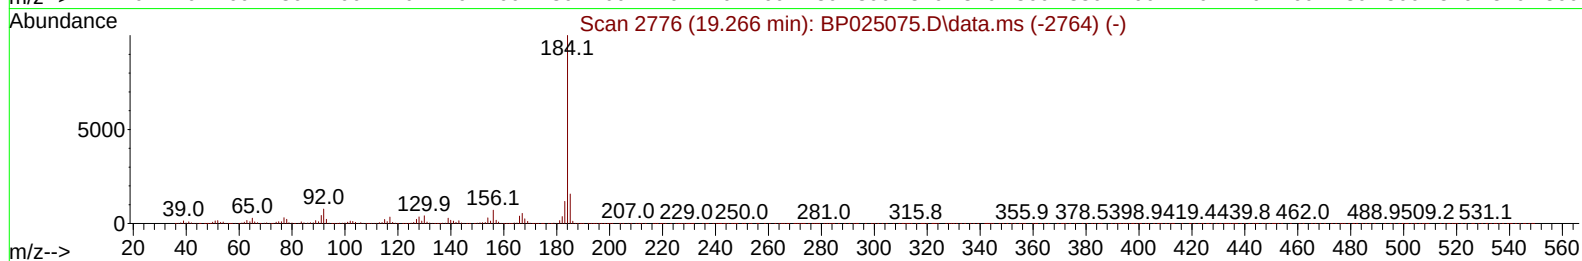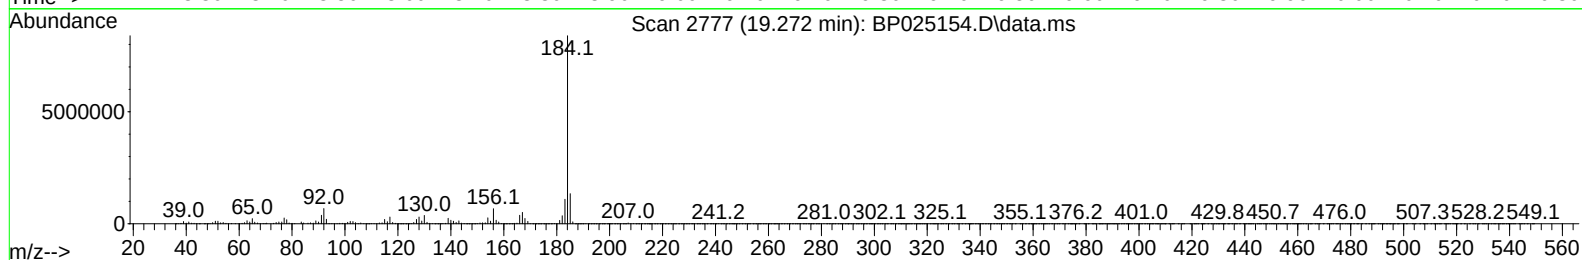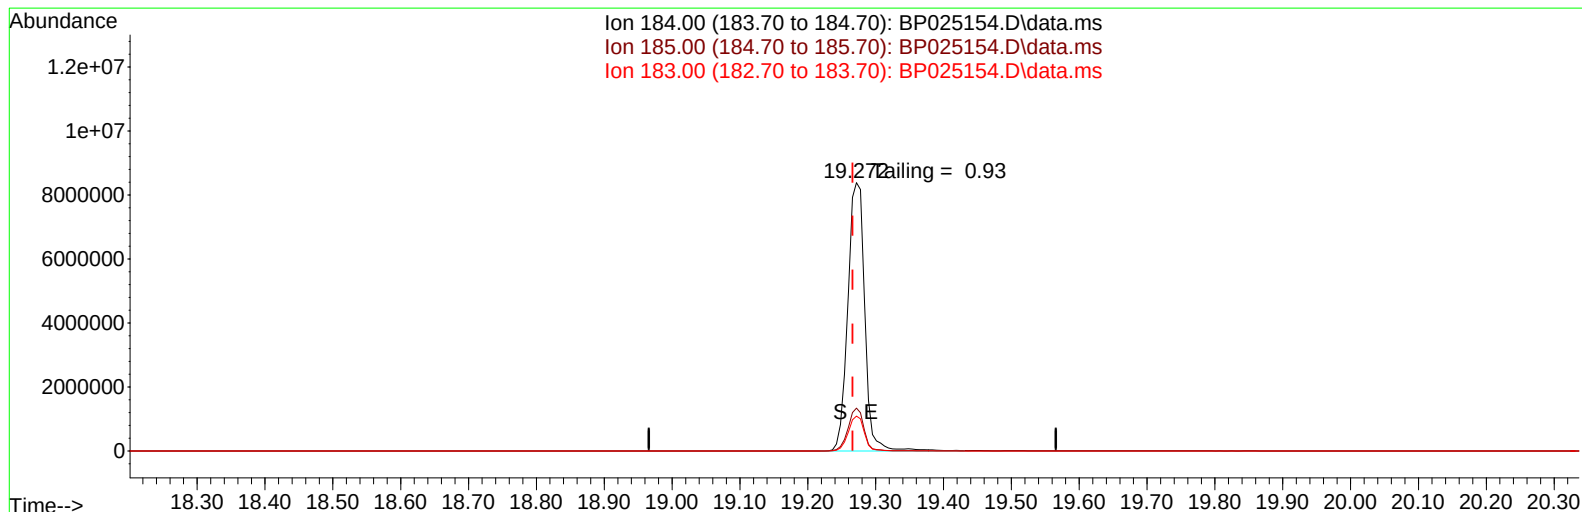

TIC: BP025154.D\data.ms

(77) Benzidine**19.272min (+ 0.006) 56461.29 ng****response 14377417**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	16.02
183.00	11.80	13.02
0.00	0.00	0.00