
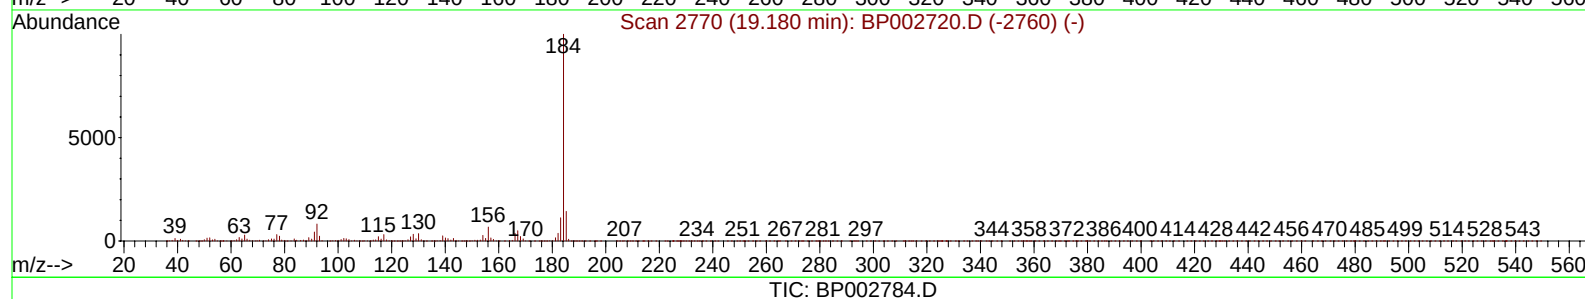
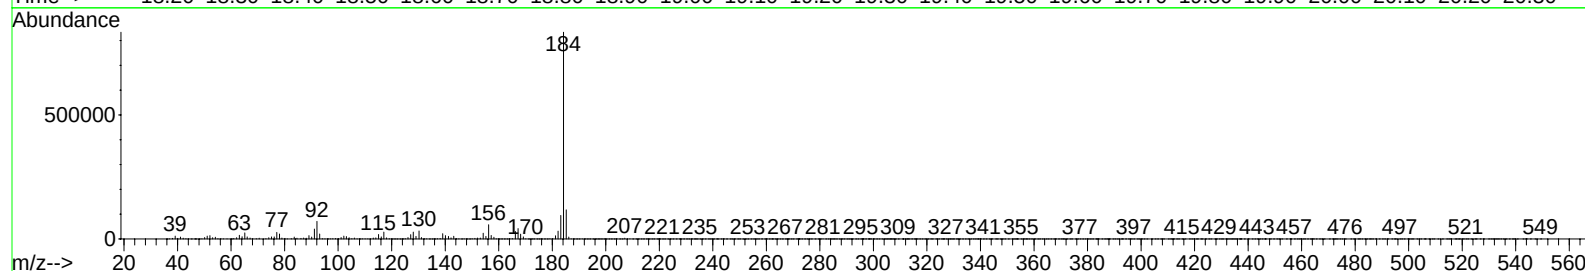


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP071720\
Data File : BP002784.D
Acq On : 17 Jul 2020 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 17 13:28:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 13 10:54:03 2020
Response via : Initial Calibration

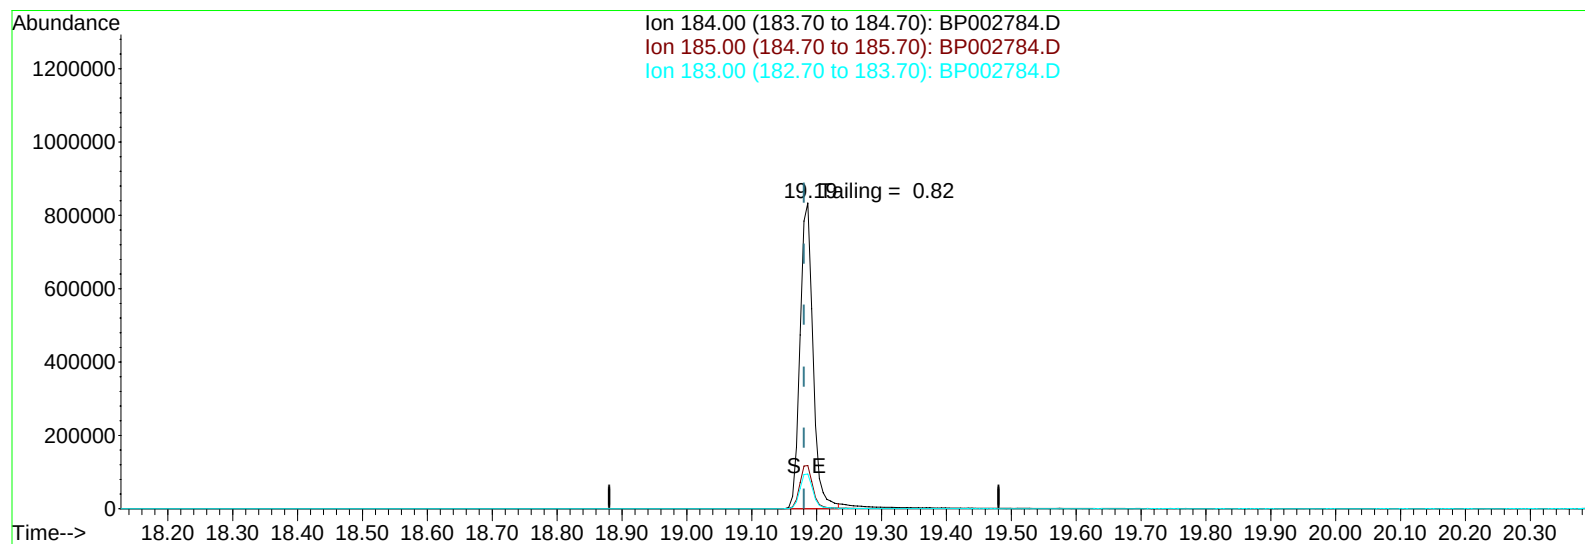

(77) Benzidine




19.186min (+0.006) 62829.09ng

response 1197594

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	14.13
183.00	11.20	11.35
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP071720\
Data File : BP002784.D
Acq On : 17 Jul 2020 09:18
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 17 13:28:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 13 10:54:03 2020
Response via : Initial Calibration

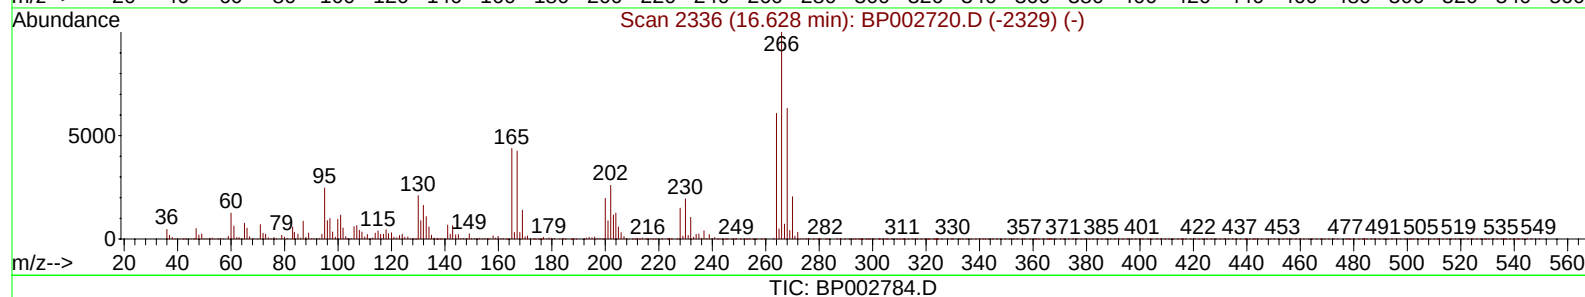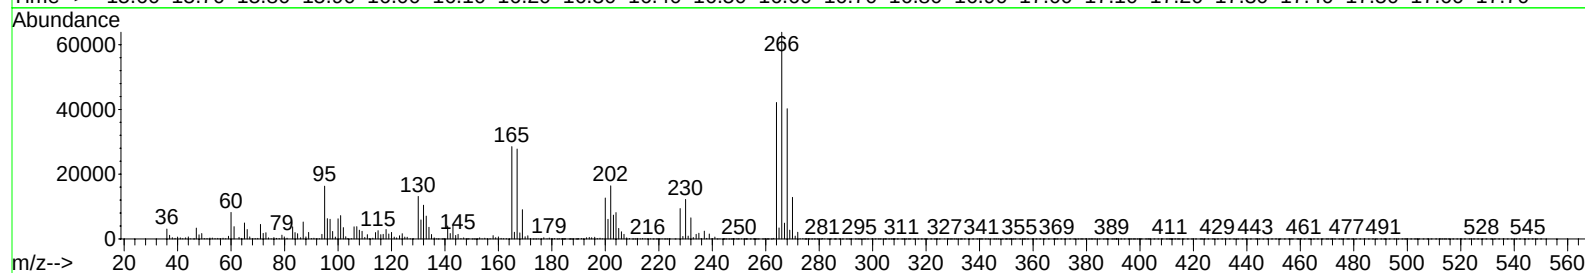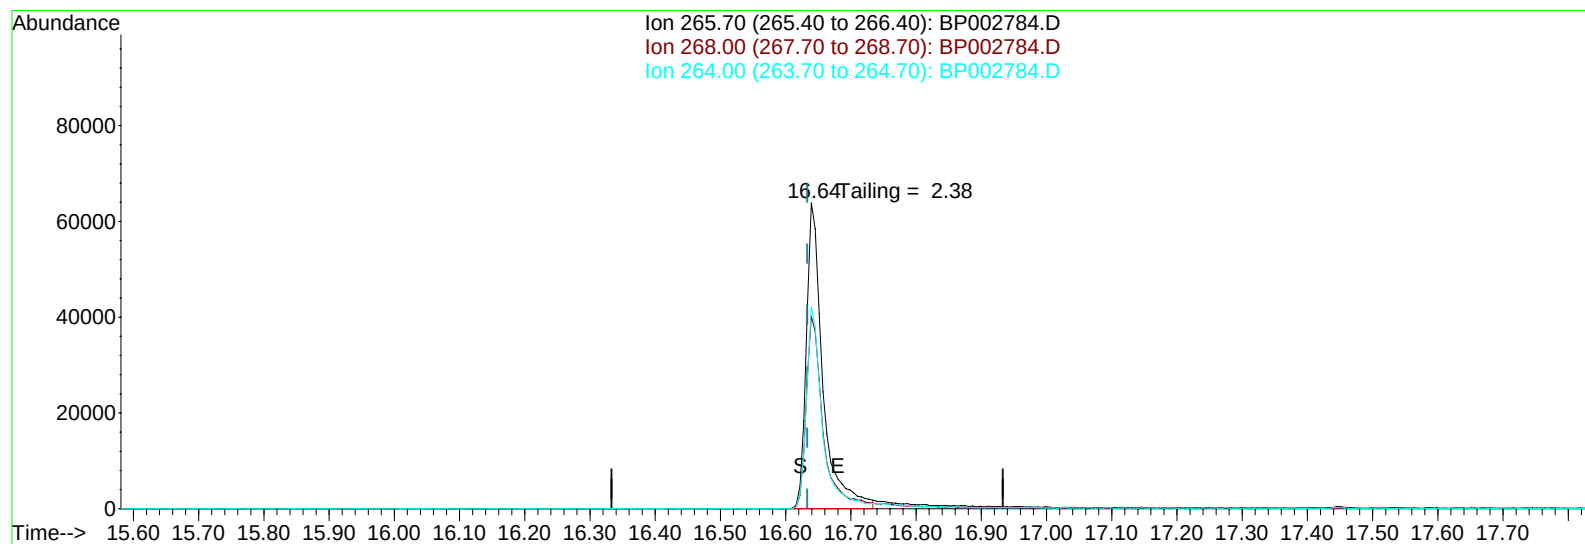

(70) Pentachlorophenol (C)

16.640min (+0.006) 43232.48ng

response 119045

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	63.01
264.00	60.70	66.05
0.00	0.00	0.00