
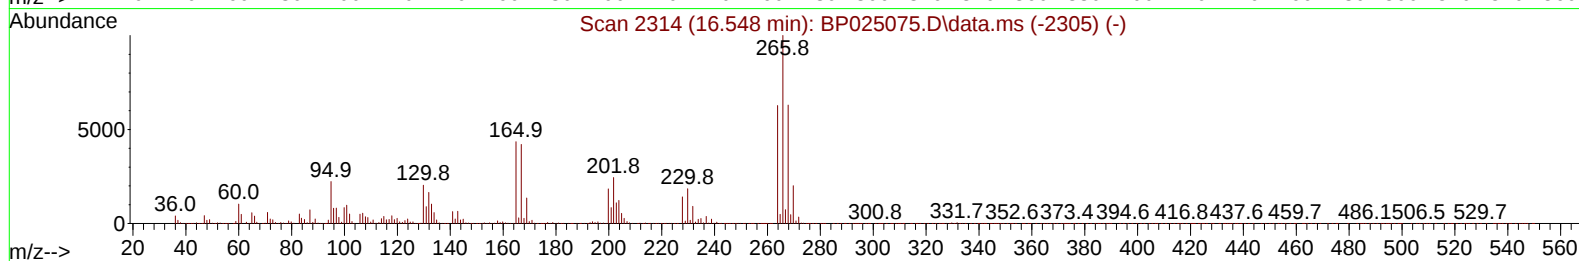
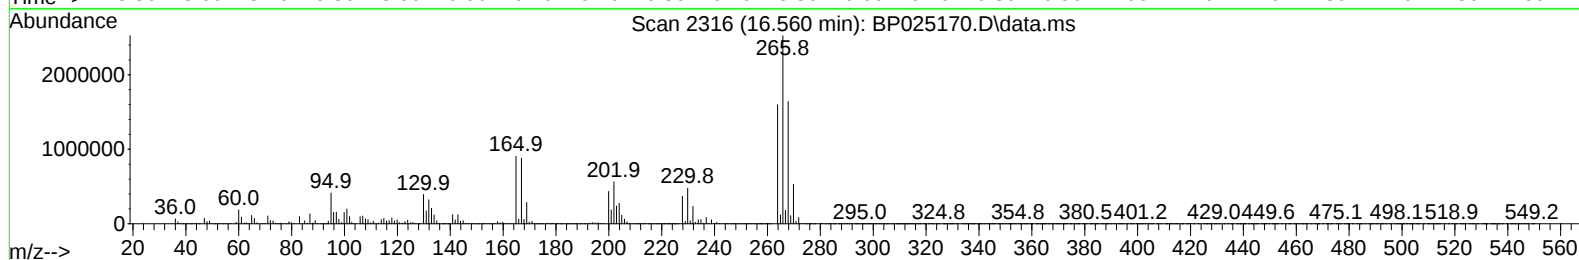


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071725\
Data File : BP025170.D
Acq On : 17 Jul 2025 09:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 17 12:10:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

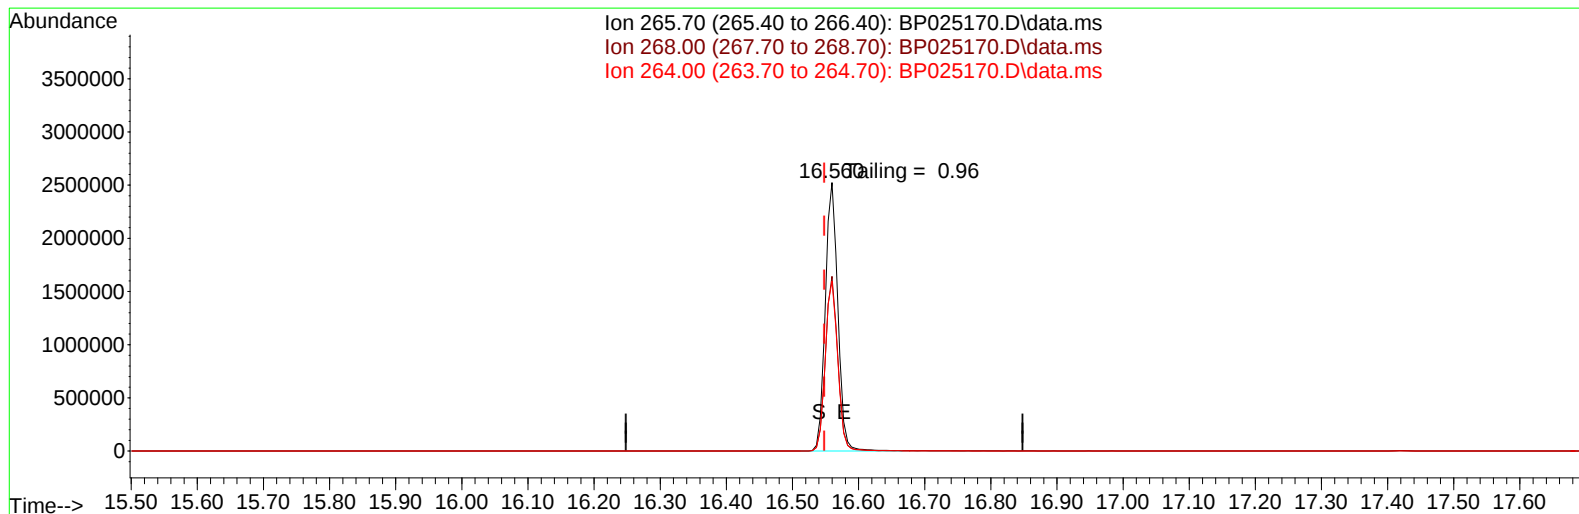

TIC: BP025170.D\data.ms

(70) Pentachlorophenol (C)




16.560min (+ 0.012) 71796.13 ng

response 3339294

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	65.06
264.00	62.70	63.28
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071725\  
Data File : BP025170.D  
Acq On    : 17 Jul 2025  09:23  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Jul 17 12:10:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

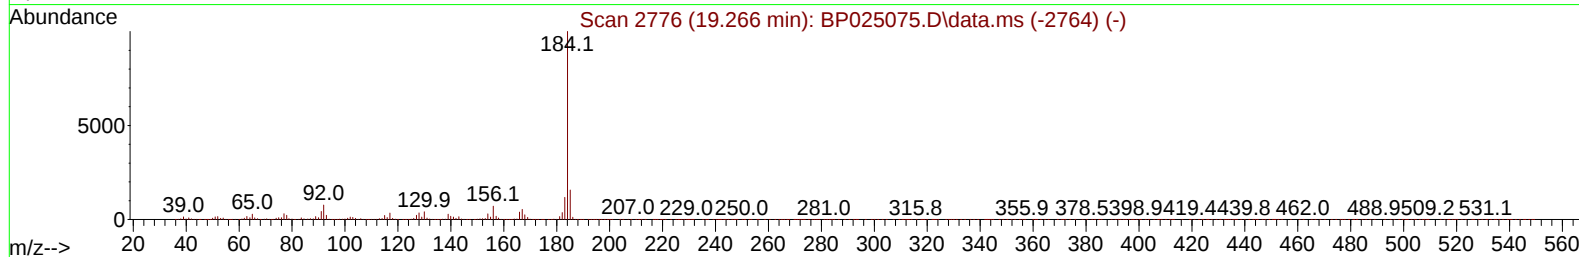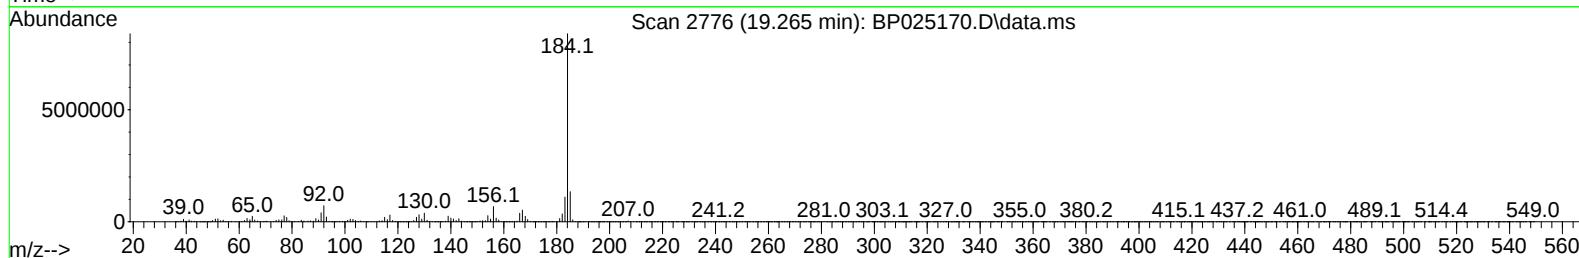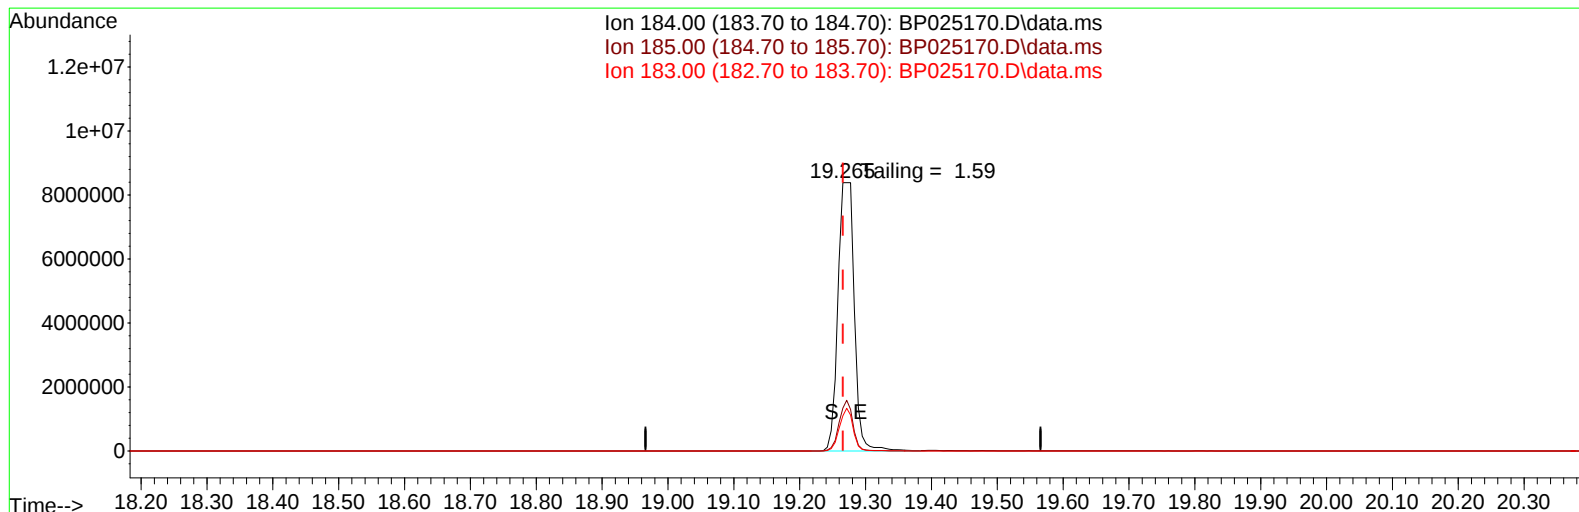

TIC: BP025170.D\data.ms

(77) Benzidine

19.265min (-0.001) 52959.79 ng

response **14593235**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	16.00
183.00	11.80	13.13
0.00	0.00	0.00