
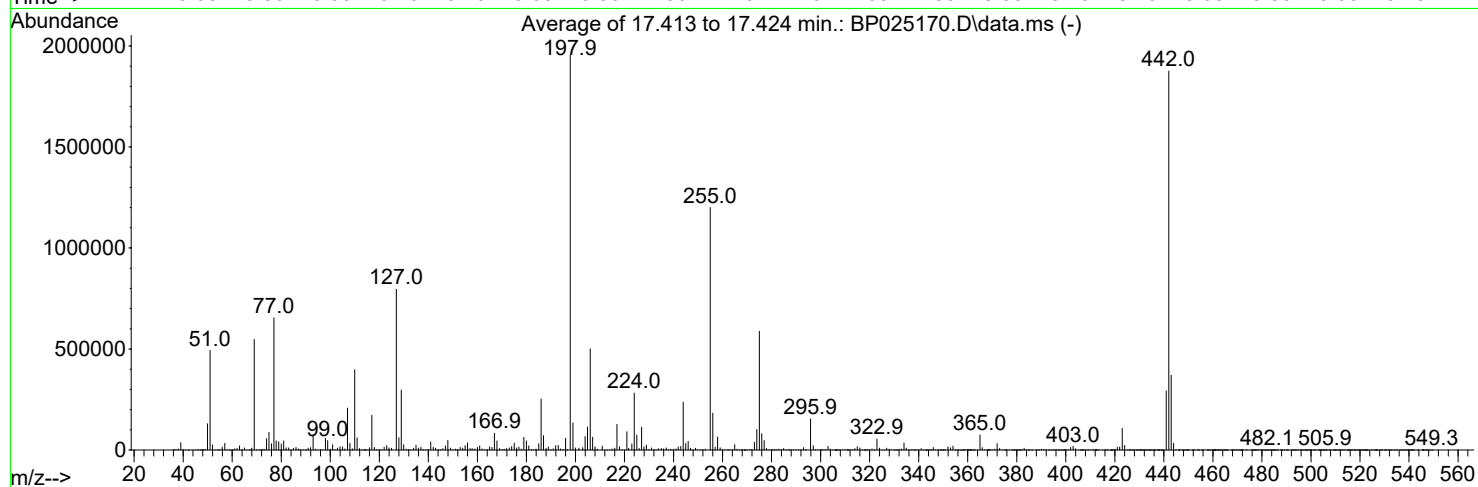


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071725\
Data File : BP025170.D
Acq On : 17 Jul 2025 09:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 03 16:05:44 2025

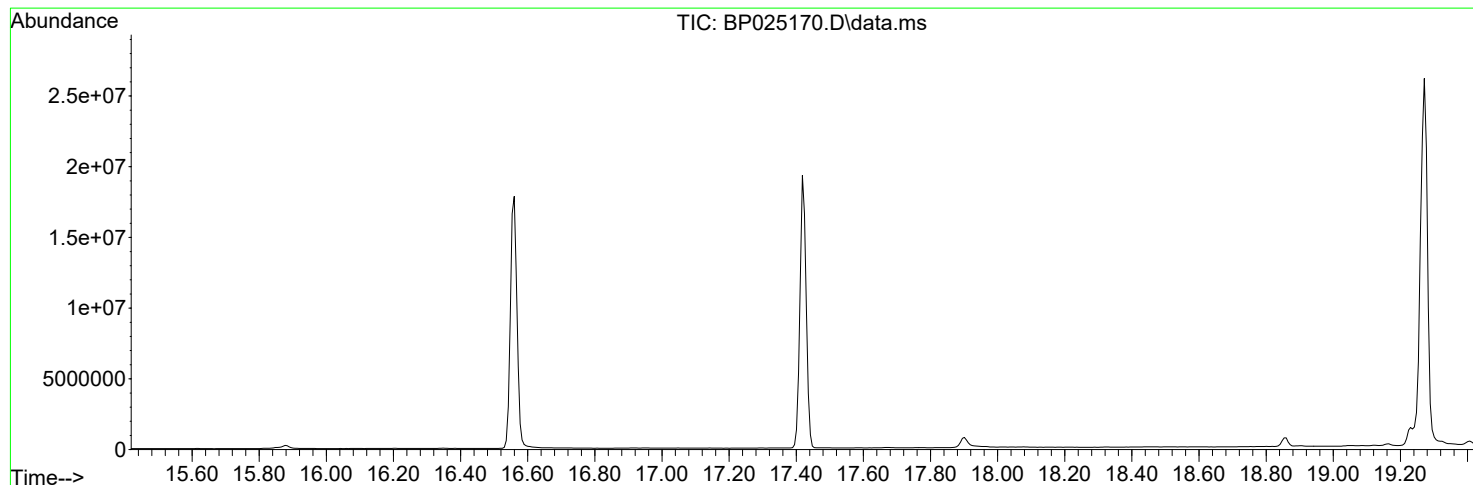

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2450

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	9463	PASS
69	69	100	100	100.0	547036	PASS
70	69	0.00	2	0.5	2642	PASS
197	198	0.00	2	0.1	2625	PASS
198	198	100	100	100.0	1954556	PASS
199	198	5	9	6.9	134189	PASS
365	198	1	100	3.8	74755	PASS
441	443	0.01	150	79.4	293480	PASS
442	442	100	100	100.0	1875797	PASS
443	442	15	24	19.7	369692	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/17/2025	BNA_P	<u>BP025170.D</u>
Compound Name	Response	Retention Time
DDT	7685363	20.583
DDD	198265	20.118
DDE	8633	19.589
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
206898	7892261	2.62

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071725\
Data File : BP025170.D
Acq On : 17 Jul 2025 09:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 17 12:10:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

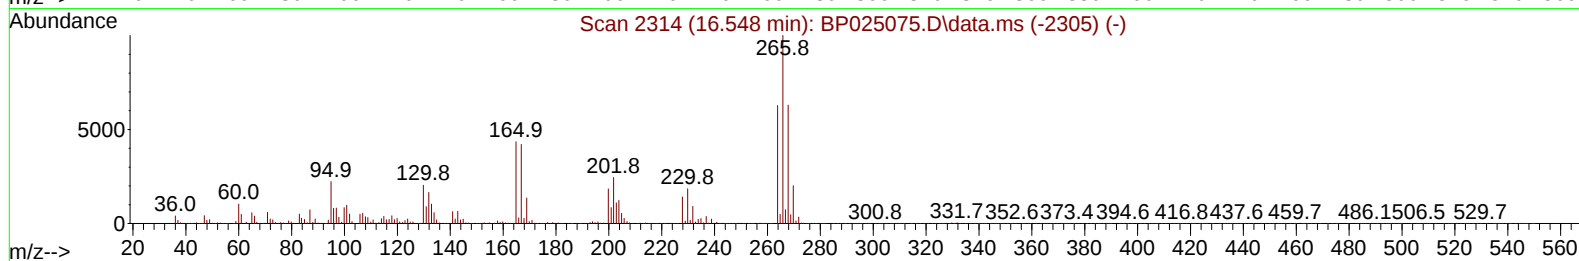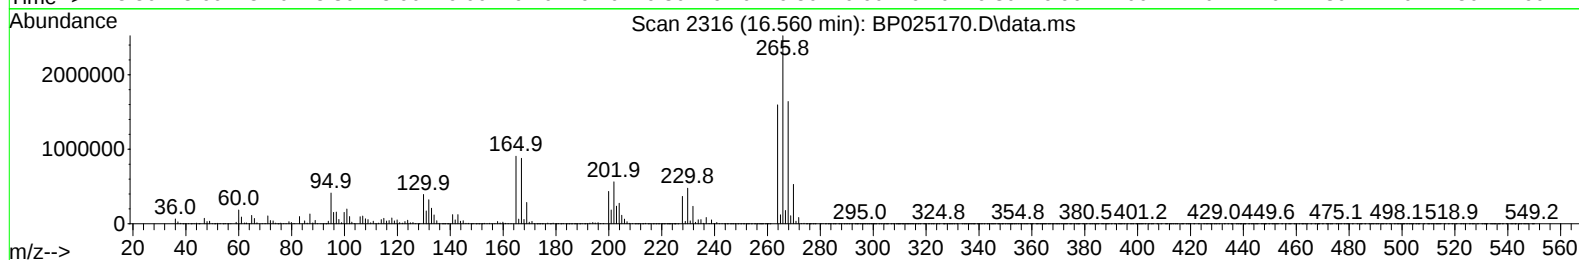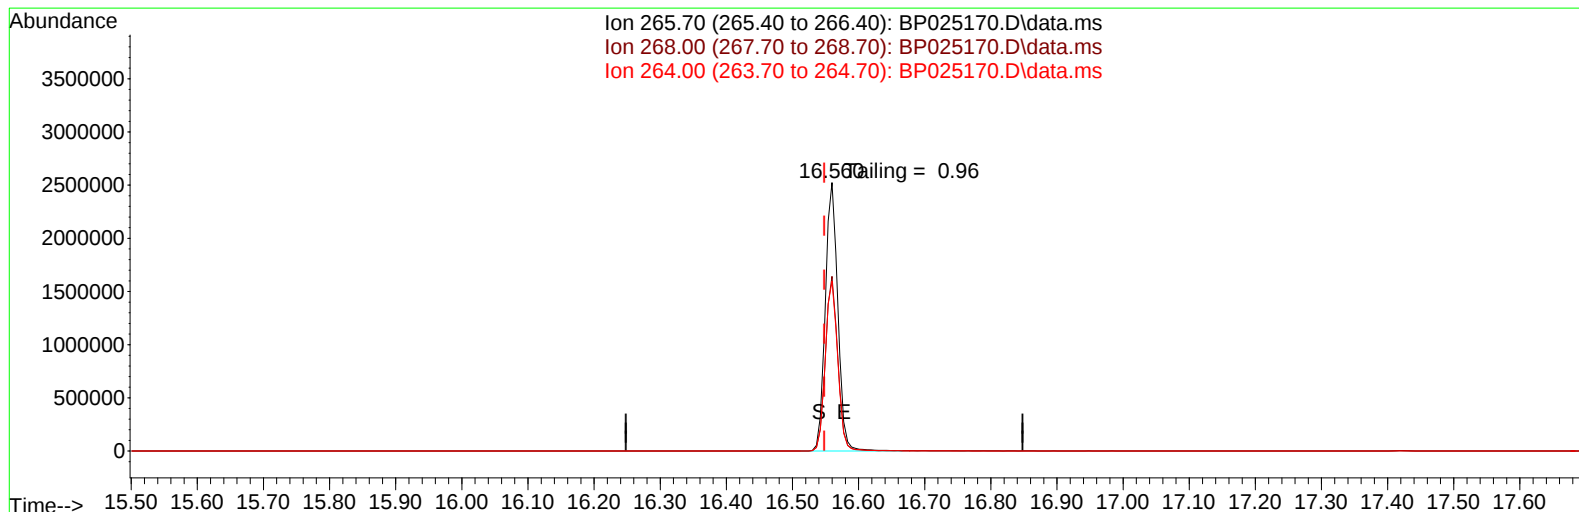

TIC: BP025170.D\data.ms

(70) Pentachlorophenol (C)

16.560min (+ 0.012) 71796.13 ng




response 3339294

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	65.06
264.00	62.70	63.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071725\
Data File : BP025170.D
Acq On : 17 Jul 2025 09:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 17 12:10:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP070325.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 03 16:05:44 2025
Response via : Initial Calibration

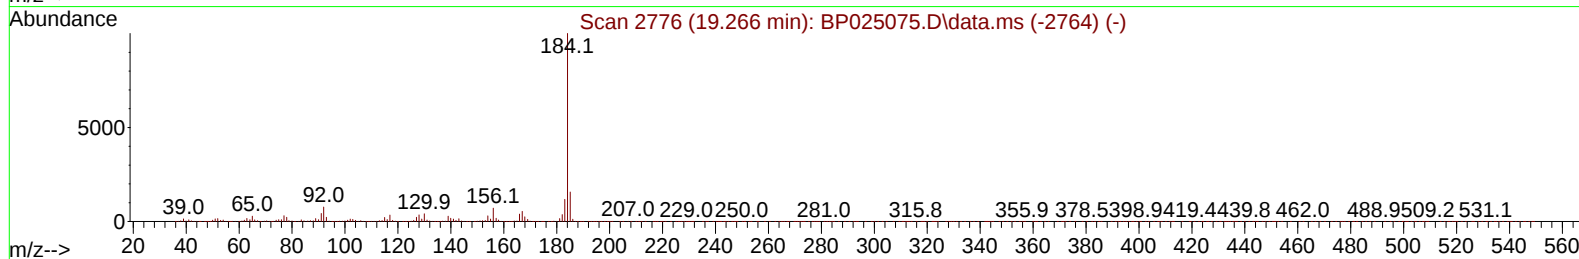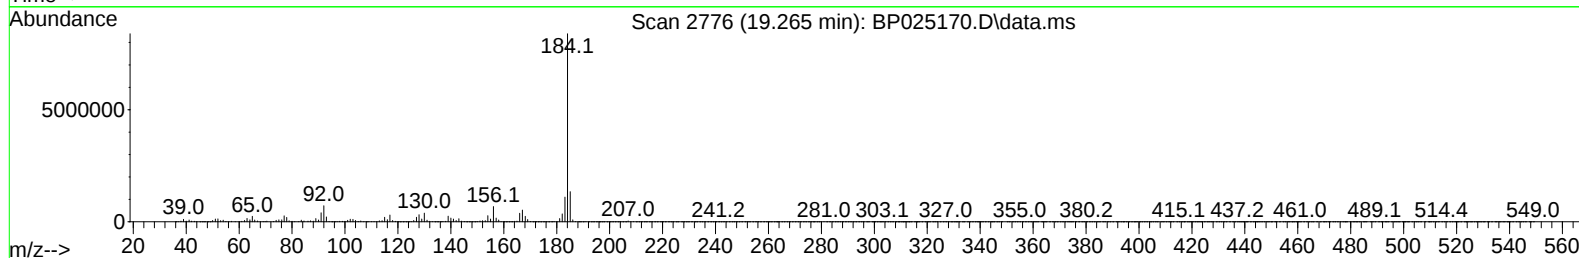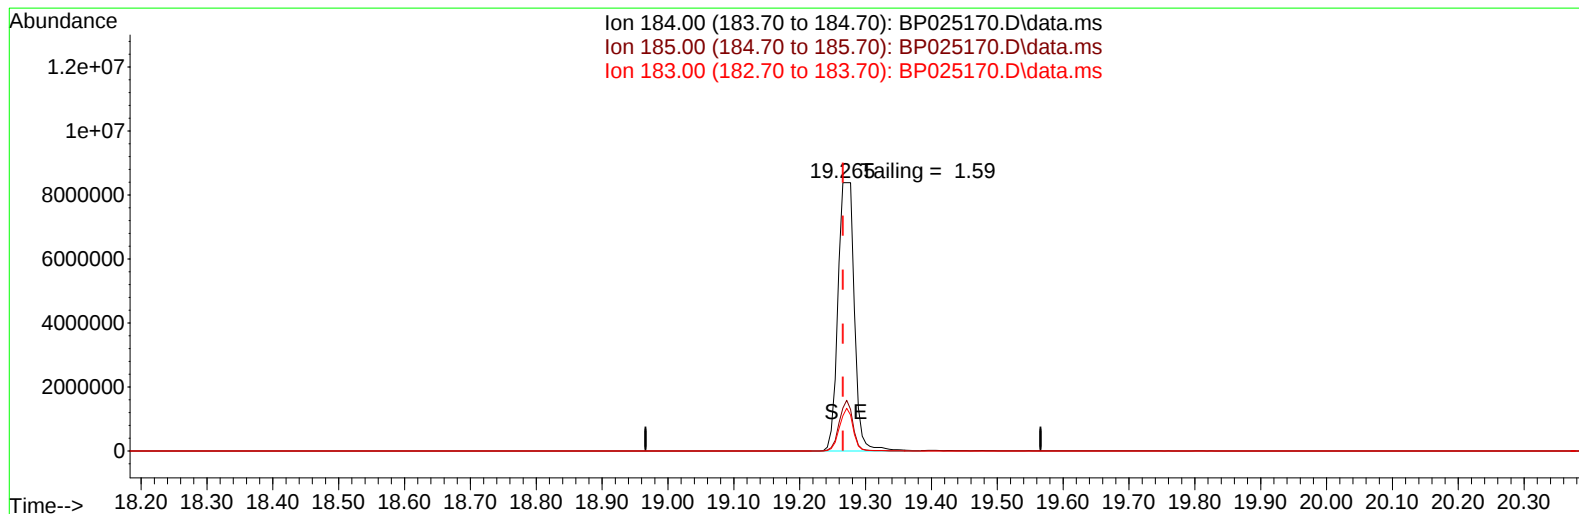

TIC: BP025170.D\data.ms

(77) Benzidine

19.265min (-0.001) 52959.79 ng

response 14593235

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	16.00
183.00	11.80	13.13
0.00	0.00	0.00