




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011035.D
Acq On : 19 Jul 2022 16:41
Operator : CG/JU
Sample : N3753-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHP9

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:40:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 19 03:25:54 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/20/2022
Supervised By :mohammad ahmed 07/21/2022

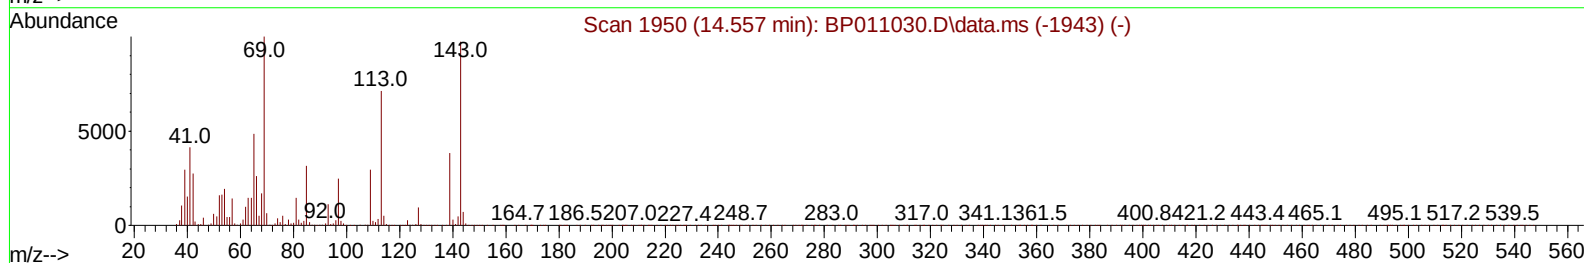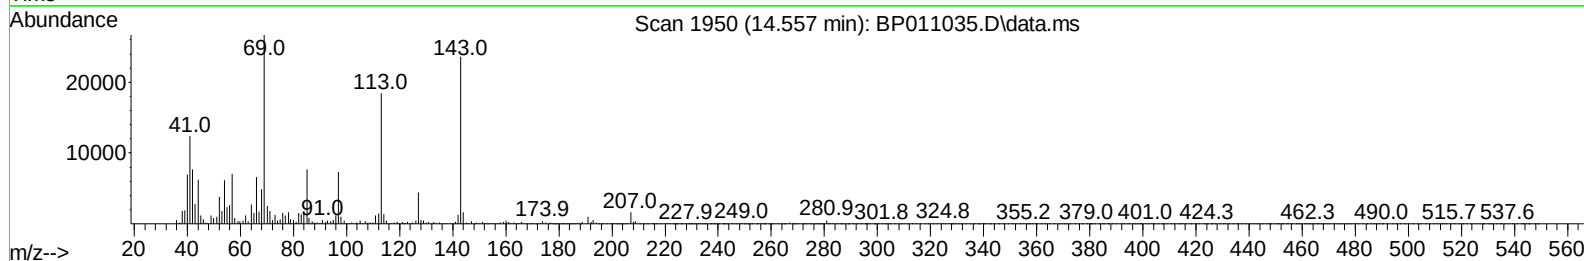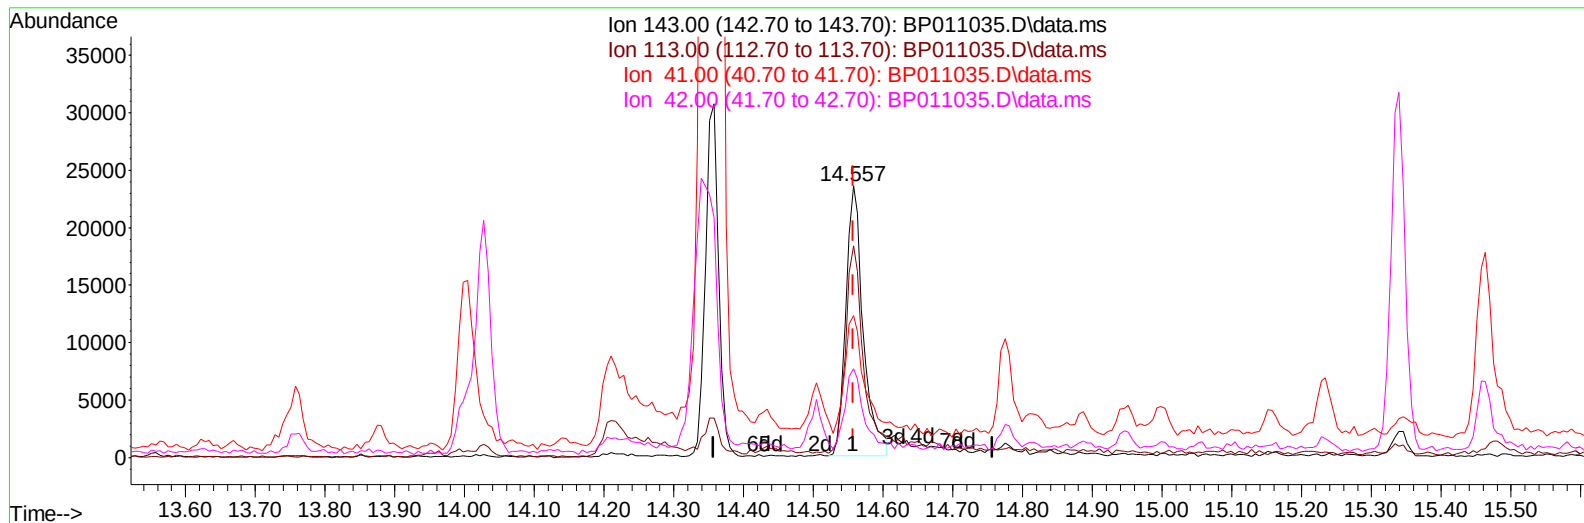

TIC: BP011035.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.557min (-0.000) 3.88 ng/u1

response 41043

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.50	77.94
41.00	59.00	52.22
42.00	41.10	32.68#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011035.D
Acq On : 19 Jul 2022 16:41
Operator : CG/JU
Sample : N3753-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHP9

Manual IntegrationsAPPROVED

Quant Time: Jul 19 23:40:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 19 03:25:54 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/20/2022
Supervised By :mohammad ahmed 07/21/2022

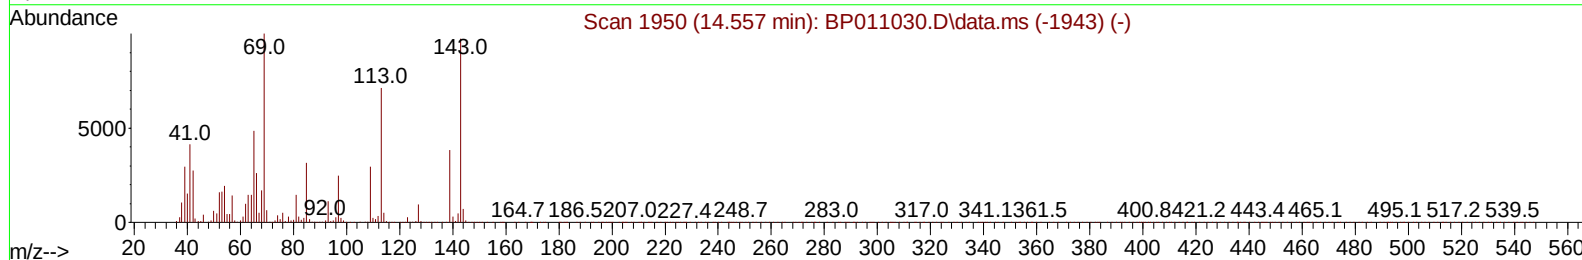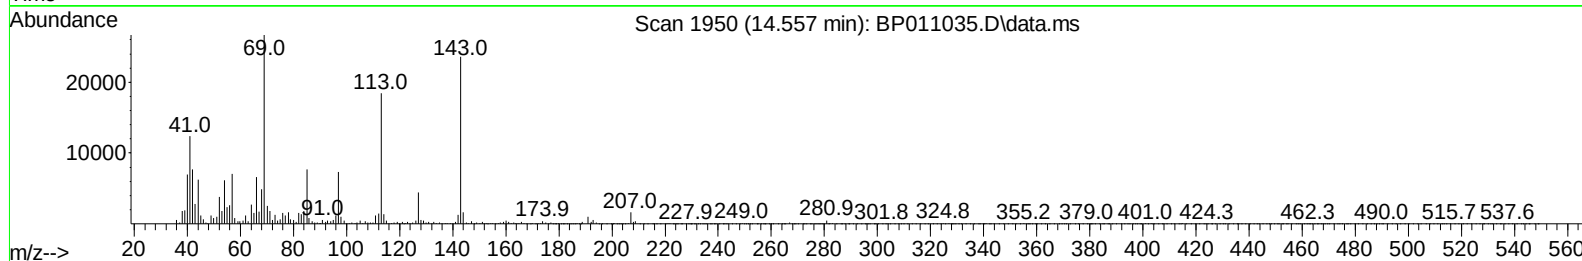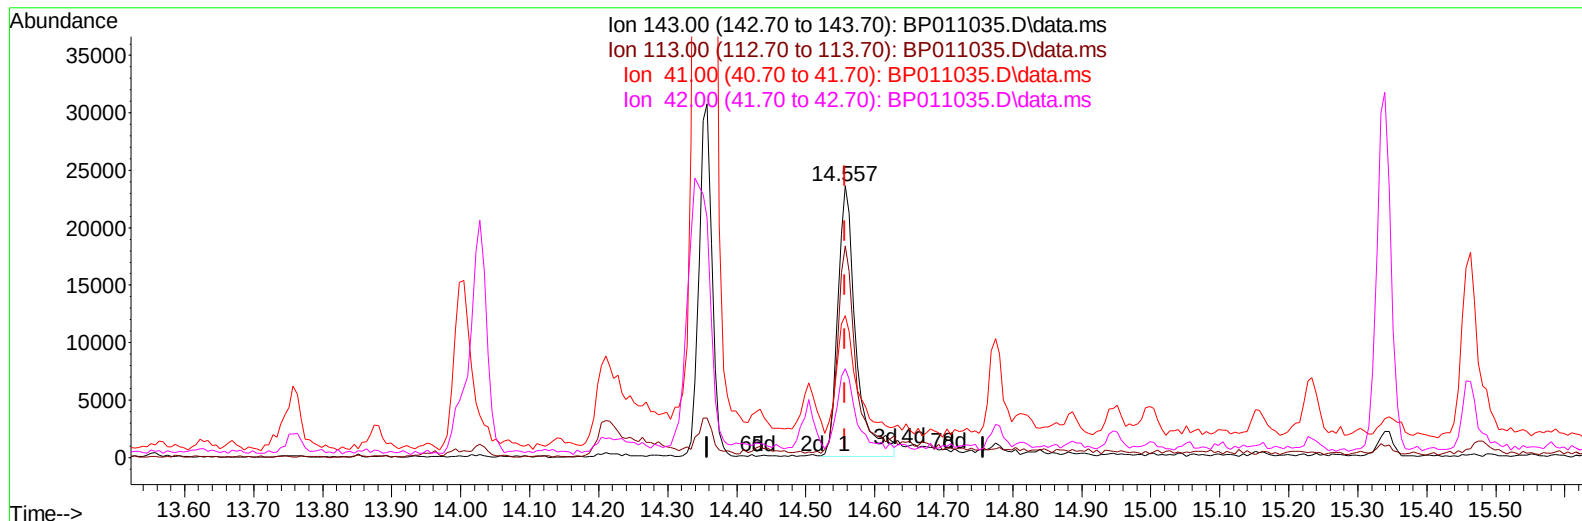

TIC: BP011035.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.557min (-0.000) 4.10 ng/ul m

response 43368

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.50	77.94
41.00	59.00	52.22
42.00	41.10	32.68#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
 Data File : BP011035.D
 Acq On : 19 Jul 2022 16:41
 Operator : CG/JU
 Sample : N3753-08
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHP9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/20/2022
 Supervised By :mohammad ahmed 07/21/2022

Quant Time: Jul 19 23:40:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 19 03:25:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.675	152	332736	20.000	ng/ul	0.00
20) Naphthalene-d8	10.469	136	1314766	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.340	164	764242	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.104	188	1459954	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.227	240	1469936	20.000	ng/ul	# 0.00
88) Perylene-d12	23.580	264	1497439	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	42548	4.610	ng/uL	0.00
4) Pyridine-d5	3.599	84	179949	7.543	ng/ul	0.00
7) Phenol-d5	6.858	99	160751	5.885	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.022	67	542089	30.865	ng/ul	0.00
11) 2-Chlorophenol-d4	7.210	132	512955	23.242	ng/ul	0.00
15) 4-Methylphenol-d8	8.393	113	301991	13.811	ng/ul	0.00
21) Nitrobenzene-d5	8.840	128	310437	32.400	ng/ul	0.00
24) 2-Nitrophenol-d4	9.557	143	281978	29.742	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.093	165	498203	28.734	ng/ul	0.00
31) 4-Chloroaniline-d4	10.616	131	517474	18.104	ng/ul	0.00
46) Dimethylphthalate-d6	13.757	166	1788357	34.238	ng/ul	0.00
49) Acenaphthylene-d8	14.028	160	2113823	34.299	ng/ul	0.00
54) 4-Nitrophenol-d4	14.557	143	43368m	4.102	ng/ul	0.00
60) Fluorene-d10	15.339	176	1504404	33.884	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.463	200	190232	26.332	ng/ul	0.00
73) Anthracene-d10	17.204	188	2451543	39.499	ng/ul	0.00
81) Pyrene-d10	19.463	212	2972680	38.506	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.433	264	2979053	41.421	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011035.D
Acq On : 19 Jul 2022 16:41
Operator : CG/JU
Sample : N3753-08
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHP9

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/20/2022
Supervised By :mohammad ahmed 07/21/2022

Quant Time: Jul 19 23:40:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 19 03:25:54 2022
Response via : Initial Calibration

