

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
 Data File : BP011031.D
 Acq On : 19 Jul 2022 14:23
 Operator : CG/JU
 Sample : PB146296BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK296

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011031.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	22	rVB	134835	180922	2.44%	0.214%
2	3.587	82	85	104	rBV	1492602	2216490	29.86%	2.623%
3	3.899	134	138	145	rVB	35331	54695	0.74%	0.065%
4	6.858	634	641	651	rBV	1604619	2425442	32.68%	2.870%
5	7.022	663	669	681	rVB	1379983	2095148	28.23%	2.479%
6	7.211	694	701	713	rBV	1684137	2584604	34.82%	3.058%
7	7.675	774	780	788	rBV	1378204	2148973	28.95%	2.543%
8	8.393	895	902	919	rBV	1947851	2985076	40.22%	3.532%
9	8.840	970	978	986	rBV	1469249	2359483	31.79%	2.792%
10	9.558	1092	1100	1111	rBV	1131967	1806780	24.34%	2.138%
11	10.093	1184	1191	1202	rBV	1736195	2777331	37.42%	3.286%
12	10.469	1248	1255	1264	rVB	1829976	2957756	39.85%	3.500%
13	10.616	1271	1280	1295	rBV	1844048	3081296	41.51%	3.646%
14	12.069	1521	1527	1536	rBV	33137	61988	0.84%	0.073%
15	12.287	1558	1564	1571	rVB	4579	8502	0.11%	0.010%
16	13.304	1730	1737	1742	rBV6	7527	11635	0.16%	0.014%
17	13.757	1807	1814	1826	rBV	2950468	4106916	55.33%	4.860%
18	14.028	1852	1860	1874	rBV	3435927	4929237	66.41%	5.833%
19	14.340	1906	1913	1921	rBV	2570539	3618931	48.75%	4.282%
20	14.557	1943	1950	1969	rBV	996882	1839583	24.78%	2.177%
21	14.987	2019	2023	2031	rVB	5331	9421	0.13%	0.011%
22	15.340	2076	2083	2091	rBV	4326928	6059854	81.64%	7.170%
23	15.463	2098	2104	2115	rBV	1131106	1545487	20.82%	1.829%
24	15.581	2120	2124	2129	rVB	53763	76728	1.03%	0.091%
25	16.134	2213	2218	2225	rVB8	16635	24802	0.33%	0.029%
26	16.240	2232	2236	2240	rBV7	4667	8081	0.11%	0.010%
27	16.787	2323	2329	2332	rBV7	9578	15886	0.21%	0.019%
28	16.887	2343	2346	2353	rVB8	8004	15859	0.21%	0.019%
29	17.110	2377	2384	2394	rBV	2924679	4178498	56.29%	4.944%
30	17.210	2394	2401	2415	rVV	4386485	6379453	85.94%	7.549%
31	19.039	2708	2712	2717	rBV3	62224	78944	1.06%	0.093%
32	19.104	2720	2723	2727	rBV2	53498	67594	0.91%	0.080%
33	19.463	2778	2784	2793	rBV	5825699	7422739	100.00%	8.783%
34	21.228	3080	3084	3095	rBV	3608422	4591183	61.85%	5.433%
35	23.433	3452	3459	3468	rBV2	3874420	7301521	98.37%	8.640%
36	23.586	3479	3485	3494	rVB2	2326525	4484493	60.42%	5.306%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011031.D
Acq On : 19 Jul 2022 14:23
Operator : CG/JU
Sample : PB146296BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK296

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Title : SVOA CALIBRATION




Sum of corrected areas: 84511331

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011031.D
Acq On : 19 Jul 2022 14:23
Operator : CG/JU
Sample : PB146296BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK296

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

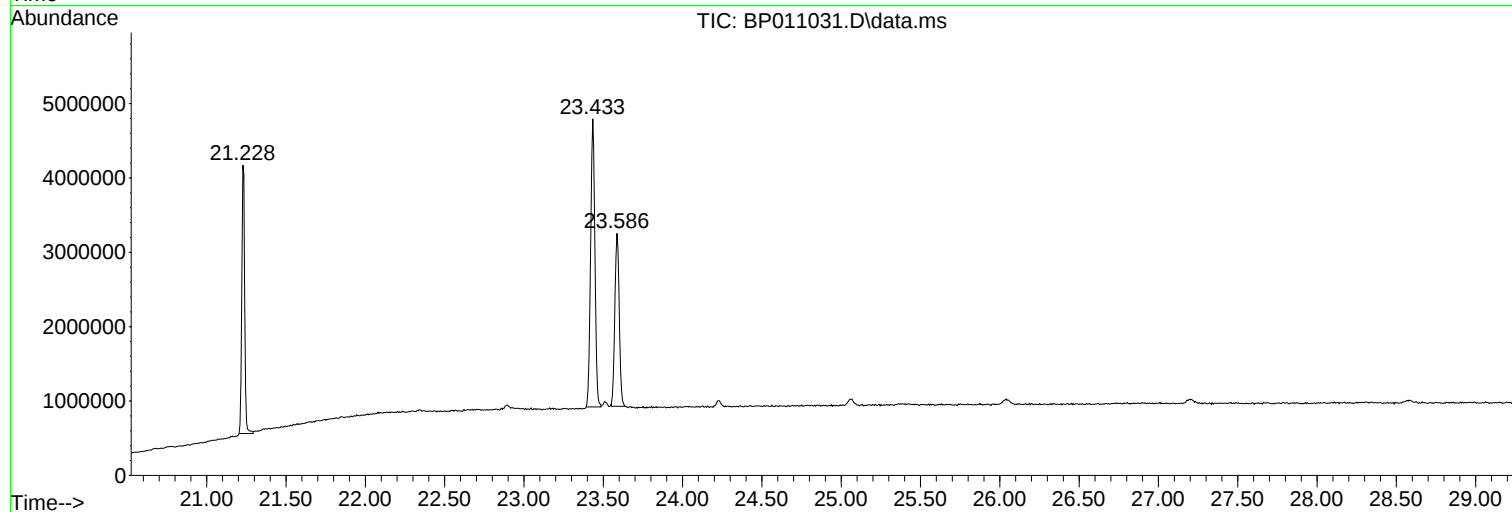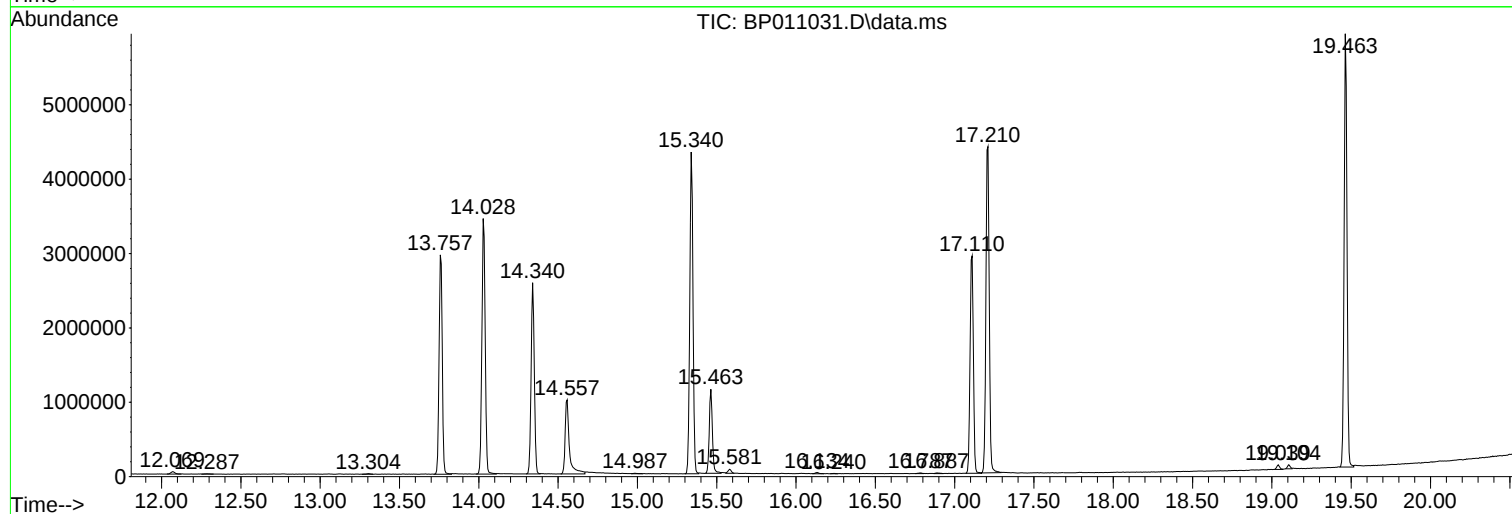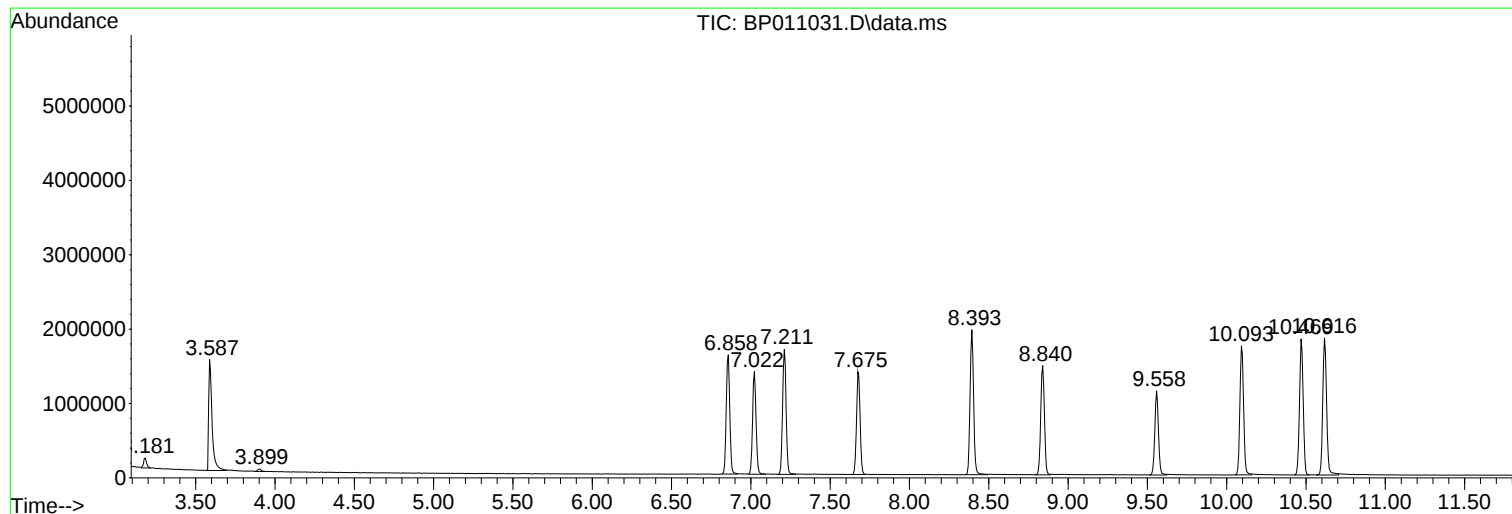

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011031.D
Acq On : 19 Jul 2022 14:23
Operator : CG/JU
Sample : PB146296BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK296

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011031.D
Acq On : 19 Jul 2022 14:23
Operator : CG/JU
Sample : PB146296BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK296

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc