

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
 Data File : BP011034.D
 Acq On : 19 Jul 2022 16:07
 Operator : CG/JU
 Sample : N3753-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011034.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	20	rVB	101667	124568	1.64%	0.174%
2	3.599	84	87	101	rBV	267069	414857	5.48%	0.580%
3	3.811	116	123	129	rVB2	45926	91963	1.21%	0.128%
4	3.899	135	138	143	rVB	33107	43990	0.58%	0.061%
5	4.269	198	201	206	rVB6	11151	14557	0.19%	0.020%
6	5.405	390	394	397	rVB2	9412	14197	0.19%	0.020%
7	6.022	496	499	504	rBV7	5393	9989	0.13%	0.014%
8	6.693	610	613	617	rBV6	6501	7932	0.10%	0.011%
9	6.857	635	641	655	rVB	290994	476547	6.29%	0.666%
10	7.022	661	669	680	rBV	1259728	1934326	25.53%	2.703%
11	7.210	694	701	712	rBV	1196867	1810513	23.89%	2.530%
12	7.305	715	717	720	rVB4	8945	8346	0.11%	0.012%
13	7.675	773	780	789	rBV	1304790	2027400	26.76%	2.833%
14	8.393	895	902	914	rBV	840609	1313230	17.33%	1.835%
15	8.840	970	978	986	rBV	1346283	2152282	28.41%	3.007%
16	9.263	1044	1050	1054	rBV3	11043	17733	0.23%	0.025%
17	9.557	1093	1100	1111	rBV	946757	1512139	19.96%	2.113%
18	10.093	1184	1191	1206	rBV	1382262	2242630	29.60%	3.133%
19	10.469	1247	1255	1263	rBV	1661264	2747072	36.26%	3.838%
20	10.616	1272	1280	1302	rBV	1272549	2185112	28.84%	3.053%
21	10.904	1327	1329	1335	rVB7	4166	7767	0.10%	0.011%
22	11.757	1468	1474	1481	rVB7	10886	19602	0.26%	0.027%
23	12.069	1522	1527	1532	rVB2	29152	45260	0.60%	0.063%
24	12.698	1626	1634	1640	rBV10	6310	14800	0.20%	0.021%
25	12.957	1673	1678	1681	rVB7	8754	13520	0.18%	0.019%
26	13.057	1692	1695	1700	rVB6	4736	8638	0.11%	0.012%
27	13.245	1719	1727	1729	rBV9	6439	11597	0.15%	0.016%
28	13.304	1732	1737	1742	rVV9	5160	10032	0.13%	0.014%
29	13.757	1807	1814	1825	rBV	2685513	3596021	47.46%	5.024%
30	14.028	1849	1860	1871	rBV	3005006	4303547	56.80%	6.013%
31	14.251	1895	1898	1901	rVB4	8825	11617	0.15%	0.016%
32	14.339	1906	1913	1922	rVV	2298891	3246839	42.85%	4.536%
33	14.557	1944	1950	1967	rBV3	92506	259362	3.42%	0.362%
34	14.775	1984	1987	1991	rVB6	7724	10094	0.13%	0.014%
35	15.157	2047	2052	2058	rBV2	31244	51391	0.68%	0.072%
36	15.204	2058	2060	2065	rVB3	11567	15031	0.20%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
 Data File : BP011034.D
 Acq On : 19 Jul 2022 16:07
 Operator : CG/JU
 Sample : N3753-04
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHP5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	15.339	2076	2083	2098	rBV	3943386	5519062	72.84%	7.711%
38	15.463	2098	2104	2114	rBV	974745	1347512	17.78%	1.883%
39	15.581	2119	2124	2131	rVB2	42700	67713	0.89%	0.095%
40	15.916	2177	2181	2185	rBV6	5536	9923	0.13%	0.014%
41	16.075	2203	2208	2212	rBV6	12511	20370	0.27%	0.028%
42	16.128	2214	2217	2224	rVB4	15630	24974	0.33%	0.035%
43	16.786	2324	2329	2333	rBV5	7688	12527	0.17%	0.018%
44	16.880	2339	2345	2352	rBV6	19234	38370	0.51%	0.054%
45	17.104	2377	2383	2394	rBV	2522780	3639311	48.03%	5.085%
46	17.210	2394	2401	2415	rBV2	4176038	6103588	80.55%	8.528%
47	17.628	2468	2472	2476	rBV4	13000	18086	0.24%	0.025%
48	17.798	2499	2501	2504	rVB4	9821	10904	0.14%	0.015%
49	18.016	2534	2538	2543	rBV2	48701	71780	0.95%	0.100%
50	18.086	2548	2550	2554	rVB2	12786	16546	0.22%	0.023%
51	18.304	2584	2587	2591	rBV5	13735	20616	0.27%	0.029%
52	19.039	2708	2712	2716	rBV	55027	69546	0.92%	0.097%
53	19.110	2720	2724	2727	rVV	44824	58112	0.77%	0.081%
54	19.463	2778	2784	2792	rBV	5589298	7222060	95.31%	10.091%
55	20.957	3035	3038	3044	rBV3	199158	316223	4.17%	0.442%
56	21.227	3079	3084	3092	rBV	3452736	4258658	56.20%	5.950%
57	23.433	3452	3459	3467	rBV2	4018788	7577045	100.00%	10.587%
58	23.586	3478	3485	3498	rVB	2221111	4374643	57.74%	6.112%




Sum of corrected areas: 71572070

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011034.D
Acq On : 19 Jul 2022 16:07
Operator : CG/JU
Sample : N3753-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

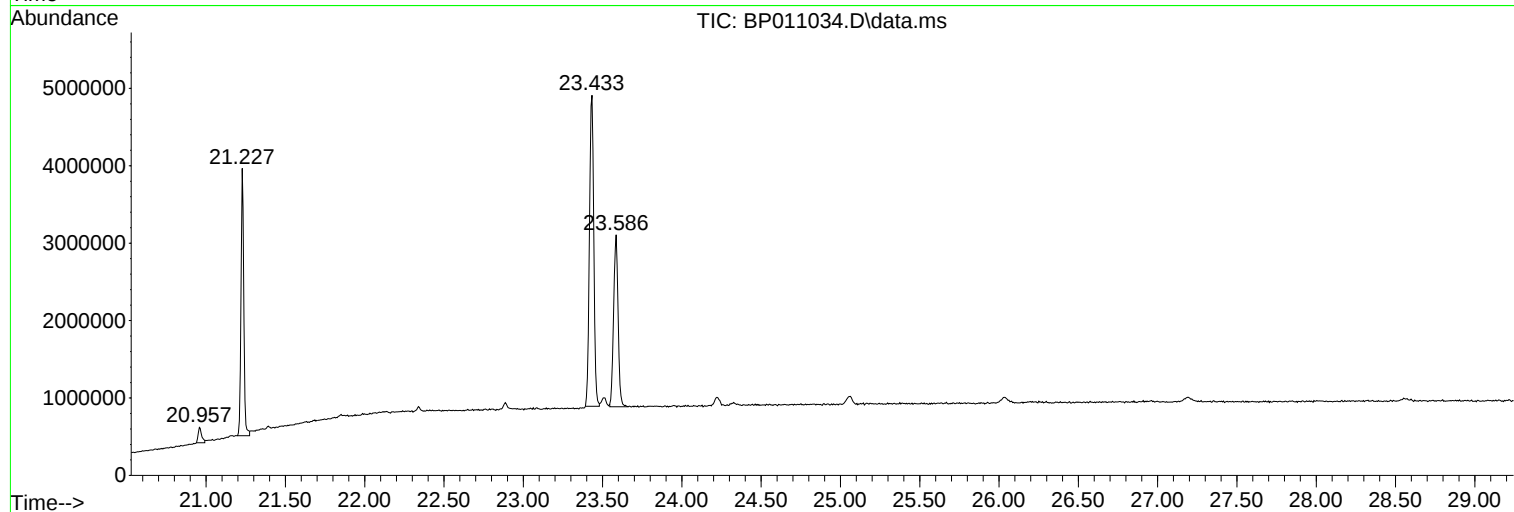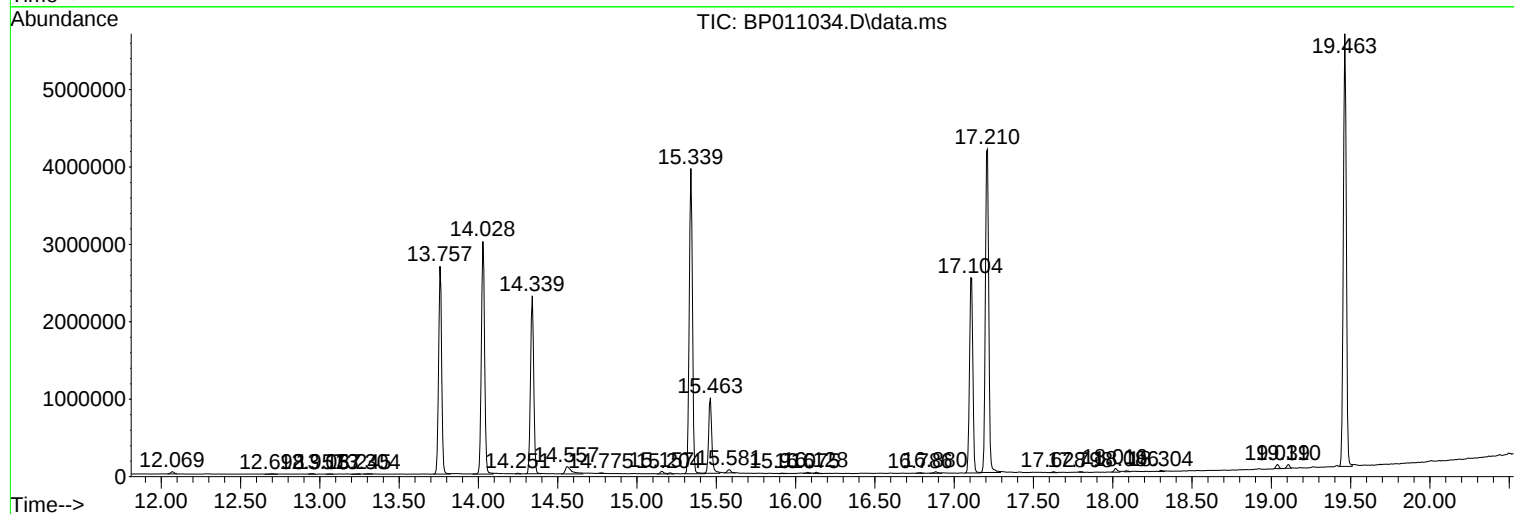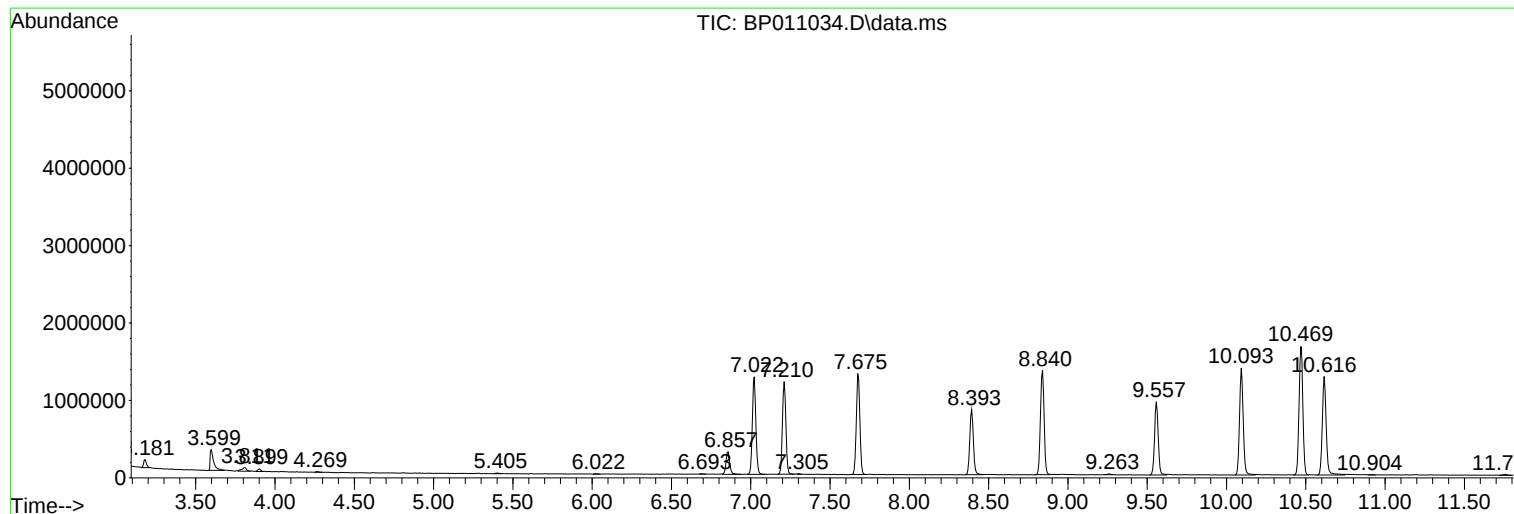

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011034.D
Acq On : 19 Jul 2022 16:07
Operator : CG/JU
Sample : N3753-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011034.D
Acq On : 19 Jul 2022 16:07
Operator : CG/JU
Sample : N3753-04
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHP5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc