

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
 Data File : BP011038.D
 Acq On : 19 Jul 2022 18:25
 Operator : CG/JU
 Sample : N3753-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHP7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011038.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	20	rBV	102836	121534	1.35%	0.151%
2	3.599	84	87	97	rBV	215924	337472	3.74%	0.420%
3	3.805	119	122	128	rVB	45241	71305	0.79%	0.089%
4	3.899	135	138	144	rVB	39674	52855	0.59%	0.066%
5	4.811	289	293	296	rBV3	6208	10416	0.12%	0.013%
6	5.399	388	393	401	rVB4	11967	20290	0.22%	0.025%
7	6.852	632	640	649	rVB	313463	492767	5.46%	0.613%
8	7.022	662	669	678	rBV	1478664	2237621	24.78%	2.784%
9	7.211	694	701	712	rBV	1373697	2068164	22.90%	2.573%
10	7.299	713	716	723	rVB8	11297	22236	0.25%	0.028%
11	7.675	773	780	788	rBV	1299224	1995995	22.10%	2.483%
12	8.346	889	894	896	rBV6	5812	12106	0.13%	0.015%
13	8.393	896	902	913	rVV	931624	1460358	16.17%	1.817%
14	8.840	970	978	987	rBV	1565866	2526461	27.97%	3.143%
15	8.963	996	999	1002	rVB4	6294	9368	0.10%	0.012%
16	9.258	1044	1049	1055	rVB	41967	63997	0.71%	0.080%
17	9.558	1092	1100	1114	rBV	1123173	1773450	19.64%	2.206%
18	10.093	1183	1191	1203	rBV	1615392	2591709	28.70%	3.225%
19	10.469	1248	1255	1266	rBV	1670806	2710317	30.01%	3.372%
20	10.616	1272	1280	1291	rBV	1503833	2475430	27.41%	3.080%
21	11.134	1364	1368	1375	rVB4	11796	23550	0.26%	0.029%
22	11.275	1386	1392	1398	rBV10	6182	13057	0.14%	0.016%
23	11.752	1466	1473	1479	rBV3	57718	101840	1.13%	0.127%
24	11.810	1479	1483	1487	rVB6	7923	11480	0.13%	0.014%
25	12.069	1521	1527	1535	rBV	34822	56746	0.63%	0.071%
26	12.281	1558	1563	1569	rVB10	7968	12662	0.14%	0.016%
27	12.881	1659	1665	1669	rBV	25365	40829	0.45%	0.051%
28	12.946	1673	1676	1680	rVB6	8130	11298	0.13%	0.014%
29	13.063	1689	1696	1700	rBV9	5328	9118	0.10%	0.011%
30	13.757	1807	1814	1827	rBV	3230935	4384671	48.55%	5.455%
31	13.899	1835	1838	1841	rVB4	6682	10149	0.11%	0.013%
32	14.028	1849	1860	1875	rBV	3678186	5203825	57.62%	6.475%
33	14.340	1905	1913	1922	rBV	2240307	3221156	35.67%	4.008%
34	14.557	1944	1950	1962	rBV2	107891	254895	2.82%	0.317%
35	14.769	1985	1986	1992	rVB6	8254	11989	0.13%	0.015%
36	15.157	2047	2052	2066	rVB2	44031	74490	0.82%	0.093%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
 Data File : BP011038.D
 Acq On : 19 Jul 2022 18:25
 Operator : CG/JU
 Sample : N3753-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHP7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	15.340	2076	2083	2090	rBV	4708047	6524530	72.24%	8.118%
38	15.463	2097	2104	2113	rBV	1240513	1725350	19.10%	2.147%
39	15.581	2120	2124	2130	rVB2	55255	78032	0.86%	0.097%
40	15.816	2160	2164	2169	rVB7	6522	11163	0.12%	0.014%
41	16.128	2213	2217	2224	rVB6	19811	30227	0.33%	0.038%
42	16.704	2311	2315	2319	rBV2	22094	29211	0.32%	0.036%
43	16.781	2322	2328	2334	rVB10	11265	21997	0.24%	0.027%
44	16.887	2343	2346	2352	rBV7	9448	16496	0.18%	0.021%
45	17.104	2375	2383	2393	rBV	2584994	3593810	39.79%	4.471%
46	17.204	2393	2400	2422	rVV2	5165774	7396917	81.90%	9.203%
47	17.410	2432	2435	2439	rVB5	7242	9206	0.10%	0.011%
48	17.792	2497	2500	2503	rVB5	9271	11525	0.13%	0.014%
49	17.904	2514	2519	2525	rBV5	12791	26768	0.30%	0.033%
50	18.022	2535	2539	2546	rBV9	23893	46997	0.52%	0.058%
51	18.087	2548	2550	2555	rVB	12486	15755	0.17%	0.020%
52	19.039	2707	2712	2716	rBV2	65158	93473	1.04%	0.116%
53	19.104	2719	2723	2727	rVV	64133	80580	0.89%	0.100%
54	19.204	2738	2740	2743	rVB4	18835	17847	0.20%	0.022%
55	19.463	2778	2784	2791	rBV	6738500	8726245	96.62%	10.857%
56	21.228	3079	3084	3090	rBV	3403157	4142838	45.87%	5.154%
57	23.433	3452	3459	3467	rVB2	4739144	9031206	100.00%	11.236%
58	23.580	3478	3484	3497	rVB2	2144242	4248342	47.04%	5.286%




Sum of corrected areas: 80374121

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011038.D
Acq On : 19 Jul 2022 18:25
Operator : CG/JU
Sample : N3753-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHP7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

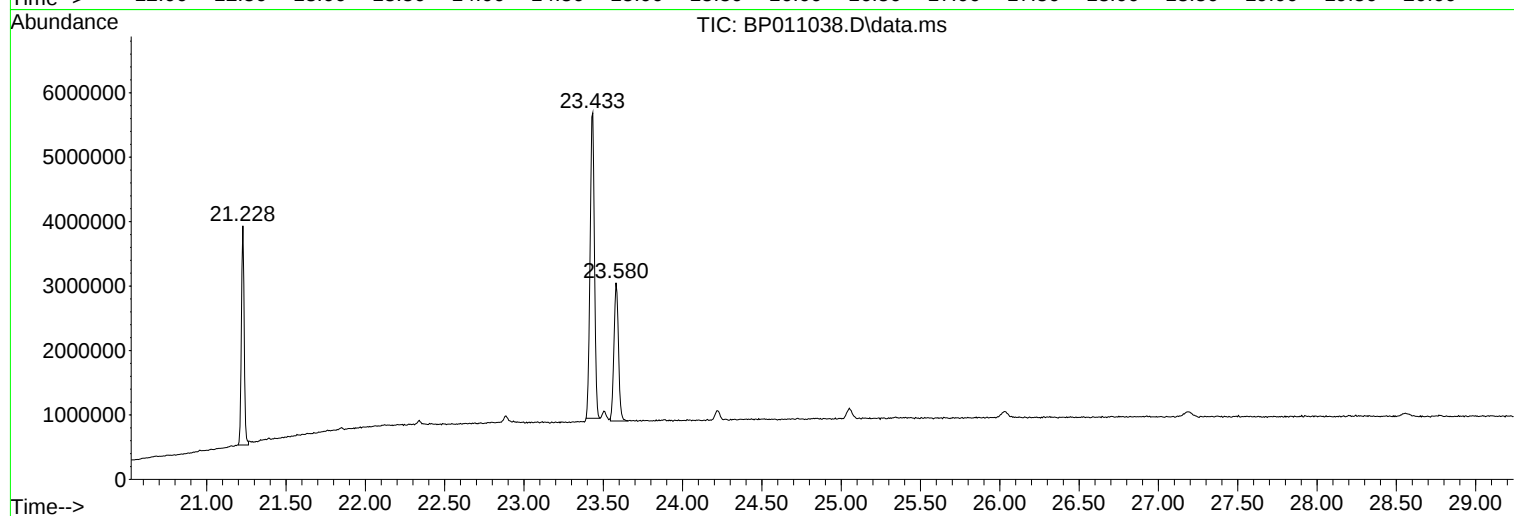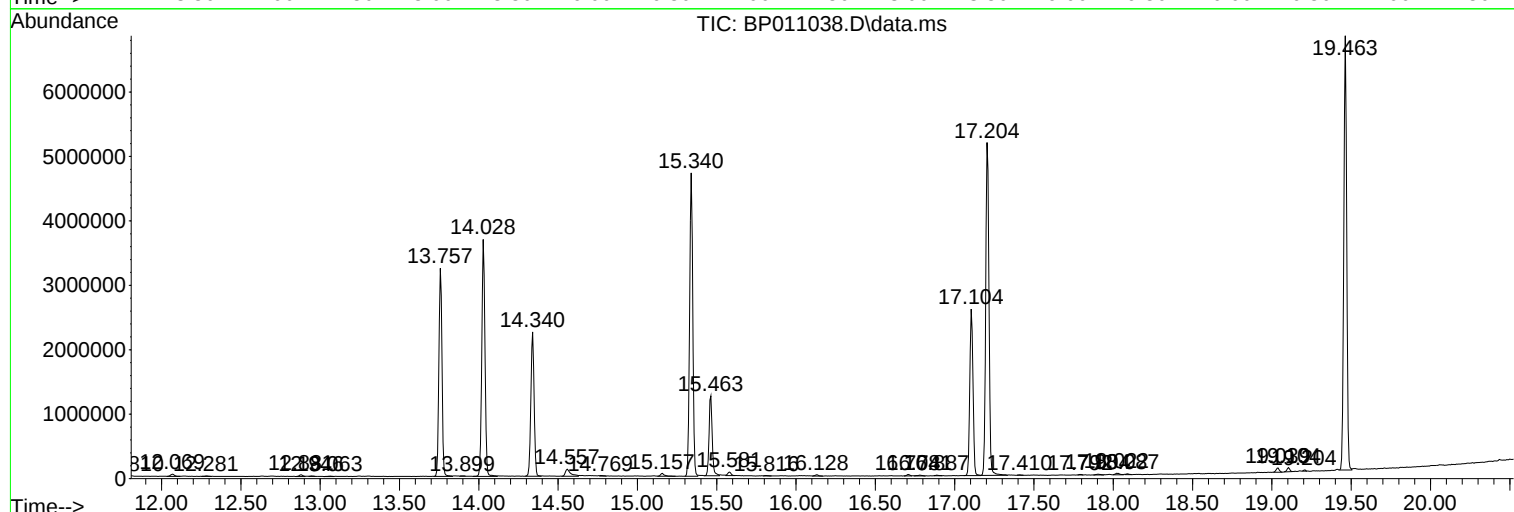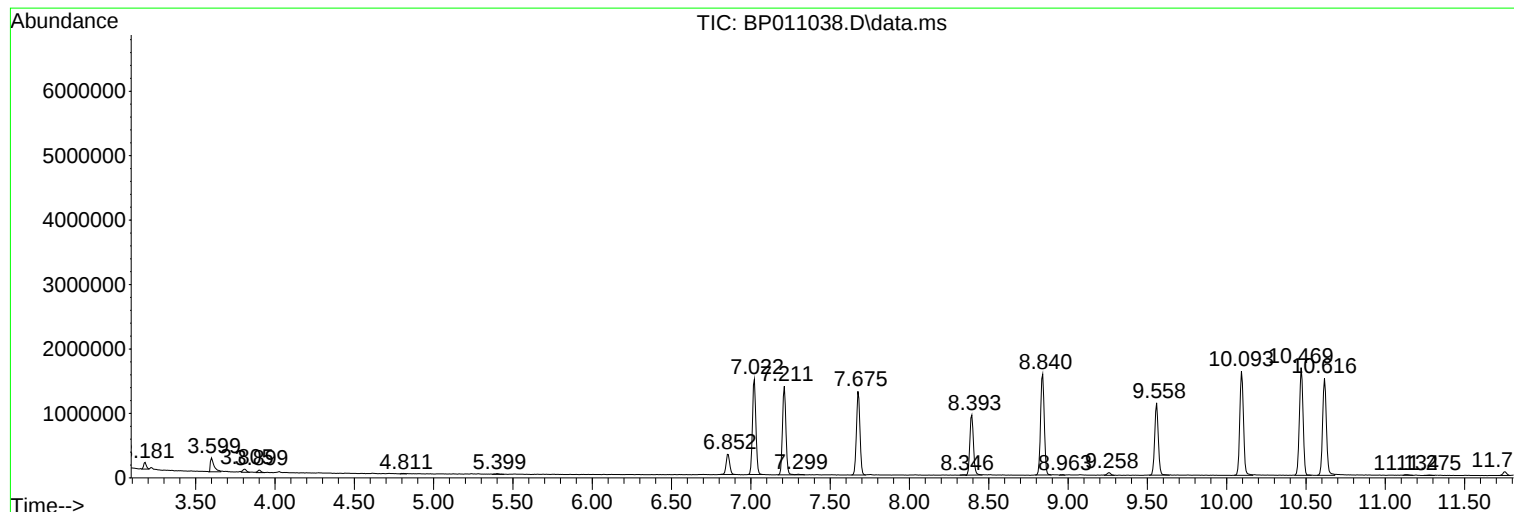

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011038.D
Acq On : 19 Jul 2022 18:25
Operator : CG/JU
Sample : N3753-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHP7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011038.D
Acq On : 19 Jul 2022 18:25
Operator : CG/JU
Sample : N3753-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHP7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc