

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
 Data File : BP011039.D
 Acq On : 19 Jul 2022 19:00
 Operator : CG/JU
 Sample : N3753-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011039.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	23	rVB	95073	126995	1.36%	0.155%
2	3.593	84	86	103	rBV	500486	769223	8.23%	0.939%
3	3.810	119	123	129	rVB	48724	78881	0.84%	0.096%
4	3.899	135	138	144	rVB2	30976	46002	0.49%	0.056%
5	5.399	390	393	399	rVB	11774	17342	0.19%	0.021%
6	6.687	610	612	619	rVB6	11199	17454	0.19%	0.021%
7	6.857	631	641	650	rBV	293054	471915	5.05%	0.576%
8	7.022	662	669	680	rBV	1406184	2161628	23.13%	2.637%
9	7.210	694	701	710	rBV	1276612	1931934	20.68%	2.357%
10	7.304	713	717	722	rVB6	10711	16820	0.18%	0.021%
11	7.675	772	780	790	rBV	1328322	1996379	21.37%	2.436%
12	8.393	895	902	915	rBV	893580	1392196	14.90%	1.699%
13	8.840	966	978	990	rBV	1567805	2528904	27.07%	3.085%
14	9.257	1042	1049	1055	rBV	29457	48146	0.52%	0.059%
15	9.557	1093	1100	1110	rBV	1071734	1713454	18.34%	2.091%
16	10.092	1184	1191	1200	rBV	1560283	2513949	26.91%	3.067%
17	10.469	1248	1255	1264	rVB	1708687	2717578	29.08%	3.316%
18	10.616	1268	1280	1303	rBV	1616874	2738852	29.31%	3.342%
19	11.757	1470	1474	1479	rVB2	21414	32660	0.35%	0.040%
20	12.069	1522	1527	1535	rVB	33407	59371	0.64%	0.072%
21	12.286	1559	1564	1570	rVB9	6506	15560	0.17%	0.019%
22	12.698	1629	1634	1639	rVB7	6363	10363	0.11%	0.013%
23	12.945	1670	1676	1681	rBV9	7955	11793	0.13%	0.014%
24	13.245	1721	1727	1732	rBV4	11817	21728	0.23%	0.027%
25	13.304	1732	1737	1744	rVB9	7524	16735	0.18%	0.020%
26	13.757	1808	1814	1824	rBV	3372636	4488970	48.04%	5.477%
27	14.028	1853	1860	1871	rBV	3618676	5240940	56.09%	6.394%
28	14.339	1905	1913	1920	rBV	2256968	3287802	35.19%	4.011%
29	14.557	1944	1950	1961	rBV	100727	235127	2.52%	0.287%
30	14.775	1982	1987	1991	rBV8	8486	12265	0.13%	0.015%
31	15.157	2048	2052	2059	rBV2	28393	41882	0.45%	0.051%
32	15.339	2076	2083	2093	rBV	4802753	6820819	73.00%	8.322%
33	15.463	2097	2104	2119	rVV	1270713	1763917	18.88%	2.152%
34	15.580	2119	2124	2131	rVB	59101	93320	1.00%	0.114%
35	16.039	2195	2202	2205	rBV9	6958	15151	0.16%	0.018%
36	16.127	2214	2217	2223	rVB4	17871	24663	0.26%	0.030%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
 Data File : BP011039.D
 Acq On : 19 Jul 2022 19:00
 Operator : CG/JU
 Sample : N3753-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHQ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	16.780	2324	2328	2334	rBV7	12365	19770	0.21%	0.024%
38	16.886	2341	2346	2350	rBV7	8482	15219	0.16%	0.019%
39	17.104	2377	2383	2393	rBV	2667097	3714682	39.76%	4.532%
40	17.204	2393	2400	2415	rVV2	5582903	7775175	83.21%	9.486%
41	17.310	2415	2418	2423	rVB6	25189	34935	0.37%	0.043%
42	17.410	2432	2435	2440	rVB2	12749	16804	0.18%	0.021%
43	17.792	2497	2500	2507	rVB9	11571	17017	0.18%	0.021%
44	18.016	2535	2538	2542	rBV5	8165	10177	0.11%	0.012%
45	18.086	2547	2550	2555	rVB	14690	18209	0.19%	0.022%
46	19.039	2708	2712	2716	rVB2	68399	85727	0.92%	0.105%
47	19.104	2719	2723	2728	rVV	64303	84334	0.90%	0.103%
48	19.463	2778	2784	2792	rBV	6964320	9019698	96.53%	11.005%
49	21.227	3079	3084	3089	rBV	3557236	4166900	44.60%	5.084%
50	23.427	3451	3458	3466	rBV2	4862804	9343627	100.00%	11.400%
51	23.580	3478	3484	3493	rVB2	2115990	4157977	44.50%	5.073%




Sum of corrected areas: 81960969

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011039.D
Acq On : 19 Jul 2022 19:00
Operator : CG/JU
Sample : N3753-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHQ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

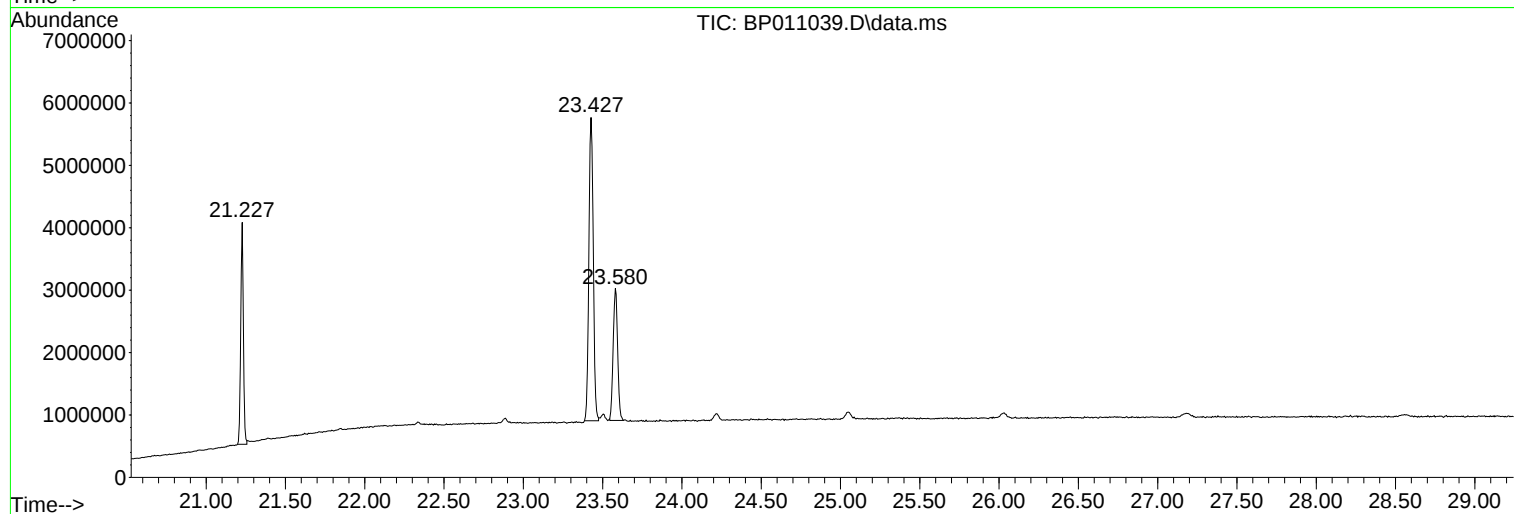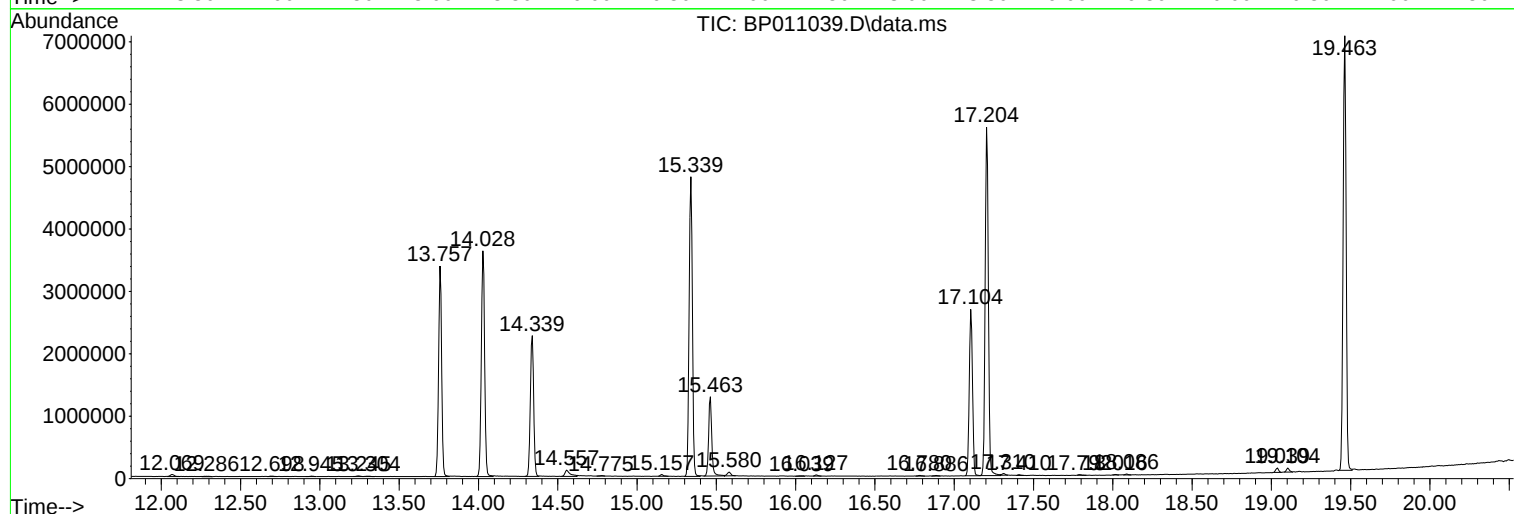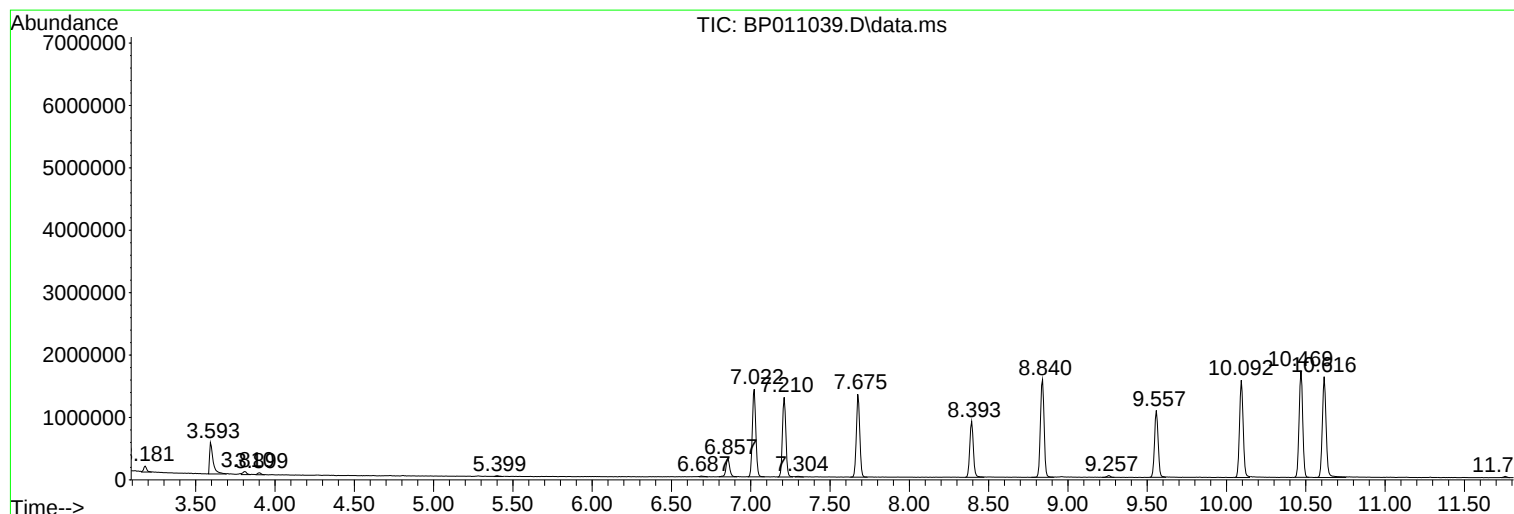

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011039.D
Acq On : 19 Jul 2022 19:00
Operator : CG/JU
Sample : N3753-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHQ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011039.D
Acq On : 19 Jul 2022 19:00
Operator : CG/JU
Sample : N3753-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHQ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------