

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
 Data File : BP011040.D
 Acq On : 19 Jul 2022 19:34
 Operator : CG/JU
 Sample : N3753-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHQ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011040.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	25	rVB	103781	158889	1.71%	0.193%
2	3.593	84	86	106	rVB	423652	680077	7.32%	0.825%
3	3.811	115	123	129	rVB2	49347	100595	1.08%	0.122%
4	3.899	135	138	143	rVB	34011	45977	0.50%	0.056%
5	5.240	363	366	369	rBV4	7802	11022	0.12%	0.013%
6	5.399	389	393	397	rVB	12307	17097	0.18%	0.021%
7	6.810	628	633	634	rBV4	7557	11593	0.12%	0.014%
8	6.852	634	640	651	rVB	329797	532713	5.74%	0.646%
9	7.022	662	669	682	rVB	1434158	2188093	23.57%	2.653%
10	7.210	694	701	709	rBV	1345717	2031858	21.88%	2.464%
11	7.299	713	716	720	rVB6	7194	9642	0.10%	0.012%
12	7.675	773	780	789	rVV	1311566	1998062	21.52%	2.423%
13	7.757	790	794	799	rVB7	5252	9654	0.10%	0.012%
14	8.393	895	902	917	rBV	957604	1518253	16.35%	1.841%
15	8.840	970	978	986	rBV	1522289	2473648	26.64%	2.999%
16	8.957	992	998	1001	rBV7	4718	10924	0.12%	0.013%
17	9.257	1043	1049	1054	rBV4	18457	32356	0.35%	0.039%
18	9.557	1091	1100	1114	rBV	1064464	1724729	18.57%	2.091%
19	10.093	1184	1191	1204	rBV	1606456	2575895	27.74%	3.123%
20	10.469	1247	1255	1263	rBV	1691317	2727122	29.37%	3.307%
21	10.616	1273	1280	1301	rBV	1497766	2563309	27.61%	3.108%
22	11.751	1468	1473	1480	rBV2	66232	113709	1.22%	0.138%
23	12.069	1520	1527	1533	rVB	34409	58101	0.63%	0.070%
24	12.281	1559	1563	1568	rVB7	6354	9620	0.10%	0.012%
25	12.634	1620	1623	1629	rVB7	11878	17645	0.19%	0.021%
26	13.245	1721	1727	1730	rBV5	11912	18140	0.20%	0.022%
27	13.757	1808	1814	1826	rBV	3401902	4437884	47.79%	5.381%
28	13.898	1834	1838	1844	rVB2	44857	63049	0.68%	0.076%
29	14.028	1852	1860	1875	rBV	3656335	5161369	55.59%	6.258%
30	14.339	1905	1913	1923	rBV	2266405	3299379	35.53%	4.001%
31	14.557	1944	1950	1964	rBV2	117634	295544	3.18%	0.358%
32	14.781	1983	1988	1992	rVB7	9715	17074	0.18%	0.021%
33	14.881	2002	2005	2011	rVB8	5891	11556	0.12%	0.014%
34	15.163	2047	2053	2055	rBV2	12084	22512	0.24%	0.027%
35	15.339	2076	2083	2096	rBV	4853399	6747976	72.67%	8.182%
36	15.463	2097	2104	2119	rVV	1163512	1645097	17.72%	1.995%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
 Data File : BP011040.D
 Acq On : 19 Jul 2022 19:34
 Operator : CG/JU
 Sample : N3753-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHQ4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	15.581	2119	2124	2131	rVB2	61089	93662	1.01%	0.114%
38	15.722	2145	2148	2154	rVB8	7770	12733	0.14%	0.015%
39	15.810	2160	2163	2168	rVB3	20873	27192	0.29%	0.033%
40	15.910	2176	2180	2183	rBV6	6957	10654	0.11%	0.013%
41	16.128	2213	2217	2223	rVB4	19326	26320	0.28%	0.032%
42	16.710	2311	2316	2322	rBV	31493	46027	0.50%	0.056%
43	16.786	2324	2329	2332	rVB6	11023	17082	0.18%	0.021%
44	16.886	2342	2346	2350	rBV5	6189	10520	0.11%	0.013%
45	17.104	2375	2383	2393	rBV	2594091	3694747	39.79%	4.480%
46	17.204	2394	2400	2415	rVV2	5623799	7834095	84.37%	9.499%
47	17.310	2415	2418	2423	rVB6	16617	28451	0.31%	0.034%
48	17.492	2446	2449	2452	rBV5	5805	9423	0.10%	0.011%
49	17.792	2497	2500	2504	rBV5	18431	23213	0.25%	0.028%
50	17.910	2517	2520	2525	rVB5	16085	18857	0.20%	0.023%
51	18.016	2535	2538	2547	rBV10	18740	32631	0.35%	0.040%
52	18.086	2547	2550	2555	rVV	15597	23640	0.25%	0.029%
53	18.580	2630	2634	2636	rBV5	13882	18956	0.20%	0.023%
54	19.039	2708	2712	2716	rBV	63422	85125	0.92%	0.103%
55	19.104	2719	2723	2729	rVV	66681	88217	0.95%	0.107%
56	19.410	2773	2775	2778	rBV3	19235	19625	0.21%	0.024%
57	19.463	2778	2784	2792	rBV	7198130	9182788	98.90%	11.135%
58	21.227	3079	3084	3090	rBV	3594196	4258720	45.87%	5.164%
59	23.433	3452	3459	3467	rBV	5005090	9285262	100.00%	11.259%
60	23.580	3478	3484	3495	rVB2	2181337	4282294	46.12%	5.193%




Sum of corrected areas: 82470397

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011040.D
Acq On : 19 Jul 2022 19:34
Operator : CG/JU
Sample : N3753-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHQ4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

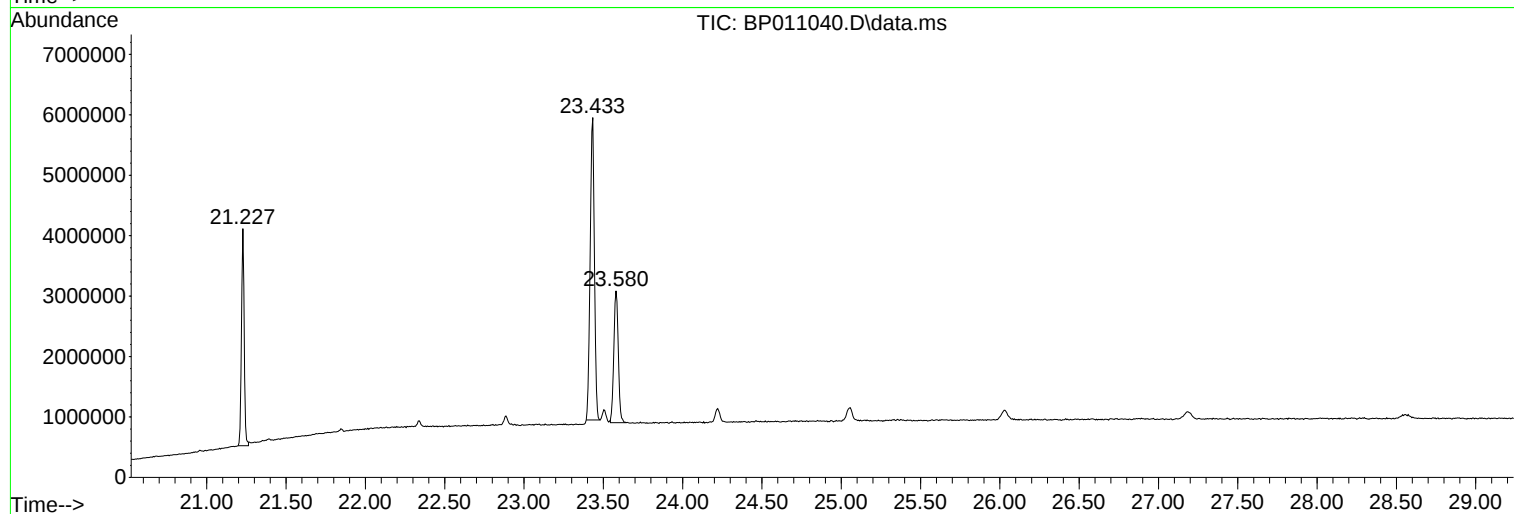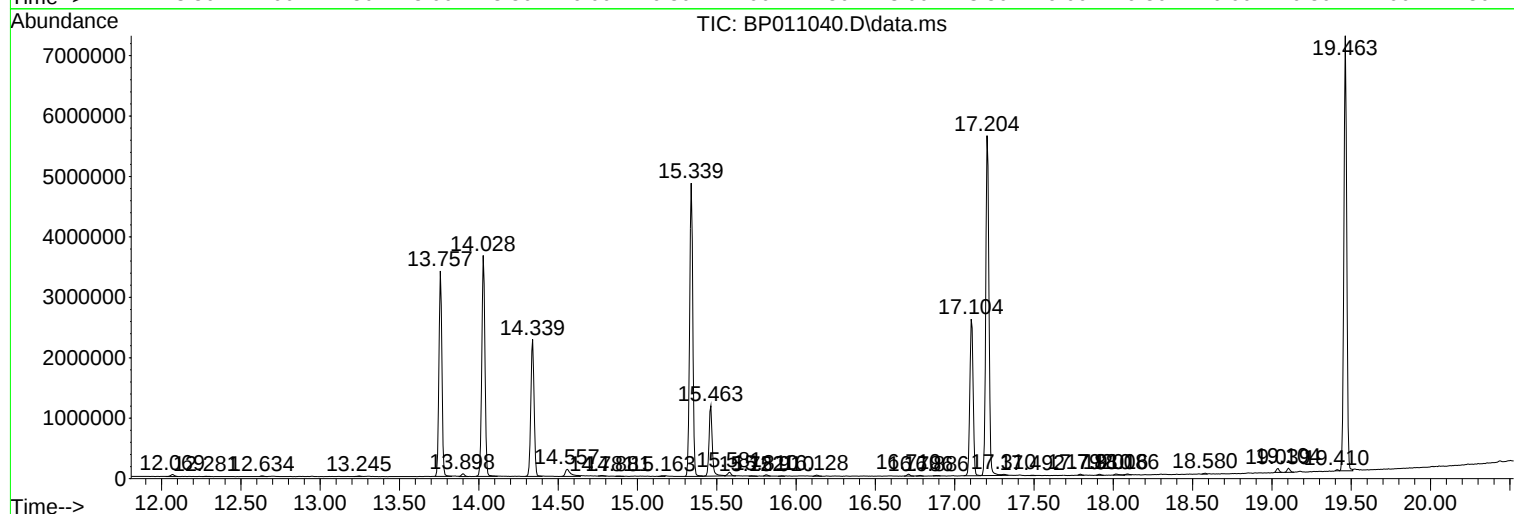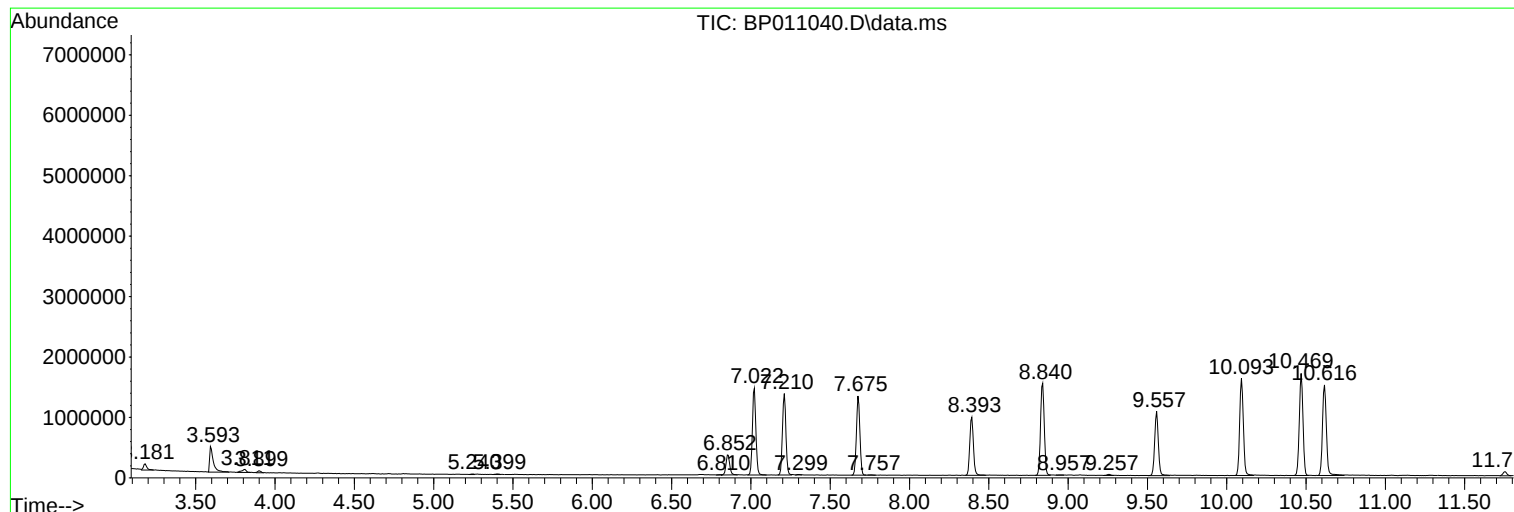

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011040.D
Acq On : 19 Jul 2022 19:34
Operator : CG/JU
Sample : N3753-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHQ4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011040.D
Acq On : 19 Jul 2022 19:34
Operator : CG/JU
Sample : N3753-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHQ4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------