

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
 Data File : BP011041.D
 Acq On : 19 Jul 2022 20:09
 Operator : CG/JU
 Sample : N3753-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011041.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	23	rVB	94985	137379	1.68%	0.177%
2	3.599	84	87	101	rBV	316014	509805	6.23%	0.657%
3	3.811	119	123	129	rVB	44080	73810	0.90%	0.095%
4	3.899	135	138	143	rVB	33172	41602	0.51%	0.054%
5	5.399	391	393	400	rVB3	11398	17964	0.22%	0.023%
6	5.481	405	407	410	rVV3	7089	8582	0.10%	0.011%
7	5.540	414	417	422	rVB	20833	28789	0.35%	0.037%
8	6.852	635	640	649	rVB	280858	443334	5.42%	0.571%
9	7.022	662	669	678	rVB	1368042	2122310	25.93%	2.735%
10	7.211	694	701	711	rBV	1271045	1927009	23.55%	2.483%
11	7.299	713	716	722	rVB8	7544	13843	0.17%	0.018%
12	7.675	773	780	788	rBV	1321027	2006480	24.52%	2.585%
13	7.752	790	793	797	rVB5	8271	12067	0.15%	0.016%
14	8.393	895	902	914	rBV	852953	1357166	16.58%	1.749%
15	8.834	970	977	991	rBV	1463709	2411688	29.47%	3.108%
16	8.963	994	999	1002	rBV7	7641	10712	0.13%	0.014%
17	9.252	1042	1048	1053	rBV7	8224	14843	0.18%	0.019%
18	9.557	1093	1100	1115	rBV	1044924	1679396	20.52%	2.164%
19	10.093	1184	1191	1203	rBV	1541507	2462822	30.09%	3.174%
20	10.469	1248	1255	1266	rBV	1683275	2758545	33.71%	3.555%
21	10.616	1272	1280	1299	rBV	1423860	2419229	29.56%	3.117%
22	11.128	1363	1367	1374	rVB6	8795	17520	0.21%	0.023%
23	11.281	1389	1393	1396	rBV6	5558	9236	0.11%	0.012%
24	11.757	1468	1474	1479	rBV6	7743	13618	0.17%	0.018%
25	12.069	1522	1527	1532	rVB	30472	54363	0.66%	0.070%
26	12.287	1559	1564	1568	rVB8	5733	9159	0.11%	0.012%
27	12.687	1627	1632	1638	rBV4	10346	18325	0.22%	0.024%
28	12.946	1669	1676	1681	rBV4	17062	29192	0.36%	0.038%
29	13.246	1719	1727	1730	rBV8	8202	16996	0.21%	0.022%
30	13.304	1730	1737	1745	rVB8	7412	21322	0.26%	0.027%
31	13.757	1807	1814	1825	rBV	3256353	4247982	51.91%	5.474%
32	14.028	1851	1860	1871	rBV	3566978	4969541	60.72%	6.404%
33	14.340	1905	1913	1924	rBV	2334405	3346745	40.89%	4.313%
34	14.557	1944	1950	1962	rBV	91234	220901	2.70%	0.285%
35	14.775	1984	1987	1992	rVB7	6099	9207	0.11%	0.012%
36	14.975	2017	2021	2026	rVB3	20763	25743	0.31%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
 Data File : BP011041.D
 Acq On : 19 Jul 2022 20:09
 Operator : CG/JU
 Sample : N3753-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHQ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	15.157	2046	2052	2059	rBV2	49102	77613	0.95%	0.100%
38	15.340	2076	2083	2091	rBV	4629582	6387345	78.05%	8.231%
39	15.457	2097	2103	2115	rBV	1118492	1590531	19.44%	2.050%
40	15.581	2119	2124	2128	rVB	55987	80431	0.98%	0.104%
41	15.904	2175	2179	2183	rBV7	5114	9870	0.12%	0.013%
42	16.128	2213	2217	2222	rBV6	18461	29317	0.36%	0.038%
43	16.781	2321	2328	2334	rBV9	10498	19829	0.24%	0.026%
44	16.892	2342	2347	2355	rVB8	10437	23572	0.29%	0.030%
45	17.104	2376	2383	2392	rBV	2763955	3800682	46.44%	4.897%
46	17.204	2394	2400	2422	rVV2	4932018	7009016	85.64%	9.032%
47	17.410	2433	2435	2441	rVB5	12528	14294	0.17%	0.018%
48	17.786	2497	2499	2504	rVB5	11831	12978	0.16%	0.017%
49	18.016	2535	2538	2541	rBV4	14446	18877	0.23%	0.024%
50	18.086	2548	2550	2554	rVB	13458	13954	0.17%	0.018%
51	19.033	2707	2711	2716	rBV2	62148	87281	1.07%	0.112%
52	19.104	2719	2723	2729	rVV	63634	84167	1.03%	0.108%
53	19.204	2738	2740	2744	rVB4	18847	14126	0.17%	0.018%
54	19.463	2778	2784	2792	rBV	6085763	8131006	99.35%	10.477%
55	21.227	3079	3084	3090	rBV	3436535	4251707	51.95%	5.479%
56	23.427	3451	3458	3466	rBV2	4384925	8183825	100.00%	10.545%
57	23.580	3477	3484	3495	rVB2	2140835	4297724	52.51%	5.538%




Sum of corrected areas: 77605370

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011041.D
Acq On : 19 Jul 2022 20:09
Operator : CG/JU
Sample : N3753-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHQ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

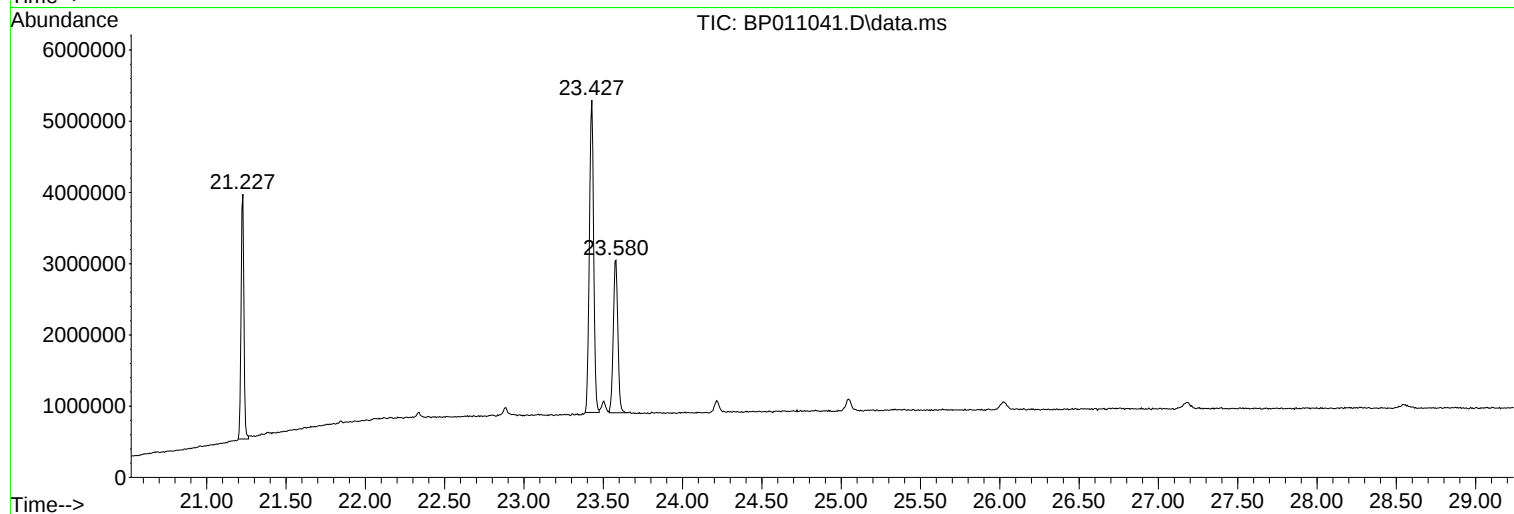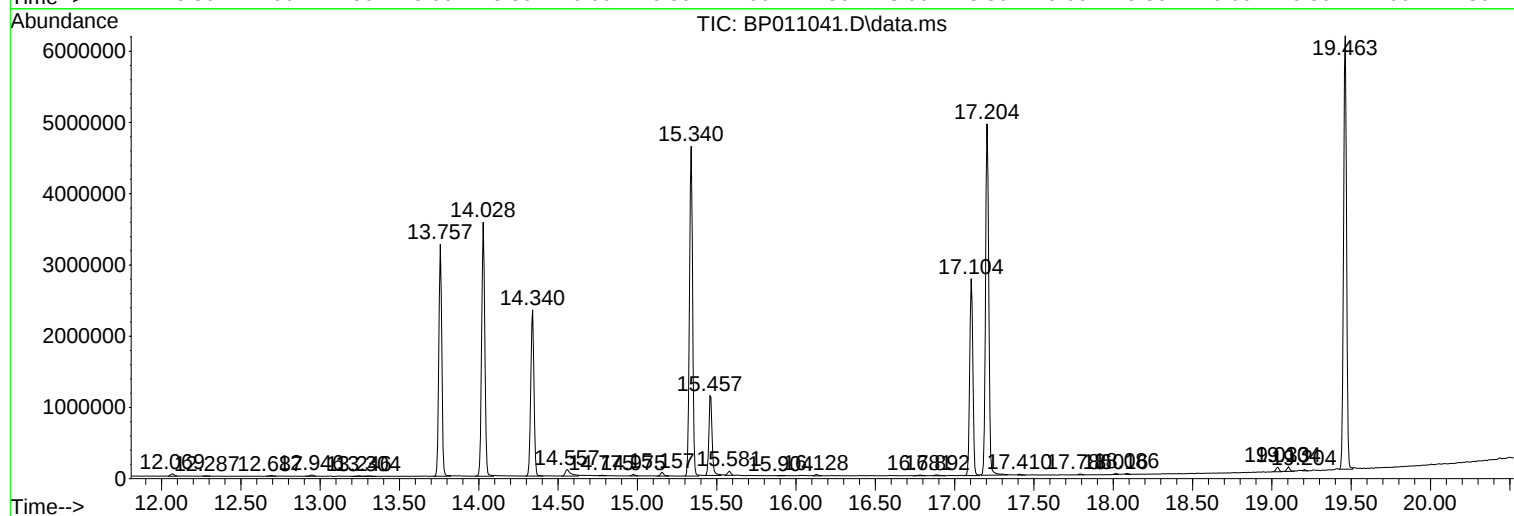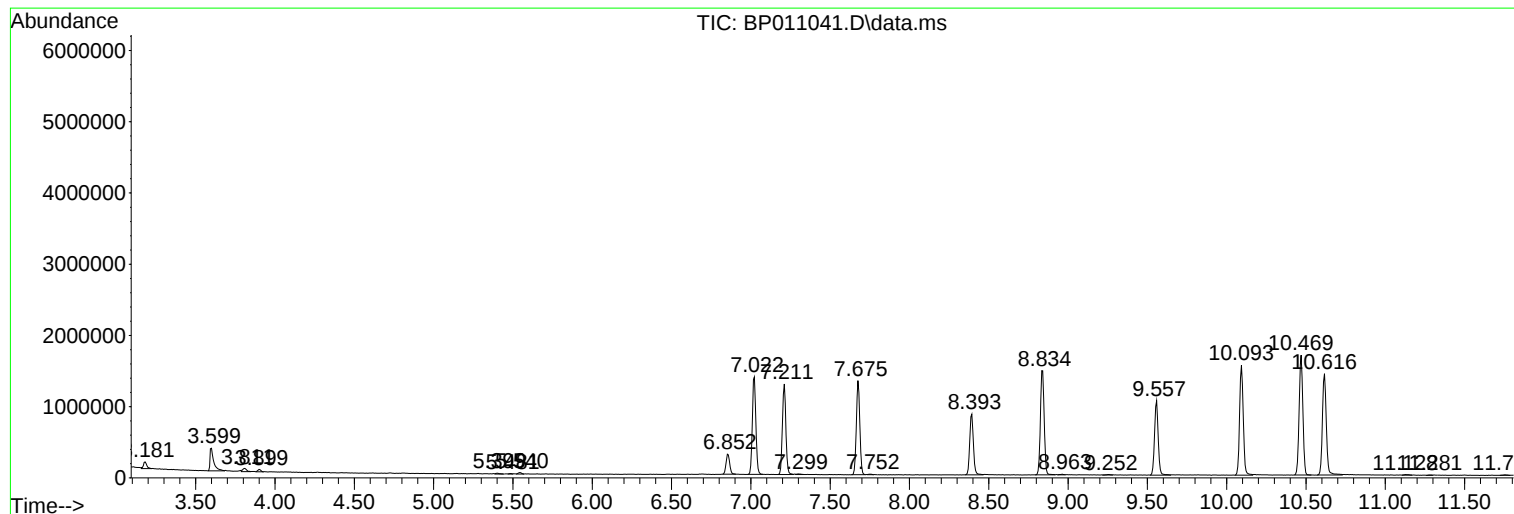

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011041.D
Acq On : 19 Jul 2022 20:09
Operator : CG/JU
Sample : N3753-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHQ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011041.D
Acq On : 19 Jul 2022 20:09
Operator : CG/JU
Sample : N3753-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHQ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc