

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
 Data File : BP011042.D
 Acq On : 19 Jul 2022 20:44
 Operator : CG/JU
 Sample : N3753-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHQ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011042.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	25	rVB	108252	157745	1.72%	0.189%
2	3.593	83	86	103	rBV	496634	771082	8.39%	0.922%
3	3.811	120	123	130	rVB2	52397	74268	0.81%	0.089%
4	3.899	135	138	144	rVB	32293	39675	0.43%	0.047%
5	5.399	391	393	397	rVB3	10838	12866	0.14%	0.015%
6	6.687	608	612	616	rVB6	6475	10872	0.12%	0.013%
7	6.852	634	640	653	rVB	310248	505462	5.50%	0.604%
8	7.016	662	668	680	rVB	1438166	2266480	24.67%	2.710%
9	7.211	694	701	711	rBV	1320907	2030147	22.10%	2.427%
10	7.305	713	717	720	rVB5	8697	11878	0.13%	0.014%
11	7.675	772	780	787	rBV	1319227	1996740	21.73%	2.387%
12	8.393	894	902	917	rBV	913205	1488258	16.20%	1.779%
13	8.840	970	978	986	rBV	1596907	2595232	28.25%	3.103%
14	9.557	1092	1100	1109	rBV	1129790	1816616	19.77%	2.172%
15	10.093	1183	1191	1202	rBV	1671574	2672125	29.08%	3.195%
16	10.469	1247	1255	1264	rBV	1674678	2761768	30.06%	3.302%
17	10.616	1270	1280	1294	rBV	1621759	2806131	30.54%	3.355%
18	11.493	1424	1429	1433	rBV8	3784	9402	0.10%	0.011%
19	12.069	1522	1527	1533	rVB2	35764	56245	0.61%	0.067%
20	12.699	1628	1634	1639	rBV6	10009	17896	0.19%	0.021%
21	12.946	1671	1676	1681	rBV4	10593	15390	0.17%	0.018%
22	13.240	1719	1726	1729	rBV7	9761	16684	0.18%	0.020%
23	13.304	1732	1737	1743	rVB9	5518	11392	0.12%	0.014%
24	13.757	1807	1814	1825	rBV	3277428	4482985	48.79%	5.360%
25	14.028	1852	1860	1872	rBV	3810364	5390655	58.67%	6.445%
26	14.340	1906	1913	1922	rBV	2283874	3400561	37.01%	4.066%
27	14.557	1942	1950	1968	rBV	102316	276534	3.01%	0.331%
28	15.157	2046	2052	2057	rBV2	23689	36797	0.40%	0.044%
29	15.340	2076	2083	2094	rBV	4685744	6770115	73.69%	8.094%
30	15.457	2097	2103	2118	rVV	1299861	1812503	19.73%	2.167%
31	15.575	2119	2123	2133	rVB	58308	96894	1.05%	0.116%
32	16.034	2194	2201	2205	rBV10	6118	13146	0.14%	0.016%
33	16.128	2212	2217	2222	rVB3	18402	26328	0.29%	0.031%
34	16.781	2325	2328	2332	rVB6	10420	15029	0.16%	0.018%
35	16.881	2342	2345	2350	rBV5	6671	10153	0.11%	0.012%
36	17.045	2368	2373	2376	rBV7	6012	9969	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
 Data File : BP011042.D
 Acq On : 19 Jul 2022 20:44
 Operator : CG/JU
 Sample : N3753-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHQ3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	17.104	2377	2383	2393	rVV	2806879	3885245	42.29%	4.645%
38	17.204	2393	2400	2414	rVV2	5732754	7913823	86.14%	9.462%
39	17.310	2414	2418	2424	rVB8	27777	50920	0.55%	0.061%
40	17.410	2432	2435	2438	rVB3	8713	9857	0.11%	0.012%
41	17.486	2443	2448	2451	rBV7	5521	9441	0.10%	0.011%
42	17.798	2497	2501	2505	rVB7	7404	13389	0.15%	0.016%
43	18.016	2534	2538	2541	rBV5	13682	19562	0.21%	0.023%
44	18.086	2548	2550	2556	rVB2	13663	13685	0.15%	0.016%
45	19.033	2707	2711	2716	rBV2	72320	96021	1.05%	0.115%
46	19.104	2718	2723	2728	rVV	64903	97057	1.06%	0.116%
47	19.463	2778	2784	2790	rBV	6870399	9153713	99.63%	10.944%
48	21.227	3079	3084	3089	rBV	3379609	4280730	46.59%	5.118%
49	23.427	3451	3458	3466	rBV2	4697940	9187391	100.00%	10.984%
50	23.574	3477	3483	3500	rVB2	2226418	4425221	48.17%	5.291%




Sum of corrected areas: 83642078

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011042.D
Acq On : 19 Jul 2022 20:44
Operator : CG/JU
Sample : N3753-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHQ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

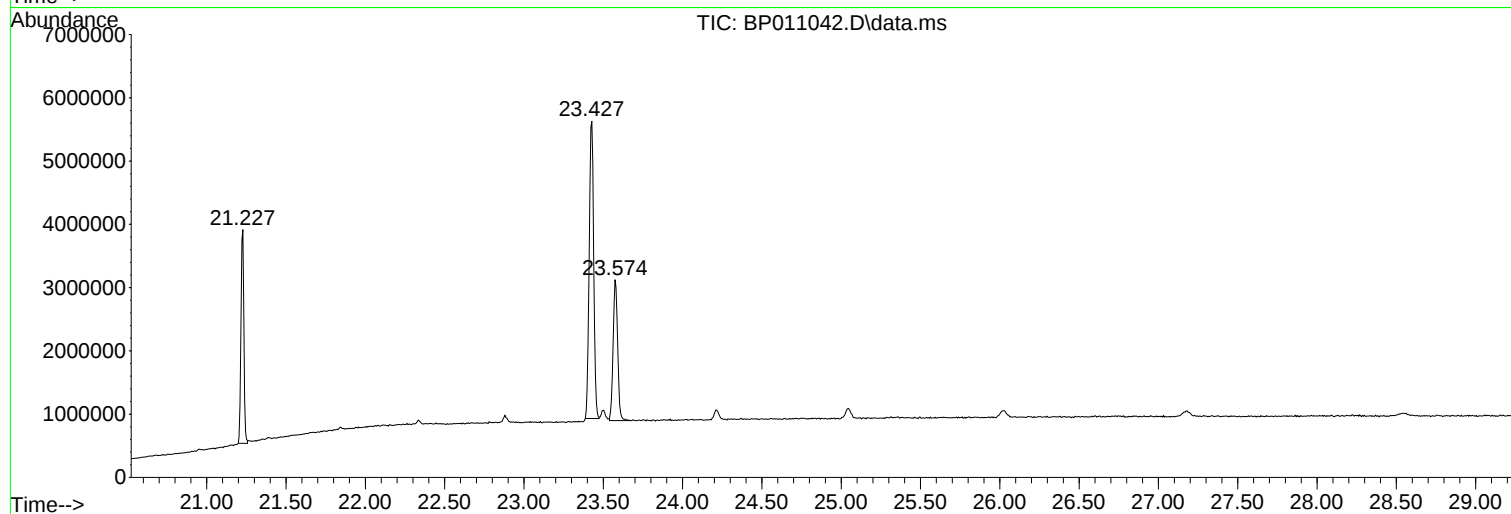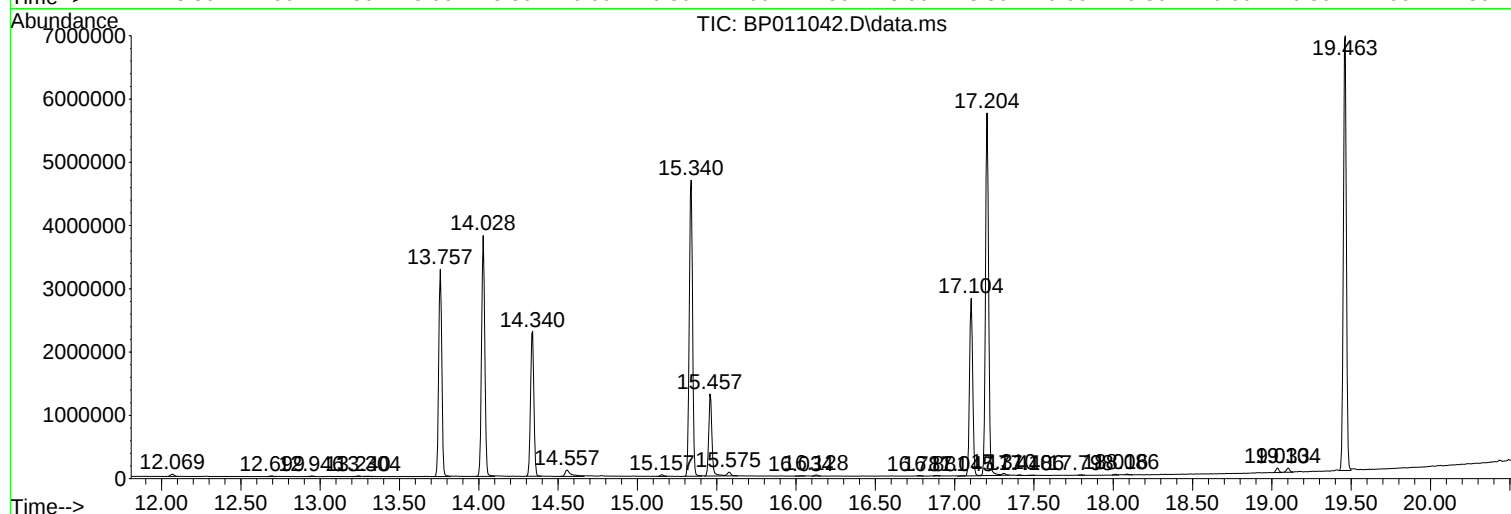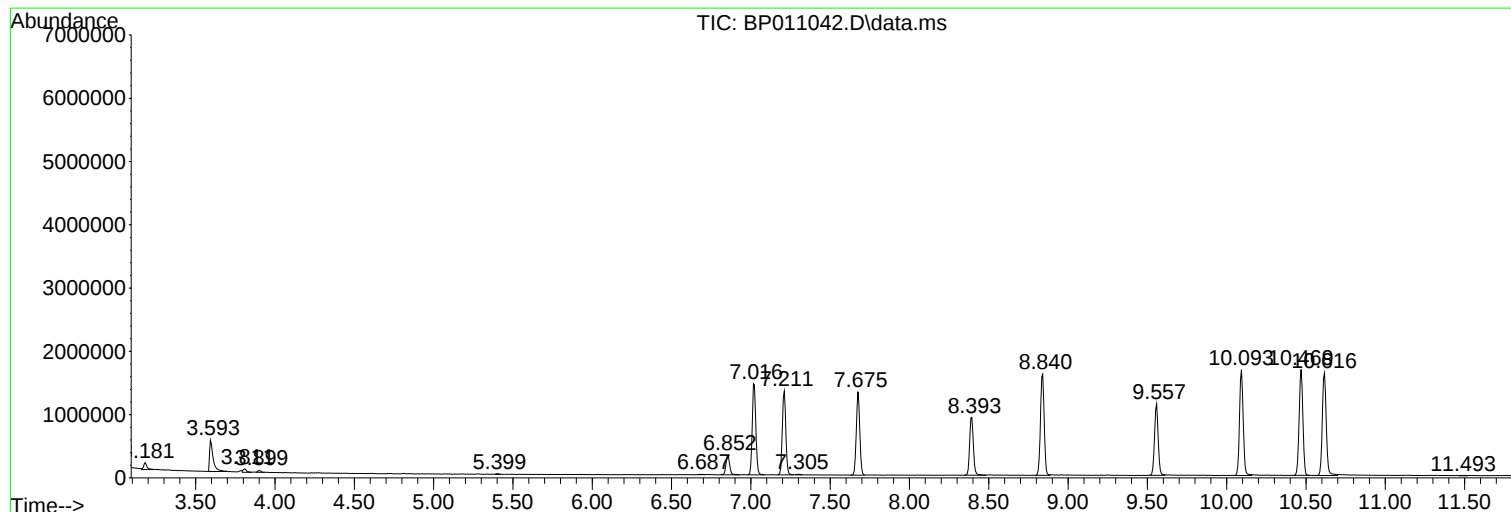

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011042.D
Acq On : 19 Jul 2022 20:44
Operator : CG/JU
Sample : N3753-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHQ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP071922\
Data File : BP011042.D
Acq On : 19 Jul 2022 20:44
Operator : CG/JU
Sample : N3753-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHQ3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc