
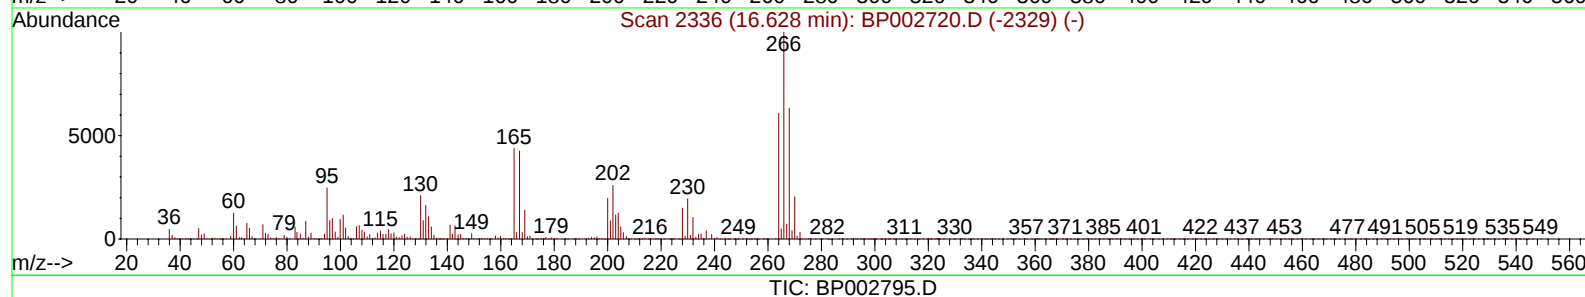
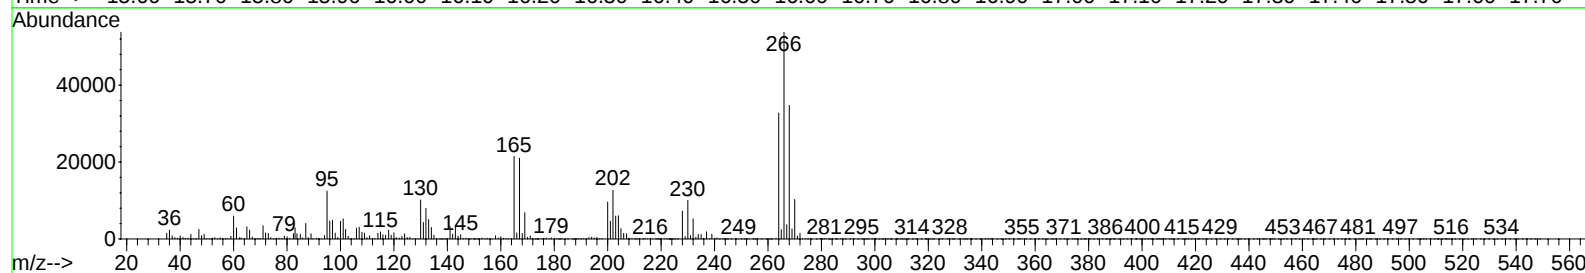


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP072020\
Data File : BP002795.D
Acq On : 20 Jul 2020 09:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 18:11:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 13 10:54:03 2020
Response via : Initial Calibration

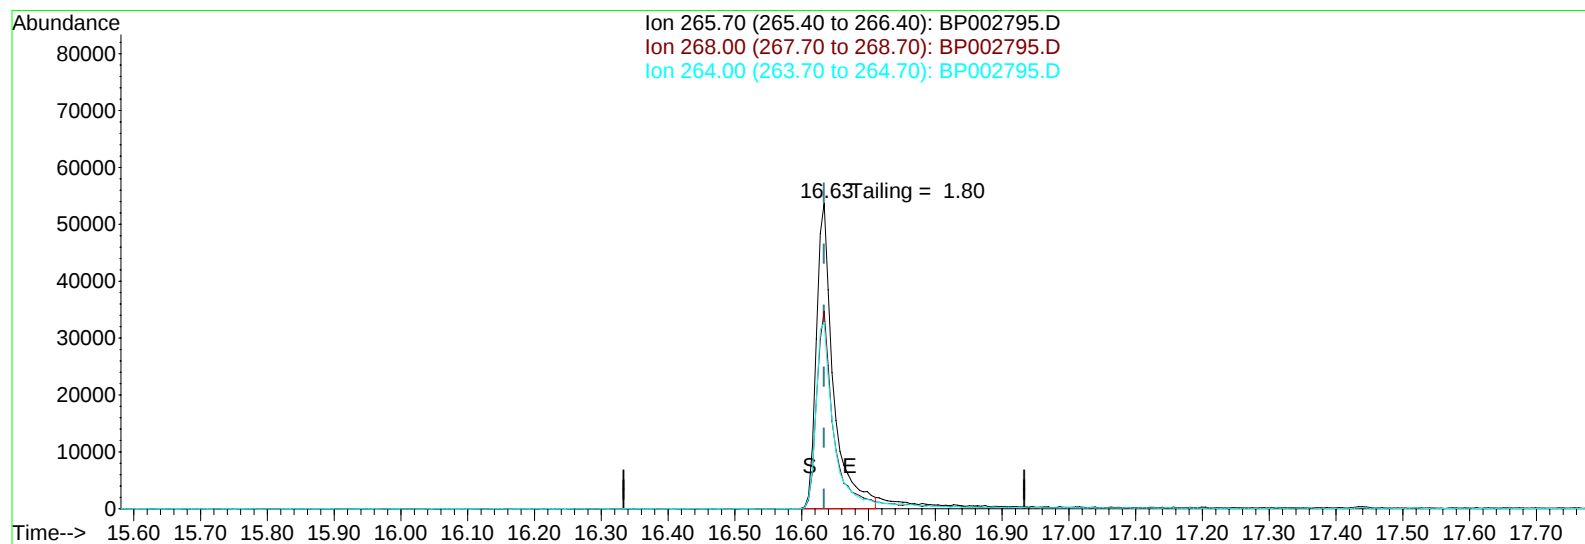

(70) Pentachlorophenol (C)




16.634min (+0.000) 230015.88ng

response 99946

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	64.61
264.00	60.70	60.93
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP072020\
 Data File : BP002795.D
 Acq On : 20 Jul 2020 09:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 18:11:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 13 10:54:03 2020
 Response via : Initial Calibration

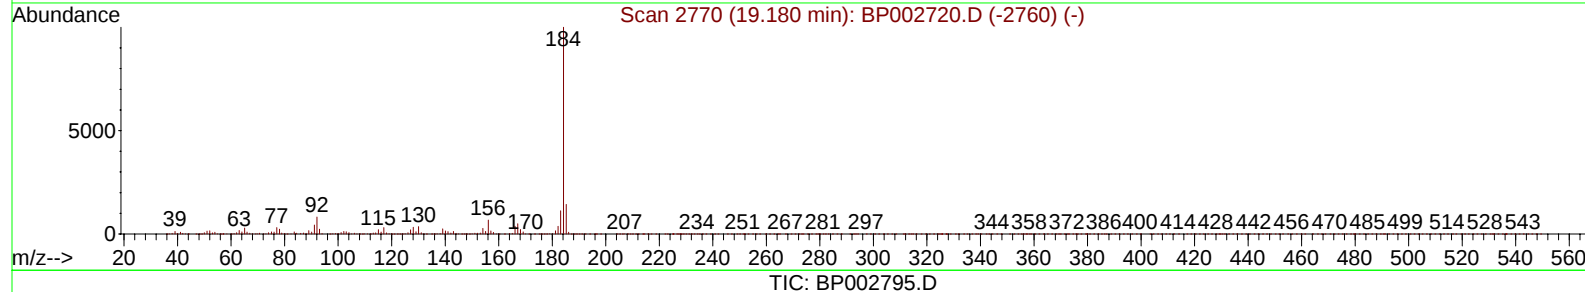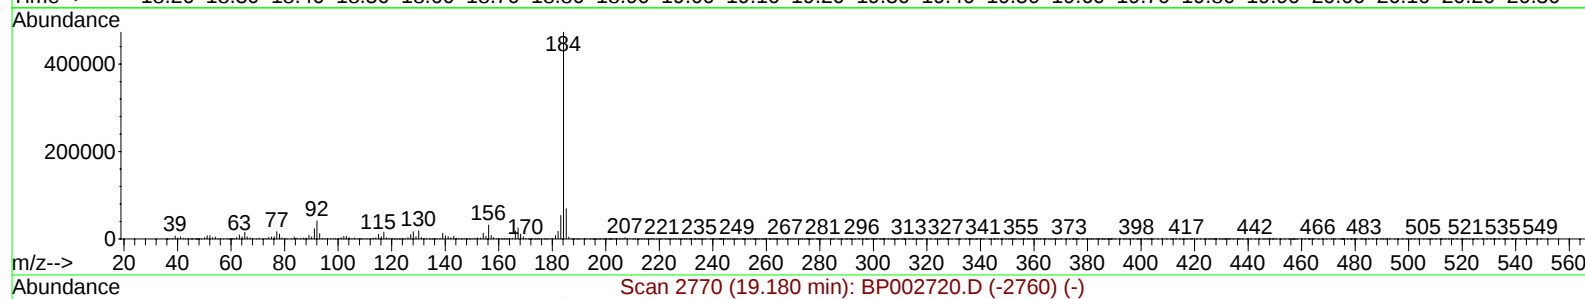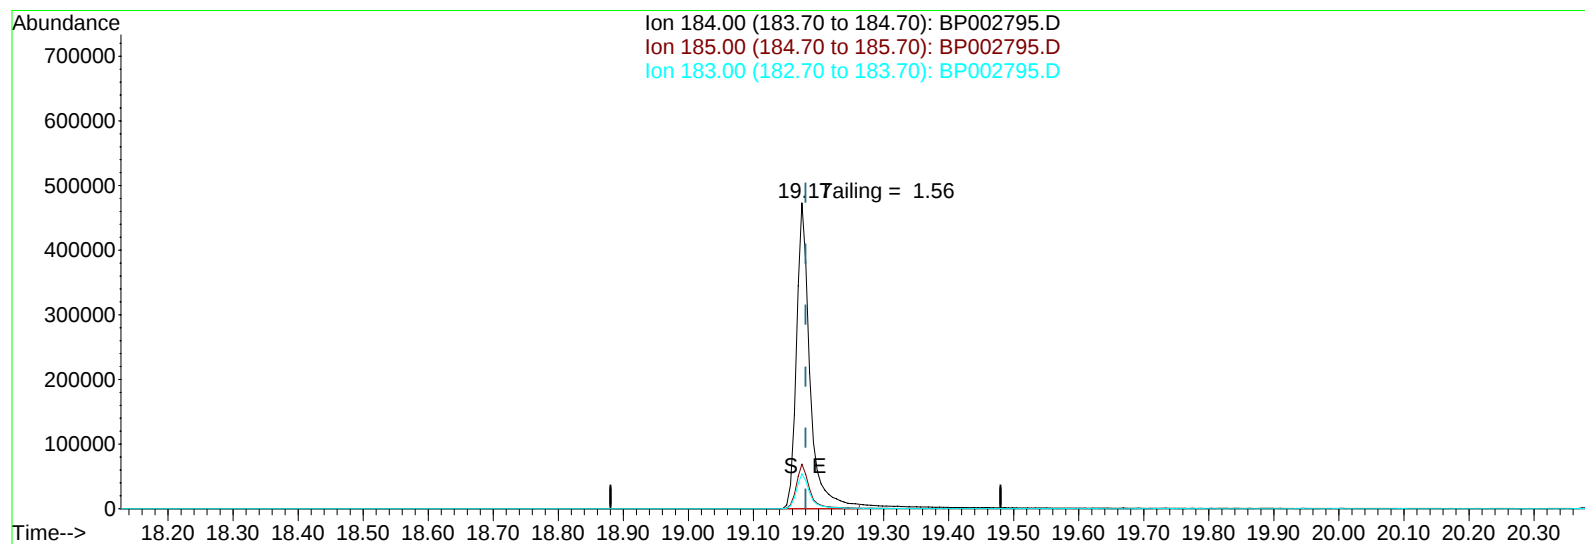

(77) Benzidine

19.175min (-0.006) 67804.26ng

response 709238

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	14.62
183.00	11.20	11.40
0.00	0.00	0.00