

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072021\
 Data File : BP006257.D
 Acq On : 20 Jul 2021 18:54
 Operator : CG/JU
 Sample : PB137705BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB137705BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP006257.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.399	386	393	409	rBV	5488354	7736013	43.57%	10.469%
2	6.975	652	661	671	rBV	4868830	7564062	42.60%	10.236%
3	7.798	795	801	810	rBV	984711	1522221	8.57%	2.060%
4	8.957	988	998	1012	rBV	2976391	4769498	26.86%	6.454%
5	10.587	1267	1275	1282	rBV	1281308	2079927	11.71%	2.815%
6	13.057	1688	1695	1708	rBV	7786991	11369307	64.03%	15.386%
7	14.427	1921	1928	1935	rBV	1925566	2784891	15.68%	3.769%
8	15.922	2174	2182	2199	rBV	5531177	7625248	42.94%	10.319%
9	17.180	2390	2396	2402	rBV	2387547	3286837	18.51%	4.448%
10	19.757	2829	2834	2839	rBV	14220714	17756826	100.00%	24.030%
11	21.274	3088	3092	3097	rBV	2980586	3602042	20.29%	4.875%
12	23.627	3487	3492	3503	rVB	1991498	3797294	21.38%	5.139%




Sum of corrected areas: 73894166

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072021\
Data File : BP006257.D
Acq On : 20 Jul 2021 18:54
Operator : CG/JU
Sample : PB137705BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137705BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

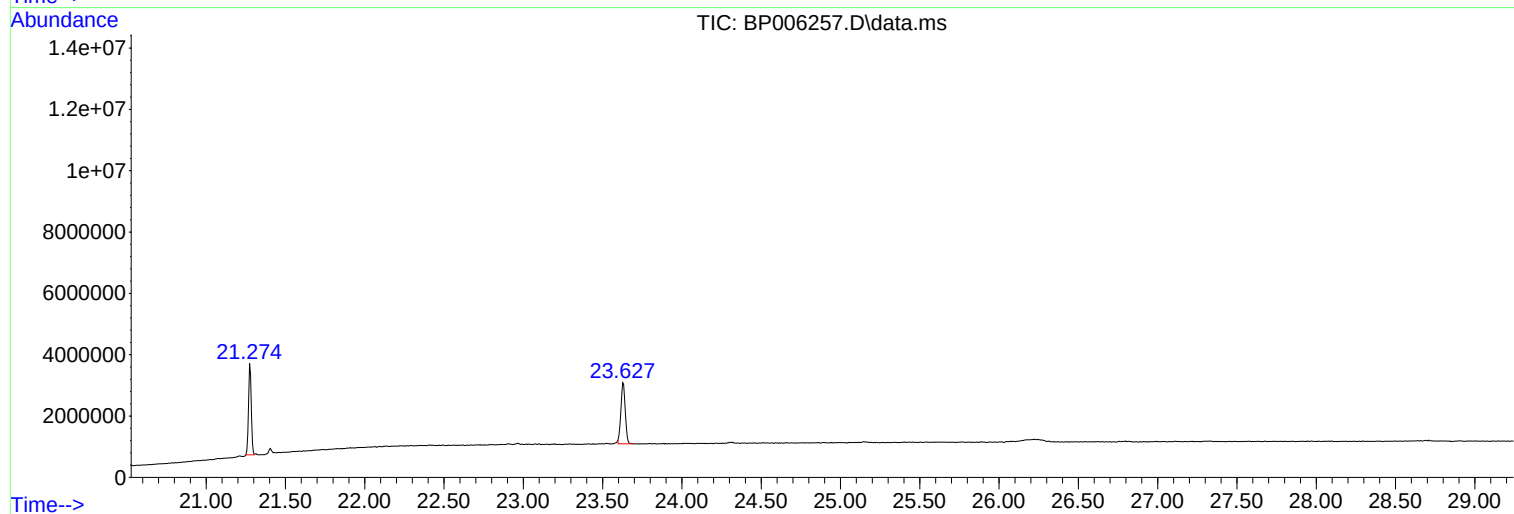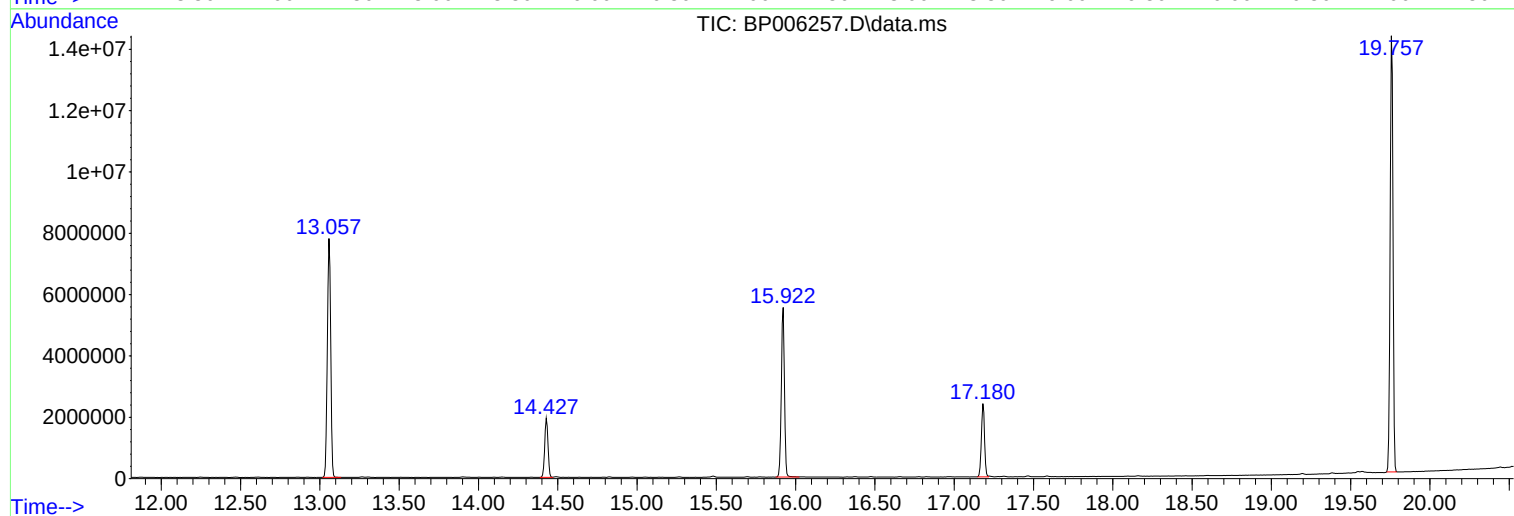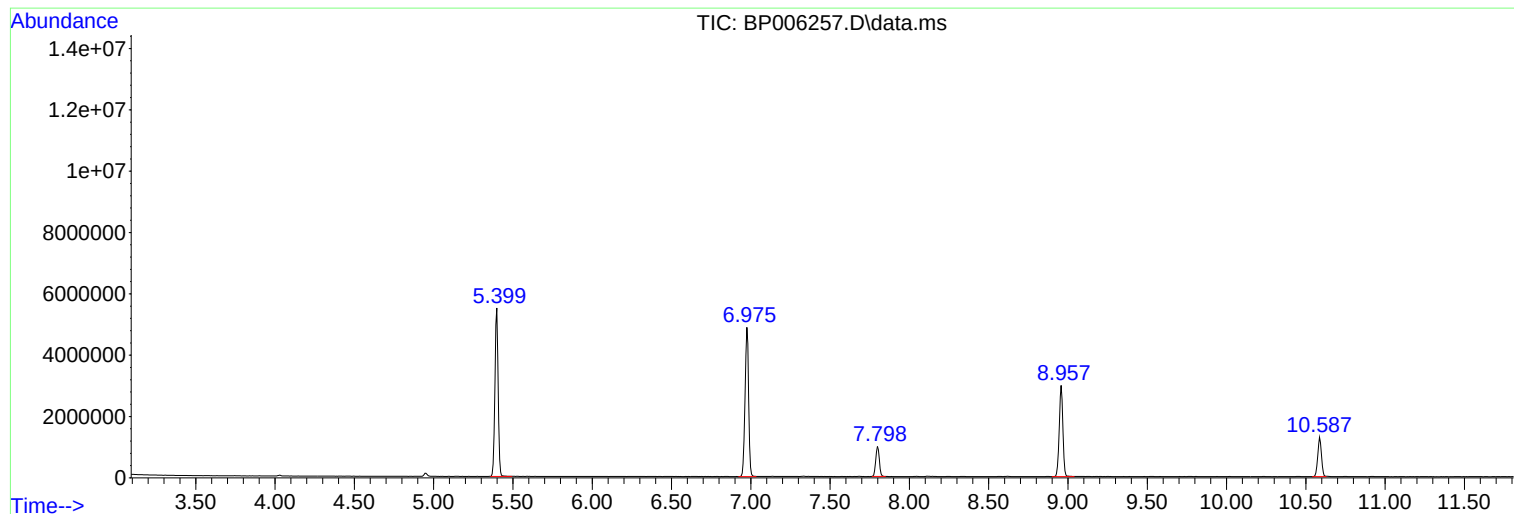

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072021\
Data File : BP006257.D
Acq On : 20 Jul 2021 18:54
Operator : CG/JU
Sample : PB137705BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137705BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072021\
Data File : BP006257.D
Acq On : 20 Jul 2021 18:54
Operator : CG/JU
Sample : PB137705BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB137705BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------