

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP072022\  
 Data File : BP011057.D  
 Acq On : 20 Jul 2022 15:38  
 Operator : CG/JU  
 Sample : SSTDCCC020  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 SSTD020708

Quant Time: Jul 21 00:43:37 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP071422.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Jul 19 03:25:54 2022  
 Response via : Initial Calibration

| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| -----                         |        |      |          |        |        |          |
| Internal Standards            |        |      |          |        |        |          |
| 1) 1,4-Dichlorobenzene-d4     | 7.675  | 152  | 498762   | 20.000 | ng/u1  | 0.00     |
| 20) Naphthalene-d8            | 10.469 | 136  | 2093338  | 20.000 | ng/u1  | # 0.00   |
| 38) Acenaphthene-d10          | 14.339 | 164  | 1188528  | 20.000 | ng/u1  | 0.00     |
| 64) Phenanthrene-d10          | 17.104 | 188  | 2353808  | 20.000 | ng/u1  | # 0.00   |
| 79) Chrysene-d12              | 21.233 | 240  | 2215547  | 20.000 | ng/u1  | # 0.00   |
| 88) Perylene-d12              | 23.586 | 264  | 2290994  | 20.000 | ng/u1  | 0.00     |
| System Monitoring Compounds   |        |      |          |        |        |          |
| 3) 1,4-Dioxane-d8             | 3.181  | 96   | 108684   | 7.856  | ng/uL  | 0.00     |
| 4) Pyridine-d5                | 3.587  | 84   | 684062   | 19.129 | ng/u1  | 0.00     |
| 7) Phenol-d5                  | 6.852  | 99   | 788316   | 19.255 | ng/u1  | 0.00     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.016  | 67   | 529032   | 20.095 | ng/u1  | 0.00     |
| 11) 2-Chlorophenol-d4         | 7.210  | 132  | 658301   | 19.899 | ng/u1  | 0.00     |
| 15) 4-Methylphenol-d8         | 8.393  | 113  | 630338   | 19.232 | ng/u1  | 0.00     |
| 21) Nitrobenzene-d5           | 8.840  | 128  | 310355   | 20.344 | ng/u1  | 0.00     |
| 24) 2-Nitrophenol-d4          | 9.557  | 143  | 296431   | 19.638 | ng/u1  | 0.00     |
| 28) 2,4-Dichlorophenol-d3     | 10.093 | 165  | 547064   | 19.817 | ng/u1  | 0.00     |
| 31) 4-Chloroaniline-d4        | 10.616 | 131  | 886732   | 19.484 | ng/u1  | 0.00     |
| 46) Dimethylphthalate-d6      | 13.757 | 166  | 1605595  | 19.766 | ng/u1  | 0.00     |
| 49) Acenaphthylene-d8         | 14.028 | 160  | 1936737  | 20.207 | ng/u1  | 0.00     |
| 54) 4-Nitrophenol-d4          | 14.557 | 143  | 297856   | 18.117 | ng/u1  | 0.00     |
| 60) Fluorene-d10              | 15.339 | 176  | 1349891  | 19.550 | ng/u1  | 0.00     |
| 65) 4,6-Dinitro-2-methylph... | 15.463 | 200  | 206343   | 17.716 | ng/u1  | 0.00     |
| 73) Anthracene-d10            | 17.204 | 188  | 2008327  | 20.070 | ng/u1  | 0.00     |
| 81) Pyrene-d10                | 19.463 | 212  | 2278089  | 19.578 | ng/u1  | 0.00     |
| 92) Benzo(a)pyrene-d12        | 23.433 | 264  | 2172142  | 19.741 | ng/u1  | 0.00     |
| Target Compounds              |        |      |          |        |        |          |
|                               |        |      |          |        | Qvalue |          |
| 2) 1,4-Dioxane                | 3.216  | 88   | 111258   | 7.664  | ng/uL# | 82       |
| 5) Pyridine                   | 3.611  | 79   | 724760   | 19.667 | ng/u1# | 75       |
| 6) Benzaldehyde               | 6.822  | 77   | 326943   | 16.440 | ng/u1  | 97       |
| 8) Phenol                     | 6.881  | 94   | 848837   | 19.505 | ng/u1# | 86       |
| 10) Bis(2-Chloroethyl)ether   | 7.110  | 93   | 683902   | 19.801 | ng/u1  | 92       |
| 12) 2-Chlorophenol            | 7.240  | 128  | 688112   | 20.122 | ng/u1  | 94       |
| 13) 2-Methylphenol            | 8.128  | 108  | 621320   | 19.306 | ng/u1  | 100      |
| 14) 2,2'-oxybis(1-Chloropr... | 8.216  | 45   | 975608   | 20.652 | ng/u1# | 97       |
| 16) Acetophenone              | 8.504  | 105  | 986508   | 19.882 | ng/u1# | 89       |
| 17) N-Nitroso-di-n-propyla... | 8.493  | 70   | 504629   | 20.270 | ng/u1  | 92       |
| 18) 4-Methylphenol            | 8.457  | 108  | 672145   | 19.561 | ng/u1  | 98       |
| 19) Hexachloroethane          | 8.746  | 117  | 279772   | 20.674 | ng/u1# | 78       |
| 22) Nitrobenzene              | 8.881  | 77   | 734667   | 20.478 | ng/u1  | 92       |
| 23) Isophorone                | 9.410  | 82   | 1352206  | 20.139 | ng/u1  | 99       |
| 25) 2-Nitrophenol             | 9.587  | 139  | 339602   | 20.043 | ng/u1# | 85       |
| 26) 2,4-Dimethylphenol        | 9.657  | 107  | 728375   | 20.328 | ng/u1  | 97       |
| 27) Bis(2-Chloroethoxy)met... | 9.893  | 93   | 879258   | 19.788 | ng/u1  | 98       |
| 29) 2,4-Dichlorophenol        | 10.116 | 162  | 567534   | 19.863 | ng/u1  | 99       |
| 30) Naphthalene               | 10.516 | 128  | 2111119  | 19.790 | ng/u1  | 99       |
| 32) 4-Chloroaniline           | 10.640 | 127  | 882992   | 19.615 | ng/u1  | 99       |
| 33) Hexachlorobutadiene       | 10.804 | 225  | 329653   | 19.820 | ng/u1  | 96       |
| 34) Caprolactam               | 11.434 | 113  | 254827   | 25.448 | ng/u1  | 96       |
| 35) 4-Chloro-3-methylphenol   | 11.775 | 107  | 643621   | 19.932 | ng/u1  | 97       |
| 36) 2-Methylnaphthalene       | 12.140 | 142  | 1367569  | 19.775 | ng/u1  | 98       |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP072022\  
 Data File : BP011057.D  
 Acq On : 20 Jul 2022 15:38  
 Operator : CG/JU  
 Sample : SSTDCCC020  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 SSTD020708

Quant Time: Jul 21 00:43:37 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP071422.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Jul 19 03:25:54 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon | Response | Conc   | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|--------|--------|----------|
| 37) 1-Methylnaphthalene       | 12.363 | 142  | 1377322  | 19.869 | ng/ul# | 99       |
| 39) 1,2,4,5-Tetrachloroben... | 12.510 | 216  | 609717   | 19.451 | ng/ul# | 98       |
| 40) Hexachlorocyclopentadiene | 12.487 | 237  | 381945   | 19.672 | ng/ul  | 96       |
| 41) 2,4,6-Trichlorophenol     | 12.757 | 196  | 395572   | 19.162 | ng/ul  | 97       |
| 42) 2,4,5-Trichlorophenol     | 12.828 | 196  | 433956   | 19.670 | ng/ul  | 99       |
| 43) 1,1'-Biphenyl             | 13.163 | 154  | 1754039  | 19.779 | ng/ul# | 97       |
| 44) 2-Chloronaphthalene       | 13.204 | 162  | 1314203  | 19.730 | ng/ul  | 97       |
| 47) Dimethylphthalate         | 13.804 | 163  | 1595830  | 19.469 | ng/ul  | 98       |
| 48) 2,6-Dinitrotoluene        | 13.922 | 165  | 310535   | 20.926 | ng/ul  | 98       |
| 50) Acenaphthylene            | 14.057 | 152  | 2155435  | 20.042 | ng/ul  | 99       |
| 51) 3-Nitroaniline            | 14.257 | 138  | 286517   | 16.070 | ng/ul  | 92       |
| 52) Acenaphthene              | 14.404 | 153  | 1405966  | 19.734 | ng/ul  | 98       |
| 53) 2,4-Dinitrophenol         | 14.457 | 184  | 159883   | 18.416 | ng/ul  | 90       |
| 55) 4-Nitrophenol             | 14.569 | 109  | 256437   | 20.373 | ng/ul# | 78       |
| 56) Dibenzofuran              | 14.739 | 168  | 1927809  | 19.610 | ng/ul  | 99       |
| 57) 2,4-Dinitrotoluene        | 14.716 | 165  | 443284   | 20.942 | ng/ul  | 88       |
| 58) 2,3,4,6-Tetrachlorophenol | 14.969 | 232  | 333179   | 19.284 | ng/ul# | 87       |
| 59) Diethylphthalate          | 15.181 | 149  | 1660780  | 19.730 | ng/ul  | 97       |
| 61) Fluorene                  | 15.392 | 166  | 1552753  | 19.682 | ng/ul  | 100      |
| 62) 4-Chlorophenyl-phenyle... | 15.392 | 204  | 708076   | 19.495 | ng/ul  | 93       |
| 63) 4-Nitroaniline            | 15.428 | 138  | 274439   | 16.749 | ng/ul# | 75       |
| 66) 4,6-Dinitro-2-methylph... | 15.475 | 198  | 216893   | 18.152 | ng/ul  | 95       |
| 67) N-Nitrosodiphenylamine    | 15.610 | 169  | 1332342  | 19.815 | ng/ul  | 99       |
| 68) 4-Bromophenyl-phenylether | 16.298 | 248  | 419551   | 19.763 | ng/ul  | 97       |
| 69) Hexachlorobenzene         | 16.398 | 284  | 479673   | 19.468 | ng/ul# | 91       |
| 70) Atrazine                  | 16.580 | 200  | 454775   | 19.552 | ng/ul  | 98       |
| 71) Pentachlorophenol         | 16.751 | 266  | 300068   | 19.775 | ng/ul  | 96       |
| 72) Phenanthrene              | 17.145 | 178  | 2419134  | 19.727 | ng/ul  | 99       |
| 74) Anthracene                | 17.239 | 178  | 2447396  | 20.063 | ng/ul  | 100      |
| 75) 1,2,3,4-Tetrachloroben... | 13.128 | 216  | 641673   | 19.043 | ng/uL  | 98       |
| 76) Pentachlorobenzene        | 14.657 | 250  | 576917   | 19.531 | ng/uL  | 99       |
| 77) Carbazole                 | 17.522 | 167  | 2289306  | 20.052 | ng/ul  | 100      |
| 78) Di-n-butylphthalate       | 18.086 | 149  | 2858302  | 20.028 | ng/ul  | 99       |
| 80) Fluoranthene              | 19.133 | 202  | 2771579  | 20.365 | ng/ul# | 86       |
| 82) Pyrene                    | 19.492 | 202  | 2820439  | 20.087 | ng/ul# | 82       |
| 83) Butylbenzylphthalate      | 20.386 | 149  | 1293884  | 20.656 | ng/ul  | 96       |
| 84) 3,3'-Dichlorobenzidine    | 21.157 | 252  | 703313   | 17.928 | ng/ul# | 97       |
| 85) Benzo(a)anthracene        | 21.216 | 228  | 2692984  | 19.959 | ng/ul  | 98       |
| 86) Bis(2-ethylhexyl)phtha... | 21.157 | 149  | 1954641  | 20.914 | ng/ul# | 96       |
| 87) Chrysene                  | 21.268 | 228  | 2582873  | 19.495 | ng/ul  | 99       |
| 89) Di-n-octyl phthalate      | 22.068 | 149  | 3261113  | 21.225 | ng/ul  | 100      |
| 90) Benzo(b)fluoranthene      | 22.868 | 252  | 2805775  | 19.835 | ng/ul# | 95       |
| 91) Benzo(k)fluoranthene      | 22.915 | 252  | 2595083  | 19.530 | ng/ul# | 93       |
| 93) Benzo(a)pyrene            | 23.480 | 252  | 2684759  | 19.762 | ng/ul# | 94       |
| 94) Indeno(1,2,3-cd)pyrene    | 26.021 | 276  | 3108916  | 19.692 | ng/ul# | 88       |
| 95) Dibenzo(a,h)anthracene    | 26.045 | 278  | 2693167  | 19.714 | ng/ul# | 90       |
| 96) Benzo(g,h,i)perylene      | 26.768 | 276  | 2654801  | 19.744 | ng/ul# | 86       |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP072022\  
 Data File : BP011057.D  
 Acq On : 20 Jul 2022 15:38  
 Operator : CG/JU  
 Sample : SSTDCCC020  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 BNA\_P  
 ClientSampleId :  
 SSTD020708

Quant Time: Jul 21 00:43:37 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\SFAM-EPA-BP071422.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Jul 19 03:25:54 2022  
 Response via : Initial Calibration




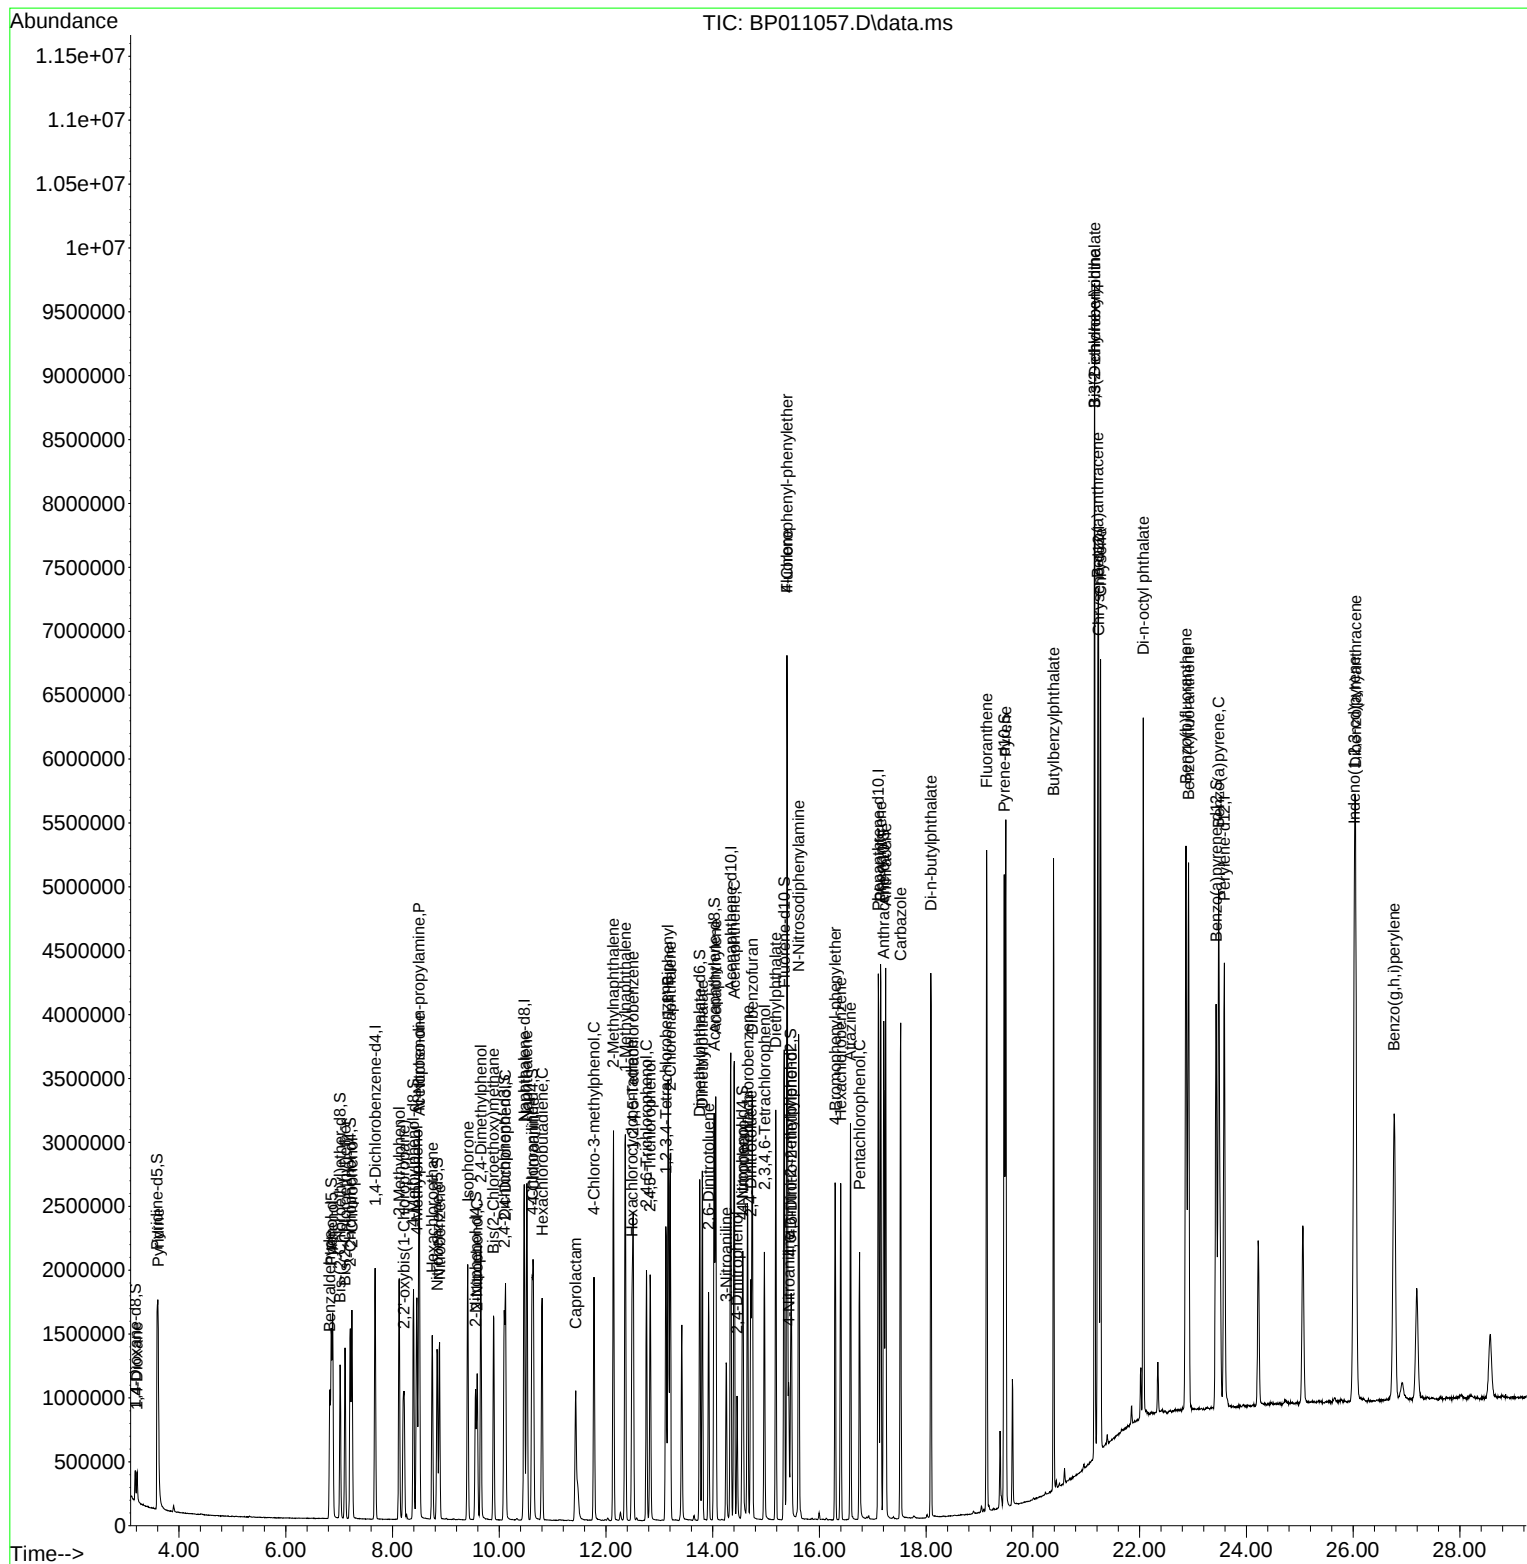




#2  
 1,4-Dioxane  
 Concen: 7.664 ng/uL  
 RT: 3.216 min Scan# 21  
 Delta R.T. -0.000 min  
 Lab File: BP011057.D  
 Acq: 20 Jul 2022 15:38




Instrument :  
 BNA\_P  
 ClientSampleId :  
 SSTD020708


Tgt Ion: 88 Resp: 111258  
 Ion Ratio Lower Upper  
 88 100  
 43 27.6 35.8 53.6#  
 58 72.5 68.1 102.1

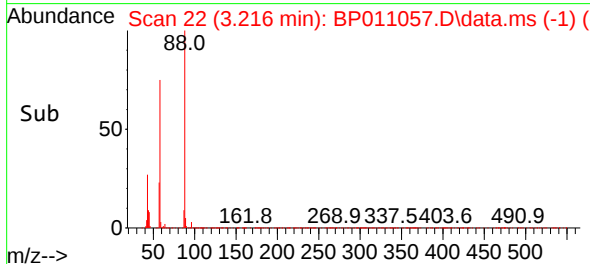

#5  
 Pyridine  
 Concen: 19.667 ng/uL  
 RT: 3.611 min Scan# 89  
 Delta R.T. -0.000 min  
 Lab File: BP011057.D  
 Acq: 20 Jul 2022 15:38

Tgt Ion: 79 Resp: 724760  
 Ion Ratio Lower Upper  
 79 100  
 52 77.1 83.8 125.8#  
 51 37.2 41.0 61.4#


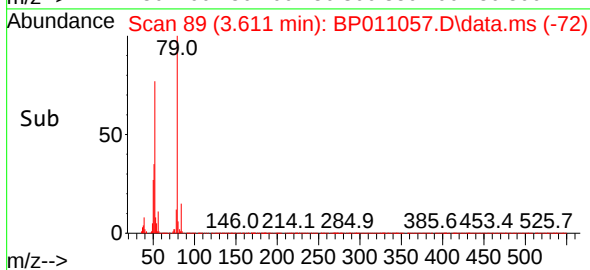

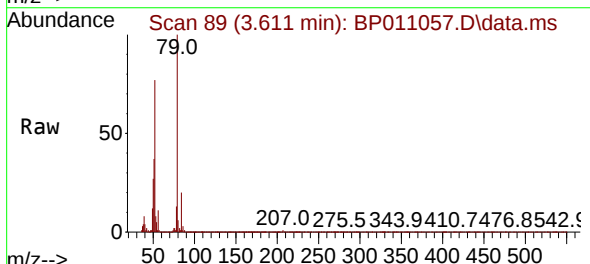




#6  
Benzaldehyde  
Concen: 16.440 ng/ul  
RT: 6.822 min Scan# 61  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion: 77 Resp: 326943  
Ion Ratio Lower Upper  
77 100  
105 99.4 76.0 114.0  
106 93.4 73.2 109.8



#8  
Phenol  
Concen: 19.505 ng/ul  
RT: 6.881 min Scan# 645  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion: 94 Resp: 848837  
Ion Ratio Lower Upper  
94 100  
65 28.0 27.4 41.2  
66 36.1 37.4 56.2#


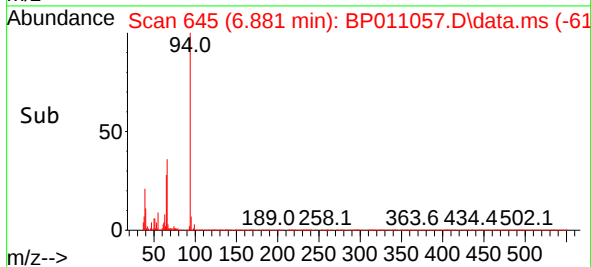

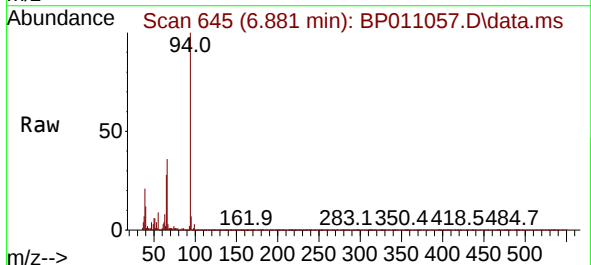




#10  
Bis(2-Chloroethyl)ether  
Concen: 19.801 ng/ul  
RT: 7.110 min Scan# 684  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion: 93 Resp: 683902  
Ion Ratio Lower Upper  
93 100  
63 80.8 72.4 108.6  
95 32.8 27.3 40.9



#12  
2-Chlorophenol  
Concen: 20.122 ng/ul  
RT: 7.240 min Scan# 706  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:128 Resp: 688112  
Ion Ratio Lower Upper  
128 100  
64 49.4 44.8 67.2  
130 31.6 25.8 38.6

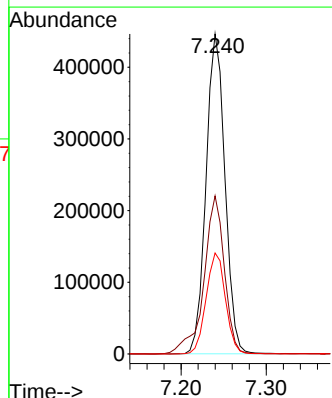



#13

2-Methylphenol

Concen: 19.306 ng/ul

RT: 8.128 min Scan# 81

Delta R.T. -0.000 min

Lab File: BP011057.D

Acq: 20 Jul 2022 15:38

Instrument :

BNA\_P

ClientSampleId :





SSTD020708

Tgt Ion:108 Resp: 621320

Ion Ratio Lower Upper

108 100

107 89.4 71.4 107.0

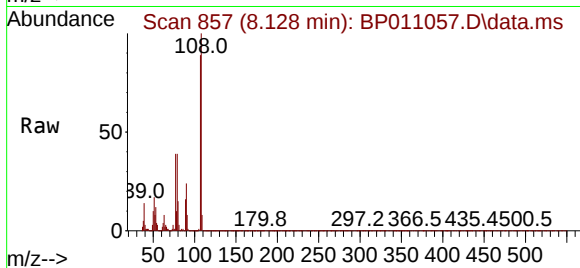

#14

2,2'-oxybis(1-Chloropropane)

Concen: 20.652 ng/ul

RT: 8.216 min Scan# 872

Delta R.T. -0.000 min

Lab File: BP011057.D

Acq: 20 Jul 2022 15:38




Tgt Ion: 45 Resp: 975608


Ion Ratio Lower Upper

45 100

77 13.7 11.2 16.8

79 10.9 6.9 10.3#


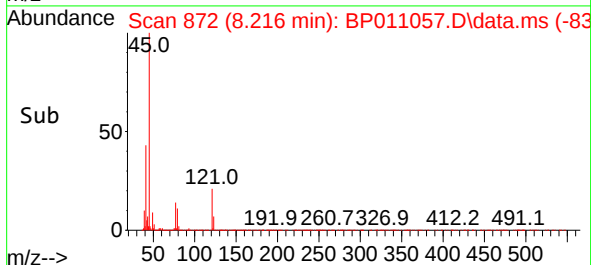
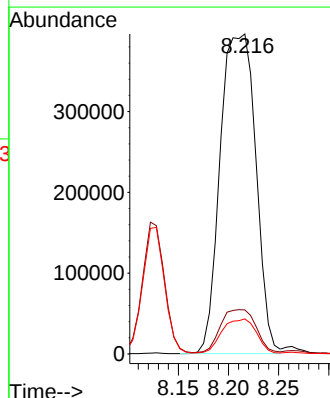
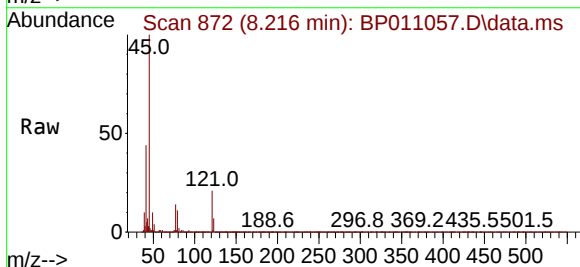




#16  
Acetophenone  
Concen: 19.882 ng/ul  
RT: 8.504 min Scan# 919  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:105 Resp: 986508  
Ion Ratio Lower Upper  
105 100  
77 77.0 67.5 101.3  
51 27.2 29.6 44.4#



#17  
N-Nitroso-di-n-propylamine  
Concen: 20.270 ng/ul  
RT: 8.493 min Scan# 919  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion: 70 Resp: 504629  
Ion Ratio Lower Upper  
70 100  
42 59.3 53.8 80.8  
101 10.2 7.8 11.6  
130 21.6 15.4 23.2









#18  
4-Methylphenol  
Concen: 19.561 ng/ul  
RT: 8.457 min Scan# 913  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:108 Resp: 672145  
Ion Ratio Lower Upper  
108 100  
107 112.1 88.3 132.5

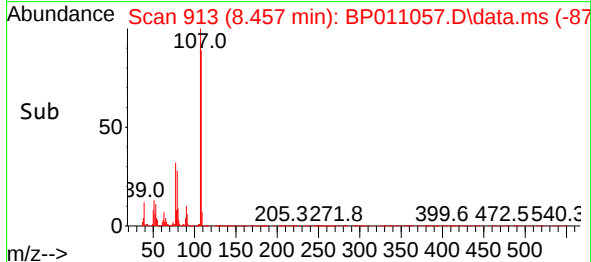

#19  
Hexachloroethane  
Concen: 20.674 ng/ul  
RT: 8.746 min Scan# 962  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:117 Resp: 279772  
Ion Ratio Lower Upper  
117 100  
201 85.6 85.7 128.5#  
199 51.7 57.4 86.0#


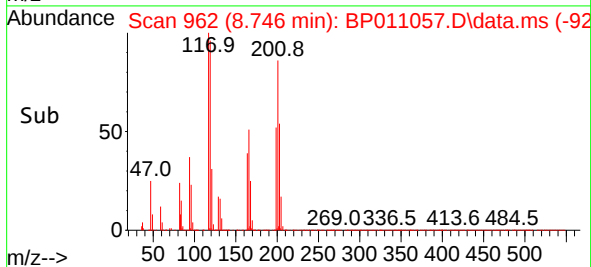

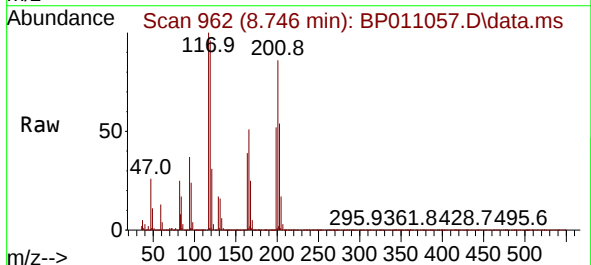




#22  
Nitrobenzene  
Concen: 20.478 ng/ul  
RT: 8.881 min Scan# 91  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion: 77 Resp: 734667  
Ion Ratio Lower Upper  
77 100  
123 45.5 31.5 47.3  
65 13.0 11.4 17.2



#23  
Isophorone  
Concen: 20.139 ng/ul  
RT: 9.410 min Scan# 1075  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion: 82 Resp: 1352206  
Ion Ratio Lower Upper  
82 100  
95 7.2 6.6 10.0  
138 17.5 13.8 20.6



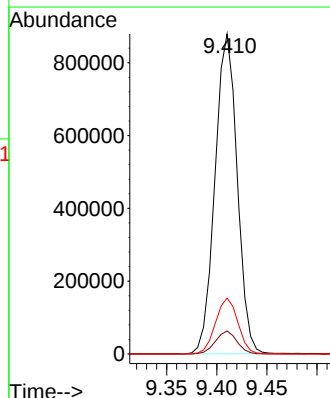





#25  
2-Nitrophenol  
Concen: 20.043 ng/ul  
RT: 9.587 min Scan# 1105  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:139 Resp: 339602  
Ion Ratio Lower Upper  
139 100  
65 54.9 54.2 81.4  
109 30.4 30.6 45.8#



#26  
2,4-Dimethylphenol  
Concen: 20.328 ng/ul  
RT: 9.657 min Scan# 1117  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:107 Resp: 728375  
Ion Ratio Lower Upper  
107 100  
121 50.6 39.1 58.7  
122 86.1 66.1 99.1









#27  
 Bis(2-Chloroethoxy)methane  
 Concen: 19.788 ng/ul  
 RT: 9.893 min Scan# 1158  
 Delta R.T. -0.006 min  
 Lab File: BP011057.D  
 Acq: 20 Jul 2022 15:38




Instrument :  
 BNA\_P  
 ClientSampleId :  
 SSTD020708


Tgt Ion: 93 Resp: 879258  
 Ion Ratio Lower Upper  
 93 100  
 95 32.2 26.6 39.8  
 123 11.3 7.8 11.8



#29  
 2,4-Dichlorophenol  
 Concen: 19.863 ng/ul  
 RT: 10.116 min Scan# 1195  
 Delta R.T. -0.006 min  
 Lab File: BP011057.D  
 Acq: 20 Jul 2022 15:38

Tgt Ion: 162 Resp: 567534  
 Ion Ratio Lower Upper  
 162 100  
 164 64.8 52.5 78.7  
 98 39.3 31.4 47.0




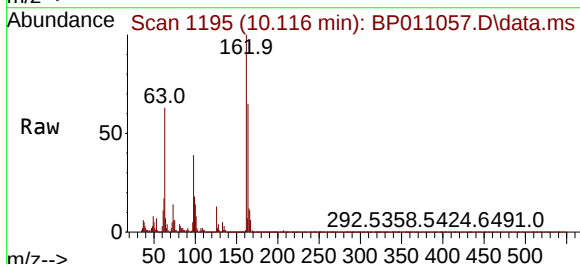




#30  
Naphthalene  
Concen: 19.790 ng/ul  
RT: 10.516 min Scan# 1263  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:128 Resp: 2111119  
Ion Ratio Lower Upper  
128 100  
129 10.9 8.7 13.1  
127 13.3 10.2 15.4



#32  
4-Chloroaniline  
Concen: 19.615 ng/ul  
RT: 10.640 min Scan# 1284  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:127 Resp: 882992  
Ion Ratio Lower Upper  
127 100  
129 32.1 26.2 39.2




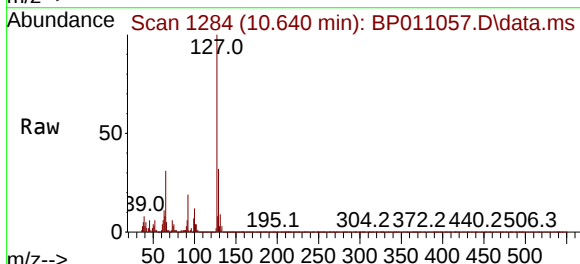




#33  
Hexachlorobutadiene  
Concen: 19.820 ng/ul  
RT: 10.804 min Scan# 11  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:225 Resp: 329653  
Ion Ratio Lower Upper  
225 100  
223 64.7 53.7 80.5  
227 65.0 49.4 74.2

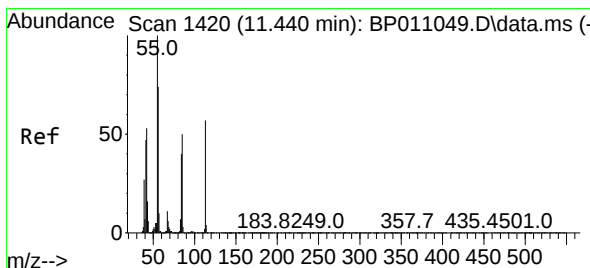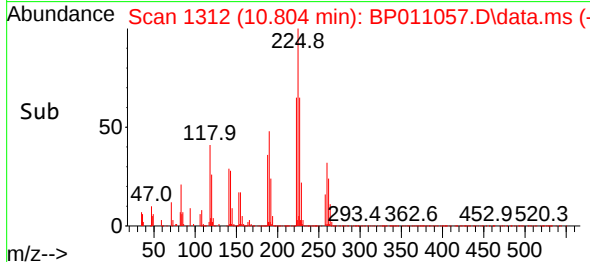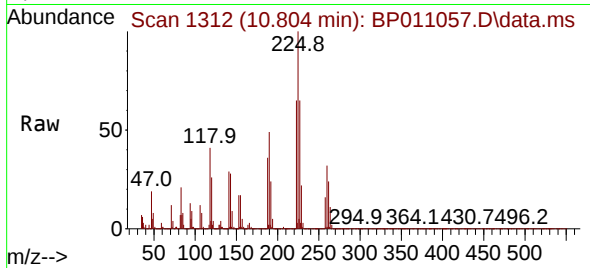

#34  
Caprolactam  
Concen: 25.448 ng/ul  
RT: 11.434 min Scan# 1419  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:113 Resp: 254827  
Ion Ratio Lower Upper  
113 100  
55 185.7 153.8 230.8  
56 134.9 110.2 165.4


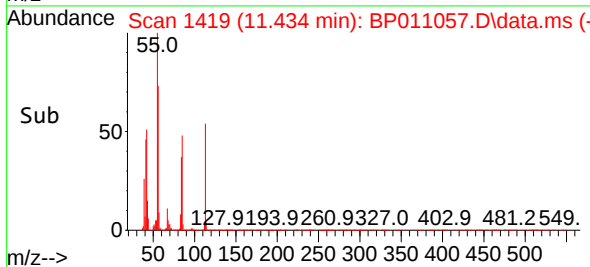

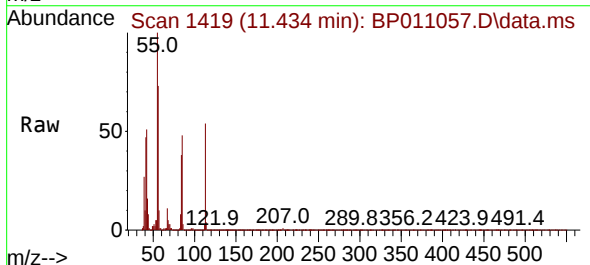




#35  
4-Chloro-3-methylphenol  
Concen: 19.932 ng/ul  
RT: 11.775 min Scan# 1478  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:107 Resp: 643621  
Ion Ratio Lower Upper  
107 100  
144 25.2 18.6 27.8  
142 76.8 59.6 89.4



#36  
2-Methylnaphthalene  
Concen: 19.775 ng/ul  
RT: 12.140 min Scan# 1539  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:142 Resp: 1367569  
Ion Ratio Lower Upper  
142 100  
141 89.9 70.1 105.1


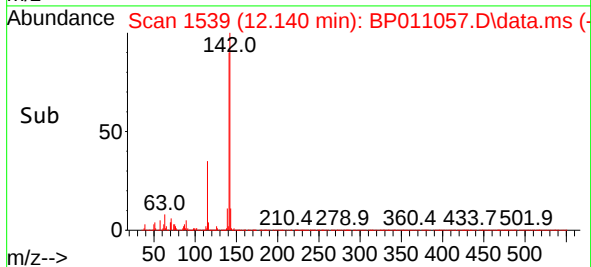

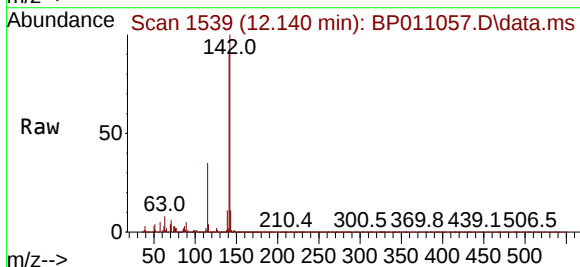




#37  
1-Methylnaphthalene  
Concen: 19.869 ng/ul  
RT: 12.363 min Scan# 11  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:142 Resp: 1377322  
Ion Ratio Lower Upper  
142 100  
141 92.7 73.3 109.9  
116 3.7 4.0 6.0#

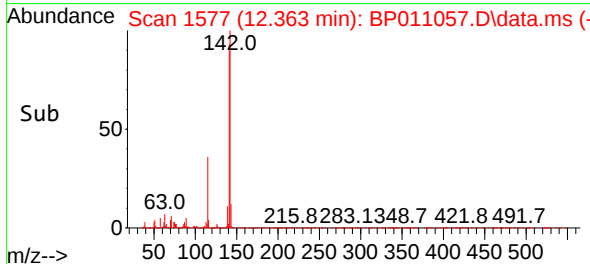

#39  
1,2,4,5-Tetrachlorobenzene  
Concen: 19.451 ng/ul  
RT: 12.510 min Scan# 1602  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:216 Resp: 609717  
Ion Ratio Lower Upper  
216 100  
214 79.7 63.0 94.6  
179 23.1 18.1 27.1  
108 20.9 13.6 20.4#


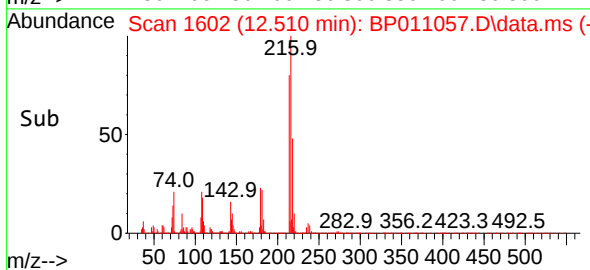

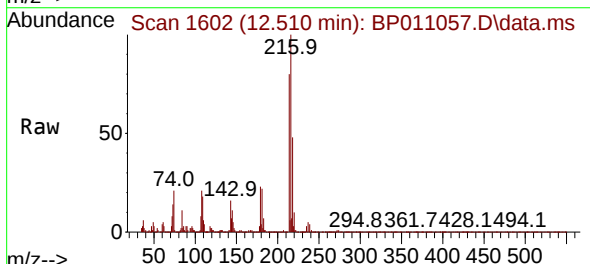




#40  
Hexachlorocyclopentadiene  
Concen: 19.672 ng/ul  
RT: 12.487 min Scan# 11  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:237 Resp: 381945  
Ion Ratio Lower Upper  
237 100  
235 63.1 52.8 79.2  
272 12.1 11.5 17.3



#41  
2,4,6-Trichlorophenol  
Concen: 19.162 ng/ul  
RT: 12.757 min Scan# 1644  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:196 Resp: 395572  
Ion Ratio Lower Upper  
196 100  
198 94.2 78.2 117.4  
200 29.6 25.0 37.6




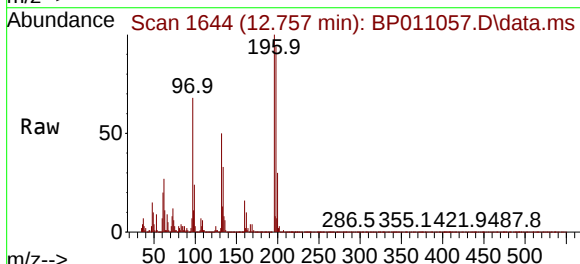




#42  
2,4,5-Trichlorophenol  
Concen: 19.670 ng/ul  
RT: 12.828 min Scan# 1  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:196 Resp: 433956  
Ion Ratio Lower Upper  
196 100  
198 94.8 77.0 115.4  
200 30.2 24.8 37.2



#43  
1,1'-Biphenyl  
Concen: 19.779 ng/ul  
RT: 13.163 min Scan# 1713  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:154 Resp: 1754039  
Ion Ratio Lower Upper  
154 100  
153 40.6 31.9 47.9  
76 15.1 9.2 13.8#

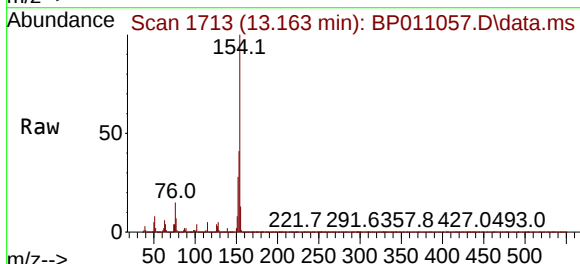



#44

2-Chloronaphthalene

Concen: 19.730 ng/ul

RT: 13.204 min Scan# 1

Delta R.T. -0.000 min

Lab File: BP011057.D

Acq: 20 Jul 2022 15:38

Instrument :

BNA\_P

ClientSampleId :

SSTD020708





Tgt Ion:162 Resp: 1314203

Ion Ratio Lower Upper

162 100

164 32.8 25.5 38.3

127 42.1 31.9 47.9

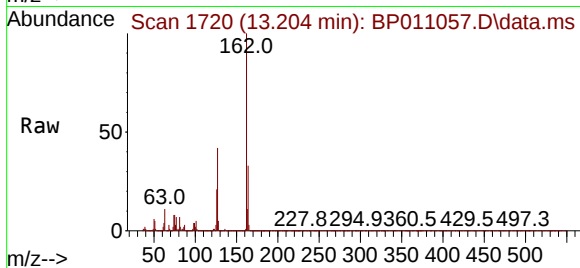

#47

Dimethylphthalate

Concen: 19.469 ng/ul

RT: 13.804 min Scan# 1822

Delta R.T. -0.006 min

Lab File: BP011057.D

Acq: 20 Jul 2022 15:38




Tgt Ion:163 Resp: 1595830


Ion Ratio Lower Upper

163 100

194 3.8 3.4 5.2

164 10.1 7.6 11.4









#48  
2,6-Dinitrotoluene  
Concen: 20.926 ng/ul  
RT: 13.922 min Scan# 1842  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:165 Resp: 310535  
Ion Ratio Lower Upper  
165 100  
89 63.9 52.9 79.3  
121 24.4 19.4 29.2



#50  
Acenaphthylene  
Concen: 20.042 ng/ul  
RT: 14.057 min Scan# 1865  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:152 Resp: 2155435  
Ion Ratio Lower Upper  
152 100  
151 20.1 16.5 24.7  
153 13.2 10.1 15.1









#51  
3-Nitroaniline  
Concen: 16.070 ng/ul  
RT: 14.257 min Scan# 1899  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:138 Resp: 286517  
Ion Ratio Lower Upper  
138 100  
108 11.9 11.0 16.4  
92 121.0 104.6 156.8



#52  
Acenaphthene  
Concen: 19.734 ng/ul  
RT: 14.404 min Scan# 1924  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:153 Resp: 1405966  
Ion Ratio Lower Upper  
153 100  
152 46.9 36.2 54.2  
154 87.3 70.8 106.2




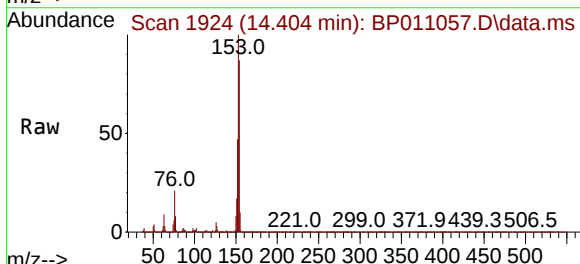




#53  
2,4-Dinitrophenol  
Concen: 18.416 ng/ul  
RT: 14.457 min Scan# 1933  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:184 Resp: 159883  
Ion Ratio Lower Upper  
184 100  
63 79.1 73.8 110.6  
154 66.4 57.2 85.8

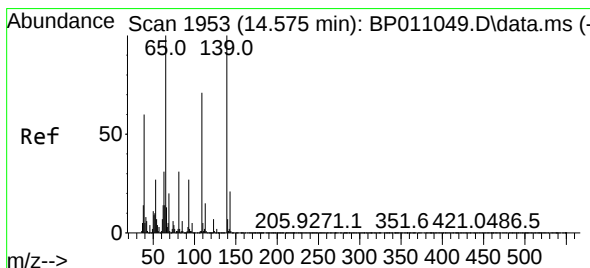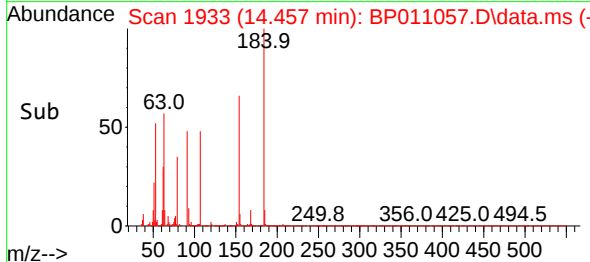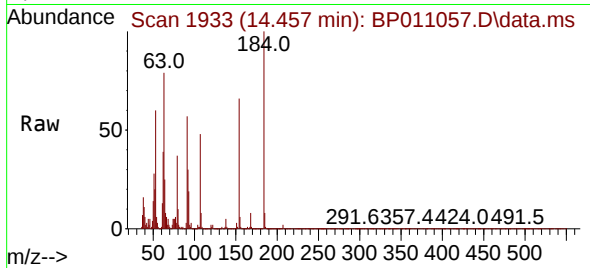

#55  
4-Nitrophenol  
Concen: 20.373 ng/ul  
RT: 14.569 min Scan# 1952  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:109 Resp: 256437  
Ion Ratio Lower Upper  
109 100  
139 140.1 75.6 113.4#  
65 138.9 107.6 161.4


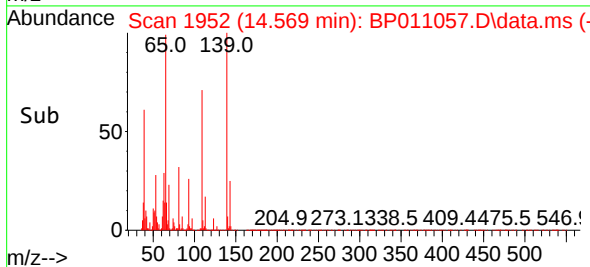

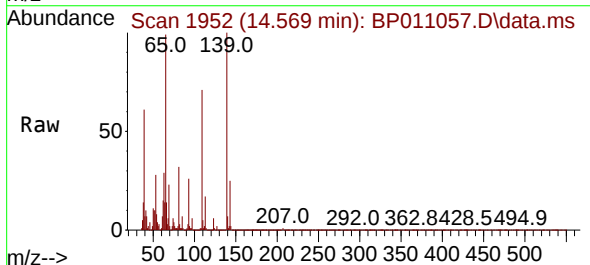




#56  
Dibenzofuran  
Concen: 19.610 ng/ul  
RT: 14.739 min Scan# 1981  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:168 Resp: 1927809  
Ion Ratio Lower Upper  
168 100  
139 40.4 32.8 49.2

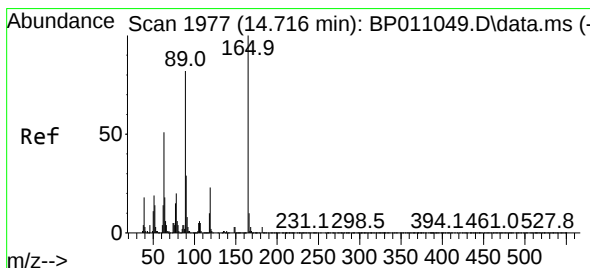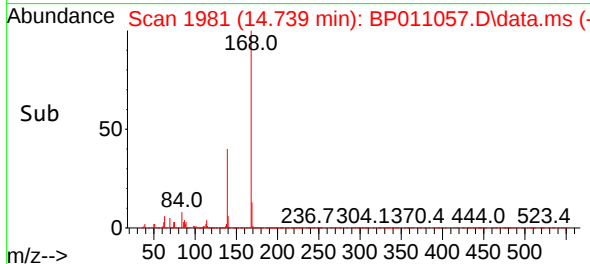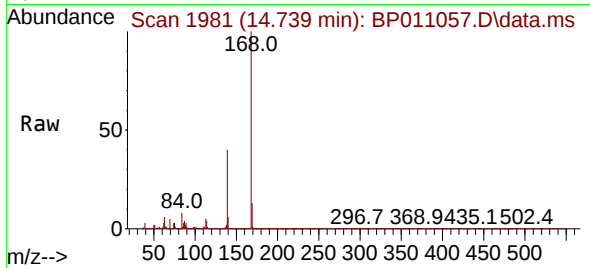

#57  
2,4-Dinitrotoluene  
Concen: 20.942 ng/ul  
RT: 14.716 min Scan# 1977  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:165 Resp: 443284  
Ion Ratio Lower Upper  
165 100  
63 49.4 47.0 70.6  
182 2.8 2.2 3.2


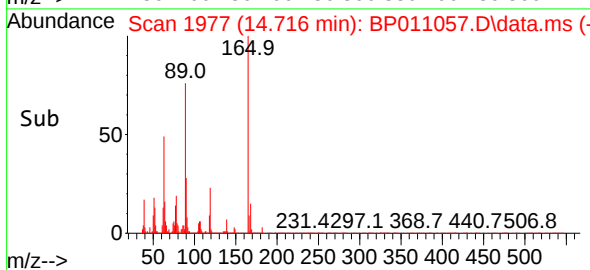

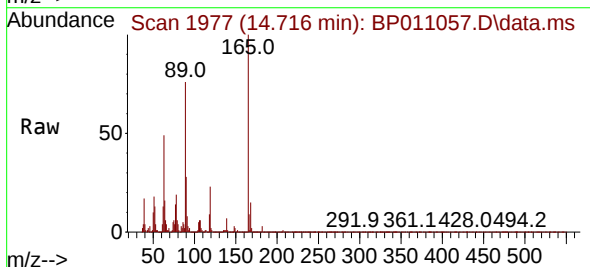




#58  
2,3,4,6-Tetrachlorophenol  
Concen: 19.284 ng/ul  
RT: 14.969 min Scan# 2021  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:232 Resp: 333179  
Ion Ratio Lower Upper  
232 100  
131 55.8 35.8 53.8#  
130 2.8 1.8 2.8#  
166 33.9 23.7 35.5



#59  
Diethylphthalate  
Concen: 19.730 ng/ul  
RT: 15.181 min Scan# 2056  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:149 Resp: 1660780  
Ion Ratio Lower Upper  
149 100  
177 20.5 17.6 26.4  
150 12.4 10.3 15.5


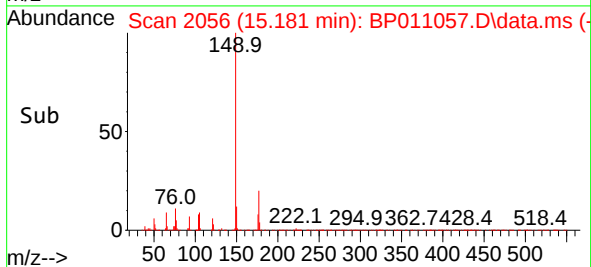

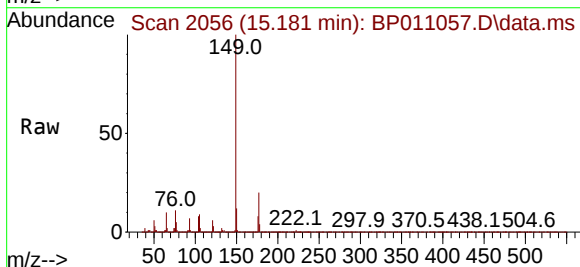




#61  
Fluorene  
Concen: 19.682 ng/ul  
RT: 15.392 min Scan# 2092  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:166 Resp: 1552753  
Ion Ratio Lower Upper  
166 100  
165 97.1 77.4 116.2  
167 13.2 10.8 16.2



#62  
4-Chlorophenyl-phenylether  
Concen: 19.495 ng/ul  
RT: 15.392 min Scan# 2092  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:204 Resp: 708076  
Ion Ratio Lower Upper  
204 100  
206 32.1 26.0 39.0  
141 69.5 49.3 73.9




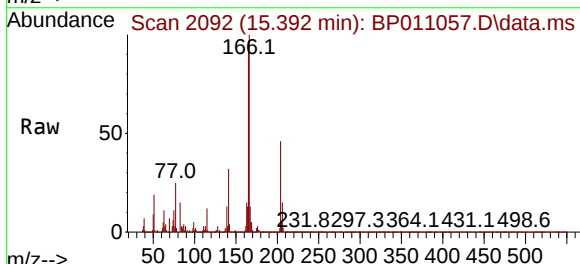




#63  
4-Nitroaniline  
Concen: 16.749 ng/ul  
RT: 15.428 min Scan# 2098  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:138 Resp: 274439  
Ion Ratio Lower Upper  
138 100  
92 51.2 46.2 69.2  
108 72.1 85.8 128.8#



#66  
4,6-Dinitro-2-methylphenol  
Concen: 18.152 ng/ul  
RT: 15.475 min Scan# 2106  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:198 Resp: 216893  
Ion Ratio Lower Upper  
198 100  
182 5.9 4.3 6.5  
77 32.8 23.7 35.5

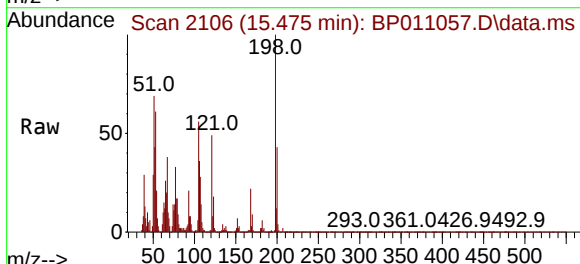



#67

N-Nitrosodiphenylamine

Concen: 19.815 ng/ul

RT: 15.610 min Scan# 2130

Delta R.T. -0.006 min

Lab File: BP011057.D

Acq: 20 Jul 2022 15:38

Instrument :

BNA\_P

ClientSampleId :

SSTD020708





Tgt Ion:169 Resp: 1332342

Ion Ratio Lower Upper

169 100

168 65.9 52.6 78.8

167 36.4 27.8 41.6

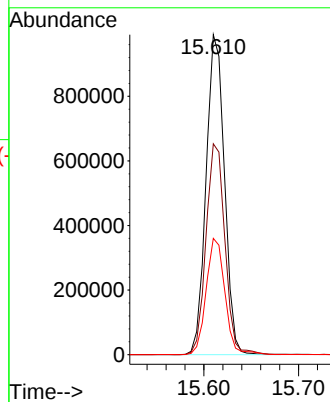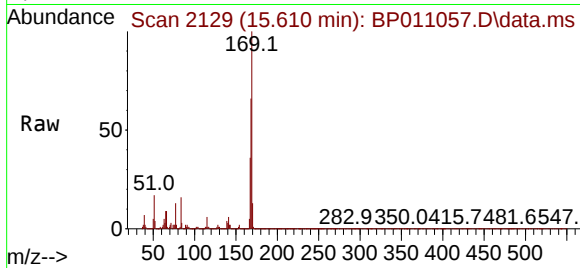

#68

4-Bromophenyl-phenylether

Concen: 19.763 ng/ul

RT: 16.298 min Scan# 2246

Delta R.T. -0.000 min

Lab File: BP011057.D

Acq: 20 Jul 2022 15:38




Tgt Ion:248 Resp: 419551


Ion Ratio Lower Upper

248 100

250 98.9 80.8 121.2

141 83.5 63.9 95.9


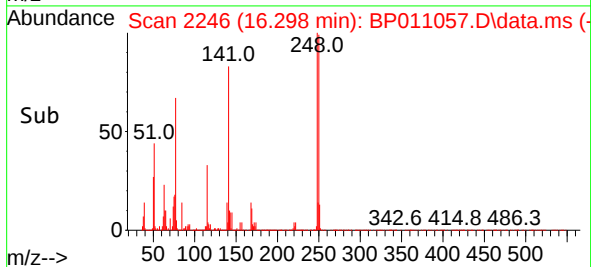

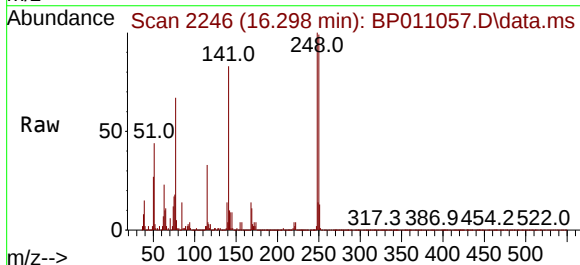




#69  
Hexachlorobenzene  
Concen: 19.468 ng/ul  
RT: 16.398 min Scan# 21  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:284 Resp: 479673  
Ion Ratio Lower Upper  
284 100  
142 44.3 27.8 41.6#  
249 32.2 25.4 38.2



#70  
Atrazine  
Concen: 19.552 ng/ul  
RT: 16.580 min Scan# 2294  
Delta R.T. -0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:200 Resp: 454775  
Ion Ratio Lower Upper  
200 100  
173 28.0 20.7 31.1  
215 47.2 38.6 57.8

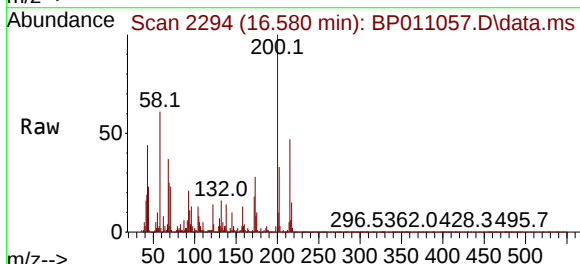

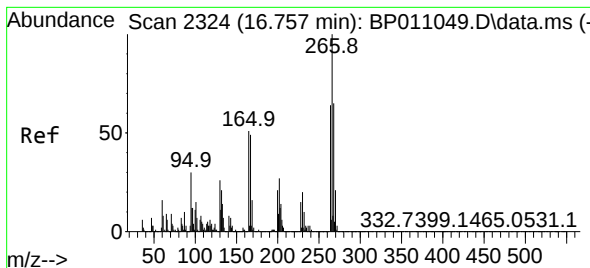

#71

Pentachlorophenol

Concen: 19.775 ng/ul

RT: 16.751 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP011057.D

Acq: 20 Jul 2022 15:38

Instrument :

BNA\_P

ClientSampleId :

SSTD020708





Tgt Ion:266 Resp: 300068

Ion Ratio Lower Upper

266 100

264 61.3 51.4 77.2

268 64.2 53.5 80.3

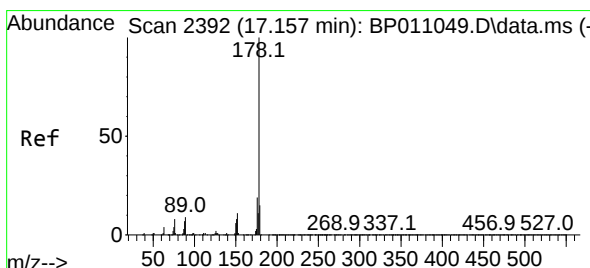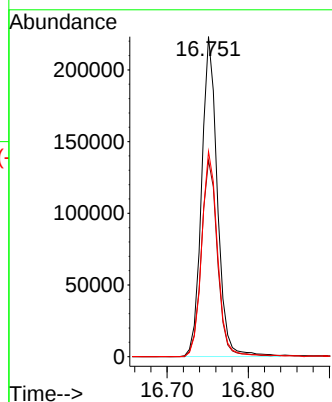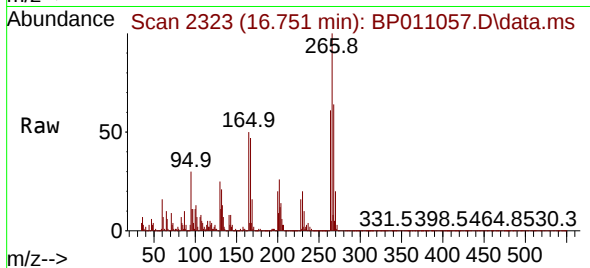

#72

Phenanthrene

Concen: 19.727 ng/ul

RT: 17.145 min Scan# 2390

Delta R.T. -0.006 min

Lab File: BP011057.D

Acq: 20 Jul 2022 15:38




Tgt Ion:178 Resp: 2419134


Ion Ratio Lower Upper

178 100

179 15.6 12.7 19.1

176 19.1 14.6 22.0

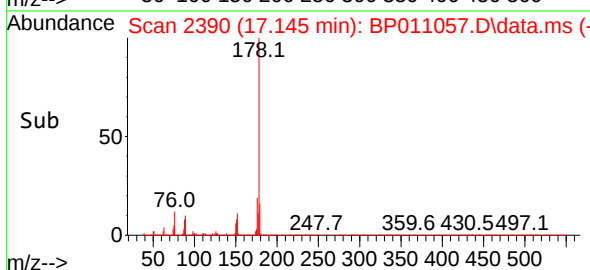



#74

Anthracene

Concen: 20.063 ng/uI

RT: 17.239 min Scan# 2407

Delta R.T. -0.000 min

Lab File: BP011057.D

Acq: 20 Jul 2022 15:38

Instrument :

BNA\_P

ClientSampleId :

SSTD020708





Tgt Ion:178 Resp: 2447396

Ion Ratio Lower Upper

178 100

179 15.2 12.2 18.2

176 18.4 14.5 21.7

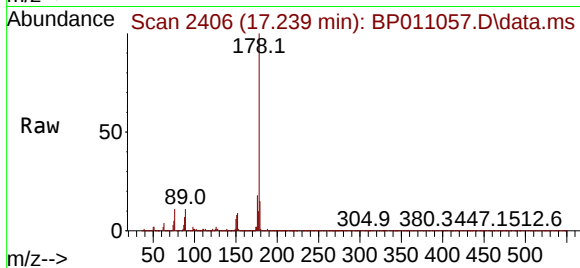

#75

1,2,3,4-Tetrachlorobenzene

Concen: 19.043 ng/uL

RT: 13.128 min Scan# 1707

Delta R.T. -0.000 min

Lab File: BP011057.D

Acq: 20 Jul 2022 15:38




Tgt Ion:216 Resp: 641673


Ion Ratio Lower Upper

216 100

214 78.5 65.0 97.4

218 48.3 39.1 58.7

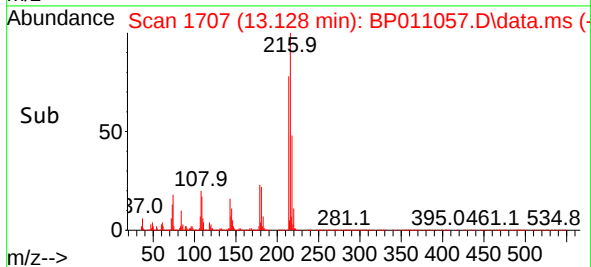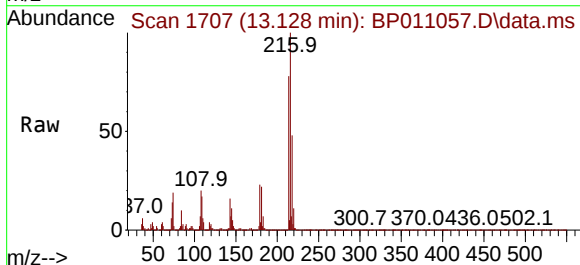



#76

Pentachlorobenzene

Concen: 19.531 ng/uL

RT: 14.657 min Scan# 1967

Delta R.T. -0.000 min

Lab File: BP011057.D

Acq: 20 Jul 2022 15:38

Instrument :

BNA\_P

ClientSampleId :

SSTD020708





Tgt Ion:250 Resp: 576917

Ion Ratio Lower Upper

250 100

248 62.7 49.8 74.6

252 64.9 51.2 76.8

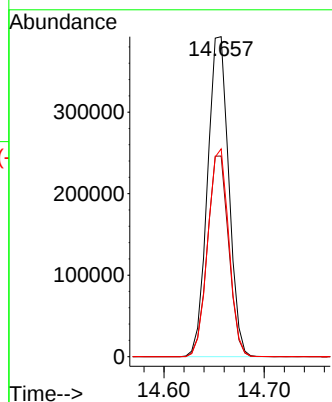

#77

Carbazole

Concen: 20.052 ng/uL

RT: 17.522 min Scan# 2454

Delta R.T. -0.000 min

Lab File: BP011057.D

Acq: 20 Jul 2022 15:38




Tgt Ion:167 Resp: 2289306


Ion Ratio Lower Upper

167 100

166 21.2 16.9 25.3

139 13.6 10.6 16.0





#78

Di-n-butylphthalate

Concen: 20.028 ng/ul

RT: 18.086 min Scan# 21

Delta R.T. -0.006 min

Lab File: BP011057.D

Acq: 20 Jul 2022 15:38

Instrument :

BNA\_P

ClientSampleId :

SSTD020708





Tgt Ion:149 Resp: 2858302

Ion Ratio Lower Upper

149 100

150 9.2 7.1 10.7

104 5.4 4.6 6.8

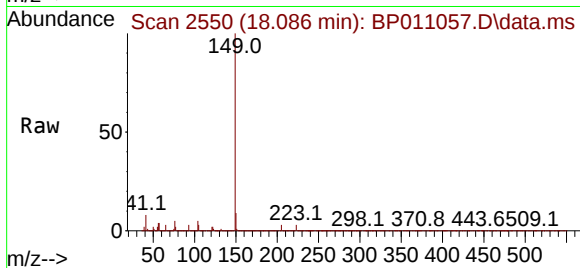

#80

Fluoranthene

Concen: 20.365 ng/ul

RT: 19.133 min Scan# 2728

Delta R.T. -0.000 min

Lab File: BP011057.D

Acq: 20 Jul 2022 15:38




Tgt Ion:202 Resp: 2771579


Ion Ratio Lower Upper

202 100

101 15.0 7.1 10.7#

100 11.1 5.7 8.5#





#82

Pyrene

Concen: 20.087 ng/ul

RT: 19.492 min Scan# 21

Delta R.T. -0.000 min

Lab File: BP011057.D

Acq: 20 Jul 2022 15:38

Instrument :

BNA\_P

ClientSampleId :

SSTD020708





Tgt Ion:202 Resp: 2820439

Ion Ratio Lower Upper

202 100

101 17.2 7.9 11.9#

100 14.2 6.7 10.1#



#83

Butylbenzylphthalate

Concen: 20.656 ng/ul

RT: 20.386 min Scan# 2941

Delta R.T. -0.000 min

Lab File: BP011057.D

Acq: 20 Jul 2022 15:38




Tgt Ion:149 Resp: 1293884


Ion Ratio Lower Upper

149 100

91 77.4 60.0 90.0

206 18.0 17.4 26.2



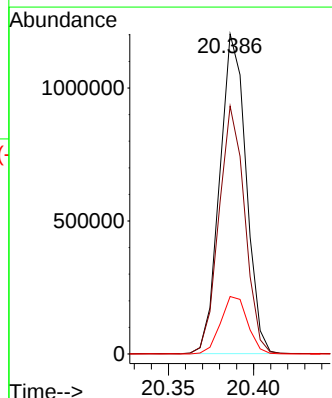





#84  
3,3'-Dichlorobenzidine  
Concen: 17.928 ng/ul  
RT: 21.157 min Scan# 3072  
Delta R.T. 0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:252 Resp: 703313  
Ion Ratio Lower Upper  
252 100  
254 65.5 51.0 76.4  
126 14.6 8.6 12.8#



#85  
Benzo(a)anthracene  
Concen: 19.959 ng/ul  
RT: 21.216 min Scan# 3082  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:228 Resp: 2692984  
Ion Ratio Lower Upper  
228 100  
229 19.7 15.0 22.4  
226 26.7 20.6 31.0









#86  
Bis(2-ethylhexyl)phthalate  
Concen: 20.914 ng/ul  
RT: 21.157 min Scan# 3072  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:149 Resp: 1954641  
Ion Ratio Lower Upper  
149 100  
167 26.2 22.6 33.8  
279 3.6 4.2 6.4#

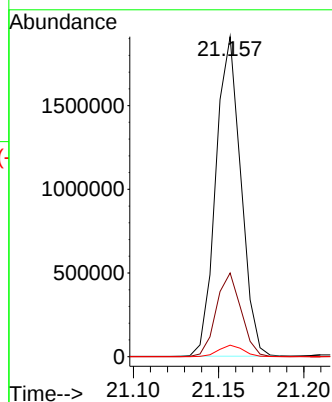

#87  
Chrysene  
Concen: 19.495 ng/ul  
RT: 21.268 min Scan# 3091  
Delta R.T. 0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:228 Resp: 2582873  
Ion Ratio Lower Upper  
228 100  
226 30.6 23.6 35.4  
229 19.7 15.6 23.4


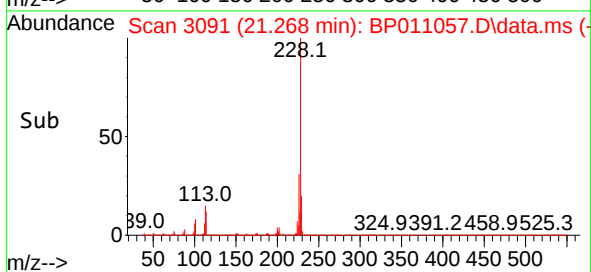
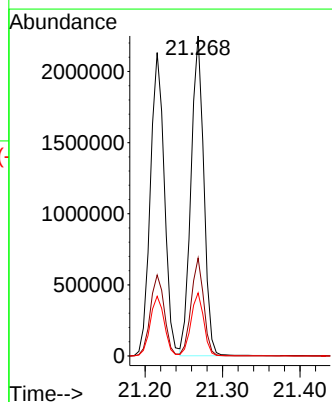





#89  
Di-n-octyl phthalate  
Concen: 21.225 ng/ul  
RT: 22.068 min Scan# 31  
Delta R.T. -0.000 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:149 Resp: 3261113

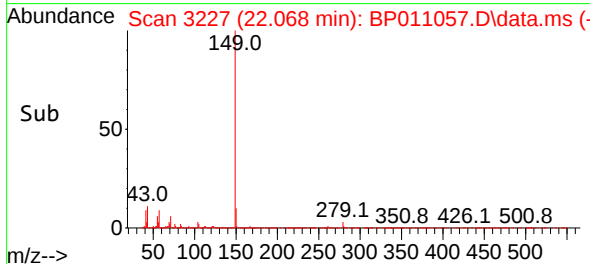

#90  
Benzo(b)fluoranthene  
Concen: 19.835 ng/ul  
RT: 22.868 min Scan# 3363  
Delta R.T. 0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:252 Resp: 2805775  
Ion Ratio Lower Upper  
252 100  
253 22.0 17.8 26.6  
125 13.5 6.2 9.2#


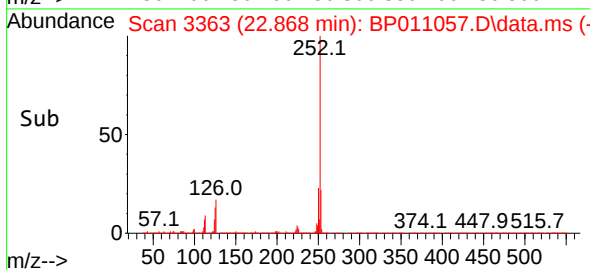

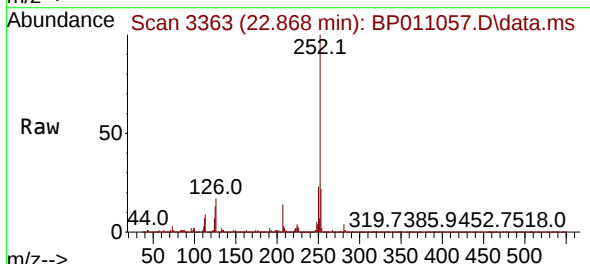




#91  
Benzo(k)fluoranthene  
Concen: 19.530 ng/ul  
RT: 22.915 min Scan# 3371  
Delta R.T. 0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38




Instrument :  
BNA\_P  
ClientSampleId :  
SSTD020708


Tgt Ion:252 Resp: 2595083  
Ion Ratio Lower Upper  
252 100  
253 22.5 17.0 25.4  
125 13.8 6.2 9.4#

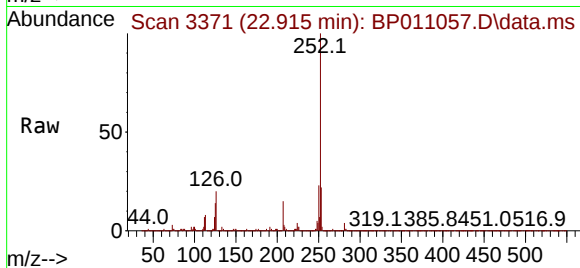

#93  
Benzo(a)pyrene  
Concen: 19.762 ng/ul  
RT: 23.480 min Scan# 3467  
Delta R.T. 0.006 min  
Lab File: BP011057.D  
Acq: 20 Jul 2022 15:38

Tgt Ion:252 Resp: 2684759  
Ion Ratio Lower Upper  
252 100  
253 22.1 17.4 26.0  
125 15.6 6.6 10.0#


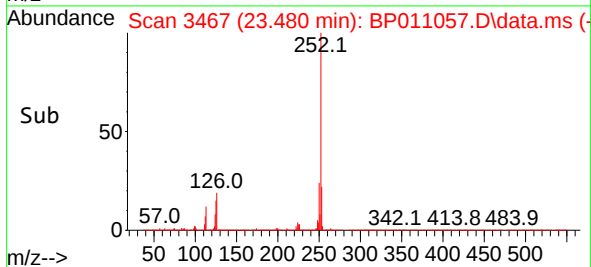

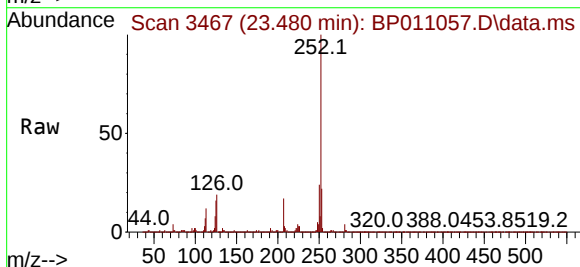




#94  
 Indeno(1,2,3-cd)pyrene  
 Concen: 19.692 ng/ul  
 RT: 26.021 min Scan# 3899  
 Delta R.T. 0.006 min  
 Lab File: BP011057.D  
 Acq: 20 Jul 2022 15:38




Instrument :  
 BNA\_P  
 ClientSampleId :  
 SST020708


Tgt Ion:276 Resp: 3108916  
 Ion Ratio Lower Upper  
 276 100  
 138 30.0 14.6 22.0#  
 277 24.8 19.6 29.4



#95  
 Dibenzo(a,h)anthracene  
 Concen: 19.714 ng/ul  
 RT: 26.045 min Scan# 3903  
 Delta R.T. 0.006 min  
 Lab File: BP011057.D  
 Acq: 20 Jul 2022 15:38

Tgt Ion:278 Resp: 2693167  
 Ion Ratio Lower Upper  
 278 100  
 139 21.8 9.4 14.2#  
 279 24.4 18.9 28.3





#96

Benzo(g,h,i)perylene

Concen: 19.744 ng/ul

RT: 26.768 min Scan# 40

Delta R.T. 0.006 min

Lab File: BP011057.D


Acq: 20 Jul 2022 15:38

Instrument :

BNA\_P

ClientSampleId :

SSTD020708

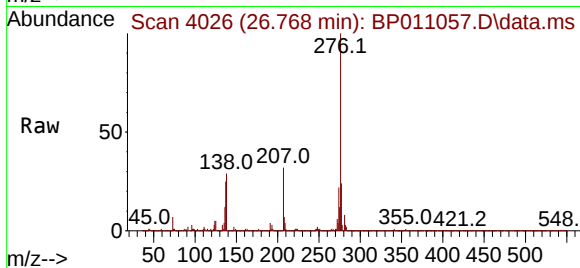

Tgt Ion:276 Resp: 2654801

Ion Ratio Lower Upper

276 100

138 29.0 12.7 19.1#

277 24.1 18.2 27.4

