




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
Data File : BP011055.D
Acq On : 20 Jul 2022 14:29
Operator : CG/JU
Sample : N3739-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0B39

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/21/2022
Supervised By :mohammad ahmed 07/21/2022

Quant Time: Jul 21 00:43:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 19 03:25:54 2022
Response via : Initial Calibration

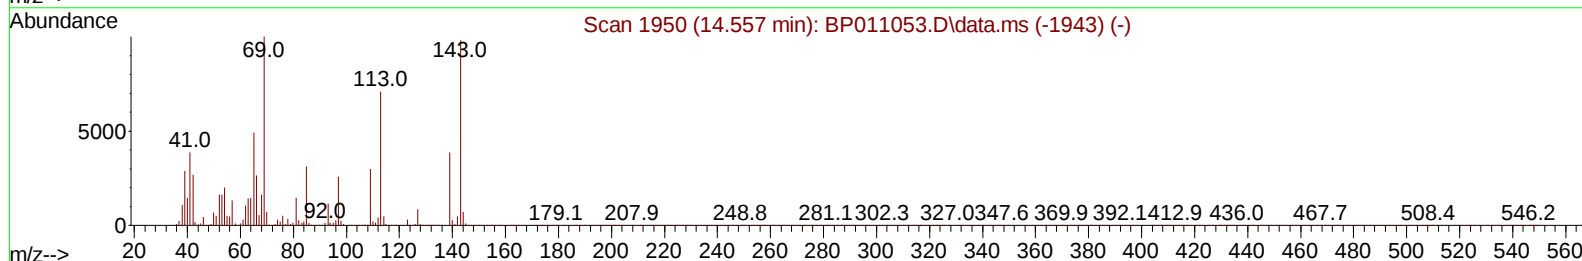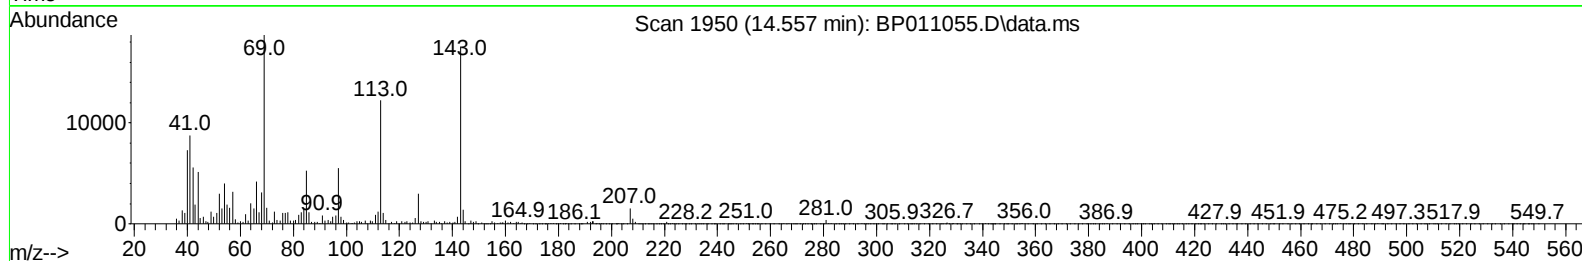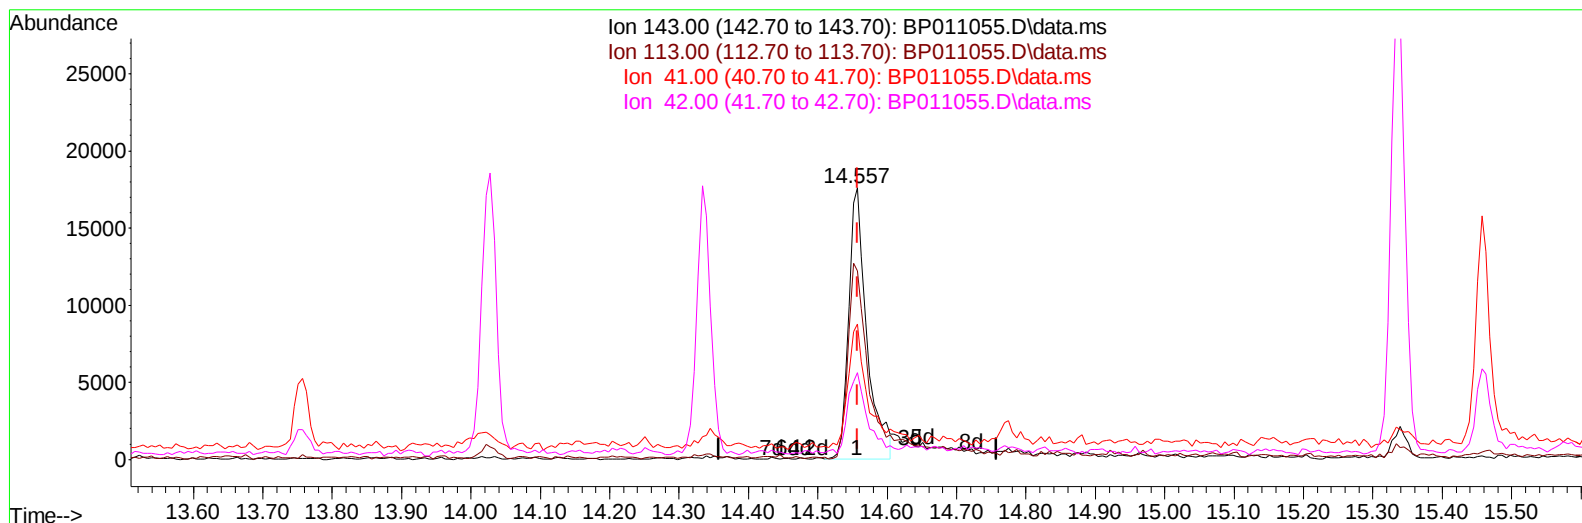

TIC: BP011055.D\data.ms

(54) 4-Nitrophenol-d4 (S)**14.557min (-0.000) 3.32 ng/u1****response 32118**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.50	69.48#
41.00	59.00	49.82
42.00	41.10	31.91#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
 Data File : BP011055.D
 Acq On : 20 Jul 2022 14:29
 Operator : CG/JU
 Sample : N3739-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0B39

Manual IntegrationsAPPROVED

Quant Time: Jul 21 00:43:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 19 03:25:54 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/21/2022
 Supervised By :mohammad ahmed 07/21/2022

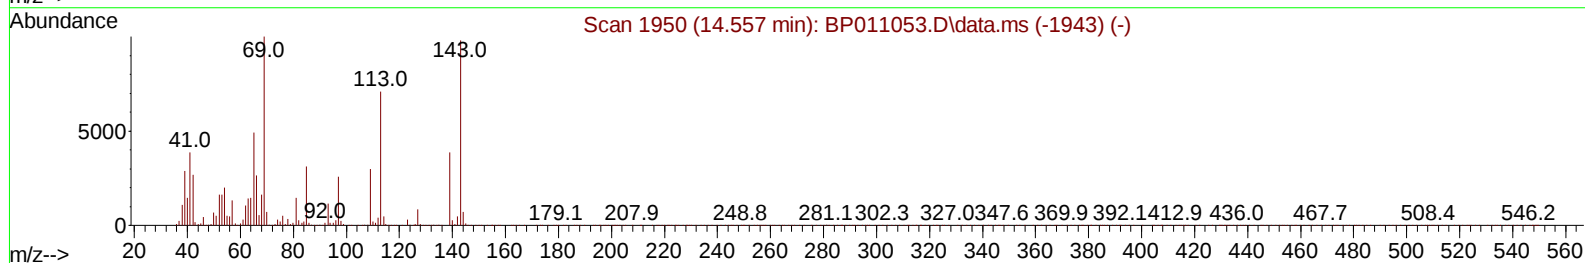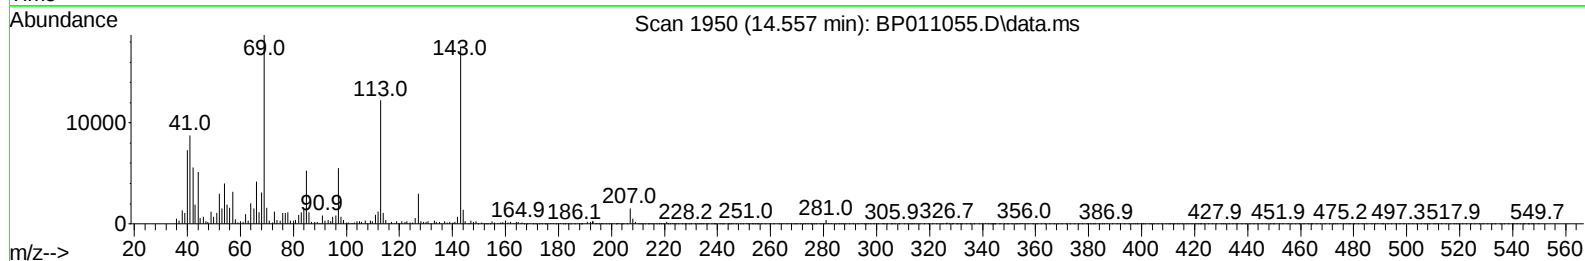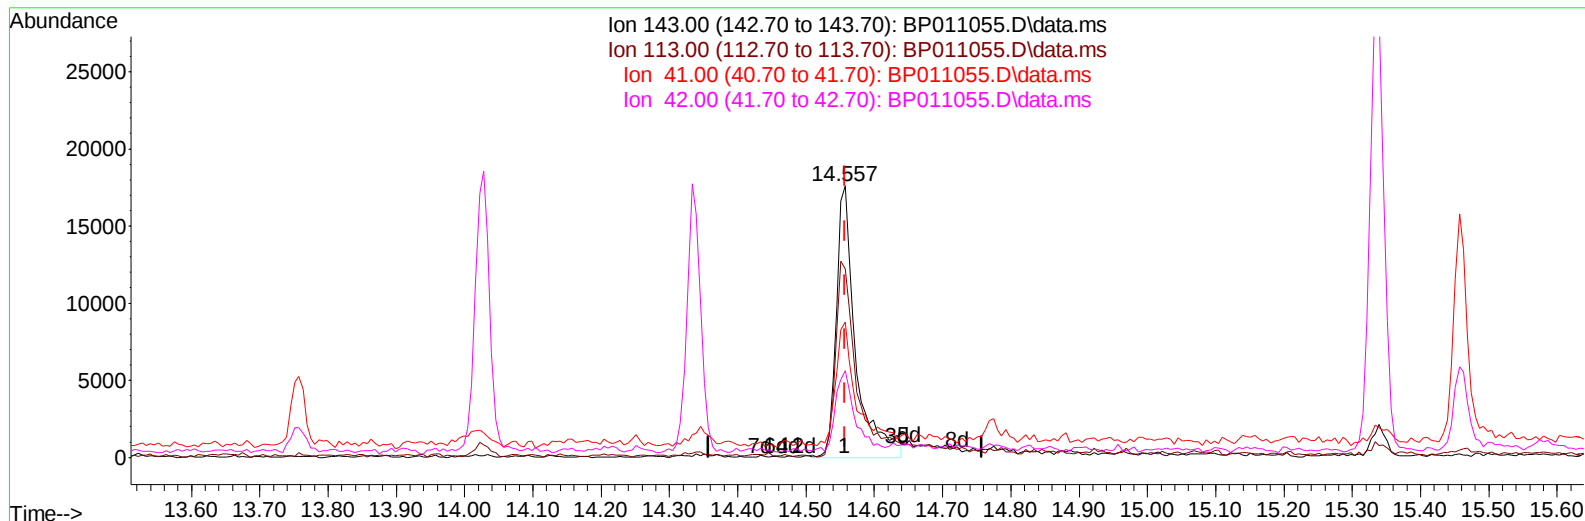

TIC: BP011055.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.557min (-0.000) 3.61 ng/ul m

response 34988

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.50	69.48#
41.00	59.00	49.82
42.00	41.10	31.91#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
 Data File : BP011055.D
 Acq On : 20 Jul 2022 14:29
 Operator : CG/JU
 Sample : N3739-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0B39

Manual IntegrationsAPPROVED

Quant Time: Jul 21 00:43:15 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 19 03:25:54 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 07/21/2022
 Supervised By :mohammad ahmed 07/21/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.675	152	323582	20.000	ng/ul	0.00
20) Naphthalene-d8	10.469	136	1282279	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.339	164	700072	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.104	188	1392788	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.227	240	1374608	20.000	ng/ul	# 0.00
88) Perylene-d12	23.586	264	1425511	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	48901	5.448	ng/uL	0.00
4) Pyridine-d5	3.593	84	222543	9.592	ng/ul	0.00
7) Phenol-d5	6.852	99	153146	5.766	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.016	67	536002	31.382	ng/ul	0.00
11) 2-Chlorophenol-d4	7.210	132	500609	23.325	ng/ul	0.00
15) 4-Methylphenol-d8	8.387	113	294586	13.854	ng/ul	-0.01
21) Nitrobenzene-d5	8.840	128	306008	32.747	ng/ul	0.00
24) 2-Nitrophenol-d4	9.557	143	273193	29.545	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.093	165	471095	27.859	ng/ul	0.00
31) 4-Chloroaniline-d4	10.616	131	525317	18.844	ng/ul	0.00
46) Dimethylphthalate-d6	13.757	166	1768573	36.963	ng/ul	0.00
49) Acenaphthylene-d8	14.028	160	2052060	36.349	ng/ul	0.00
54) 4-Nitrophenol-d4	14.557	143	34988m	3.613	ng/ul	0.00
60) Fluorene-d10	15.339	176	1475317	36.275	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.463	200	180964	26.257	ng/ul	0.00
73) Anthracene-d10	17.204	188	2354793	39.770	ng/ul	0.00
81) Pyrene-d10	19.463	212	2788570	38.626	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.433	264	2798603	40.876	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
Data File : BP011055.D
Acq On : 20 Jul 2022 14:29
Operator : CG/JU
Sample : N3739-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0B39

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 07/21/2022
Supervised By :mohammad ahmed 07/21/2022

Quant Time: Jul 21 00:43:15 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 19 03:25:54 2022
Response via : Initial Calibration

