

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
 Data File : BP011050.D
 Acq On : 20 Jul 2022 09:27
 Operator : CG/JU
 Sample : PB146316BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK316

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011050.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	28	rVB	145868	217082	2.71%	0.244%
2	3.587	82	85	104	rBV	1539168	2308551	28.79%	2.593%
3	3.899	135	138	144	rVB2	30383	40686	0.51%	0.046%
4	6.852	634	640	655	rBV	1660242	2588237	32.27%	2.907%
5	7.022	662	669	682	rVB	1444079	2188821	27.29%	2.458%
6	7.210	694	701	714	rBV	1805104	2692595	33.58%	3.024%
7	7.675	773	780	790	rVB	1368115	2127896	26.53%	2.390%
8	8.393	895	902	918	rBV	2020232	3187728	39.75%	3.580%
9	8.840	969	978	987	rBV	1590091	2519827	31.42%	2.830%
10	9.557	1093	1100	1107	rBV	1198295	1881778	23.46%	2.113%
11	10.093	1184	1191	1206	rBV	1849617	2963890	36.96%	3.329%
12	10.469	1248	1255	1263	rVB	1846854	2989917	37.28%	3.358%
13	10.616	1272	1280	1294	rBV	1856365	3173296	39.57%	3.564%
14	12.069	1521	1527	1533	rBV2	35349	60511	0.75%	0.068%
15	13.304	1734	1737	1742	rVB6	7214	9383	0.12%	0.011%
16	13.757	1807	1814	1827	rBV	3256911	4427011	55.20%	4.972%
17	14.028	1851	1860	1872	rBV	3727576	5302736	66.12%	5.955%
18	14.340	1906	1913	1920	rBV	2611292	3709092	46.25%	4.165%
19	14.551	1941	1949	1973	rBV	1119157	2045754	25.51%	2.297%
20	15.339	2076	2083	2092	rBV	4866889	6528716	81.41%	7.332%
21	15.463	2098	2104	2119	rBV	1248125	1751849	21.84%	1.967%
22	15.581	2119	2124	2129	rVB2	57898	85139	1.06%	0.096%
23	16.028	2194	2200	2206	rBV2	6259	13853	0.17%	0.016%
24	16.134	2213	2218	2223	rVB5	16482	24179	0.30%	0.027%
25	16.598	2292	2297	2299	rBV6	4477	8852	0.11%	0.010%
26	16.786	2325	2329	2333	rVB6	9812	15261	0.19%	0.017%
27	16.898	2338	2348	2350	rBV8	9227	18181	0.23%	0.020%
28	17.104	2377	2383	2394	rBV	3026737	4269040	53.23%	4.794%
29	17.204	2394	2400	2418	rVV2	4834422	6933455	86.46%	7.787%
30	19.039	2708	2712	2716	rVB2	54826	72845	0.91%	0.082%
31	19.104	2719	2723	2727	rBV	58644	78364	0.98%	0.088%
32	19.463	2778	2784	2792	rBV	6305783	8019569	100.00%	9.006%
33	21.227	3079	3084	3089	rBV	3932255	4638977	57.85%	5.210%
34	23.427	3452	3458	3468	rBV2	4102952	7599120	94.76%	8.534%
35	23.580	3478	3484	3496	rVB2	2341722	4551933	56.76%	5.112%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
Data File : BP011050.D
Acq On : 20 Jul 2022 09:27
Operator : CG/JU
Sample : PB146316BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK316

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Title : SVOA CALIBRATION




Sum of corrected areas: 89044124

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
Data File : BP011050.D
Acq On : 20 Jul 2022 09:27
Operator : CG/JU
Sample : PB146316BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK316

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

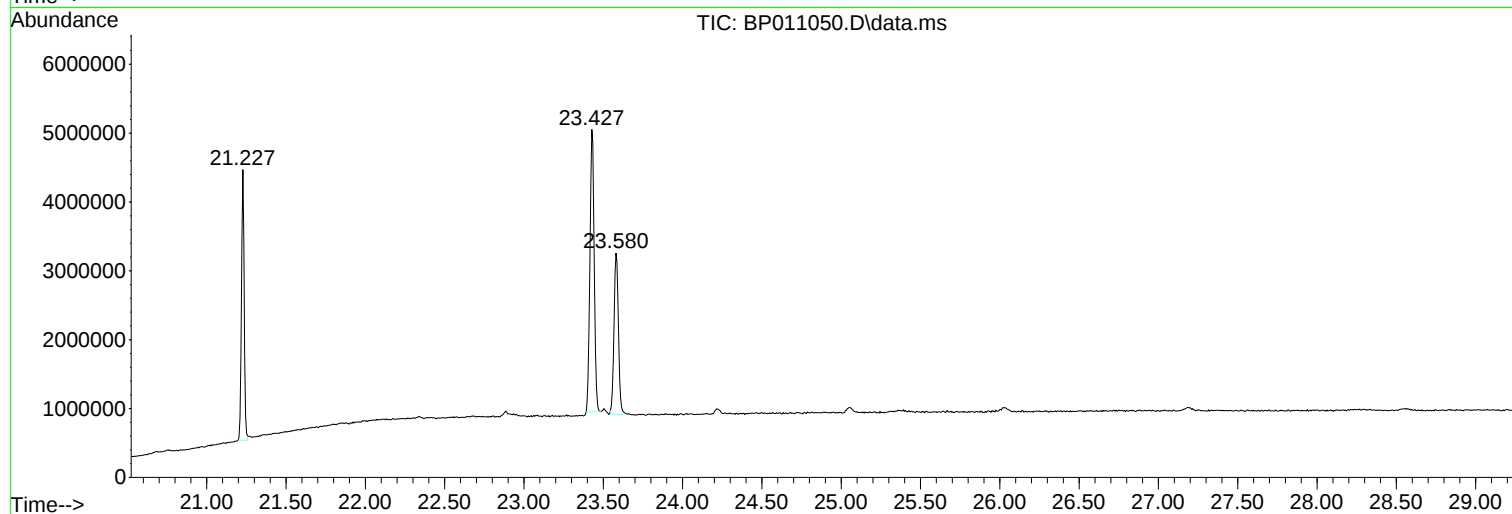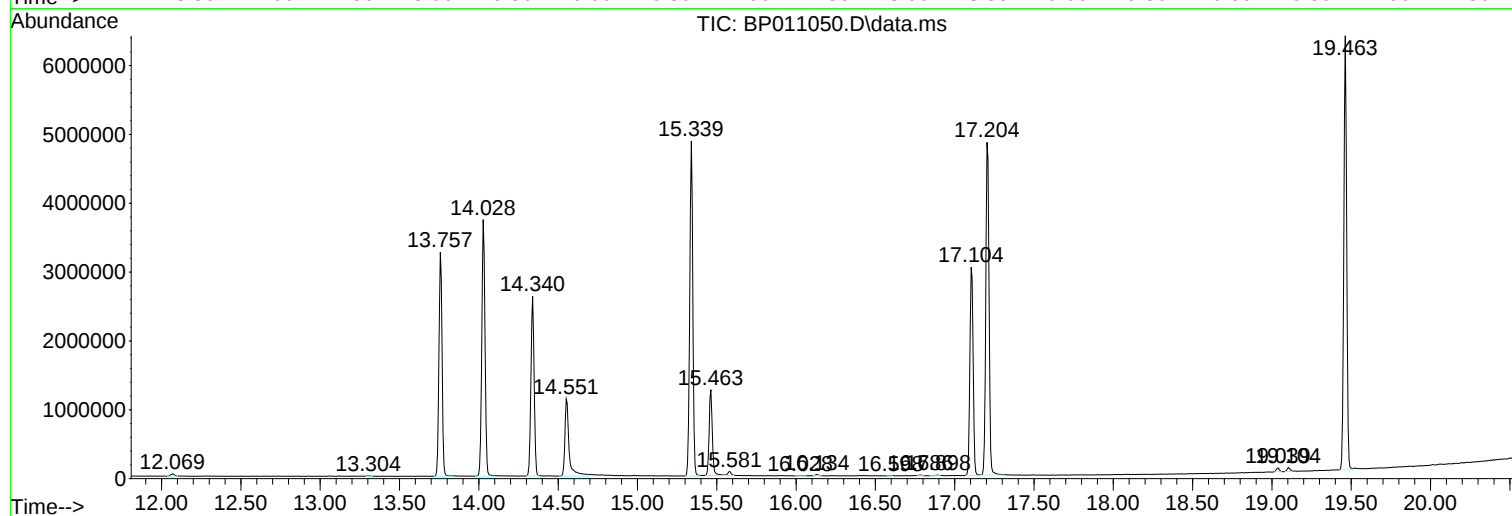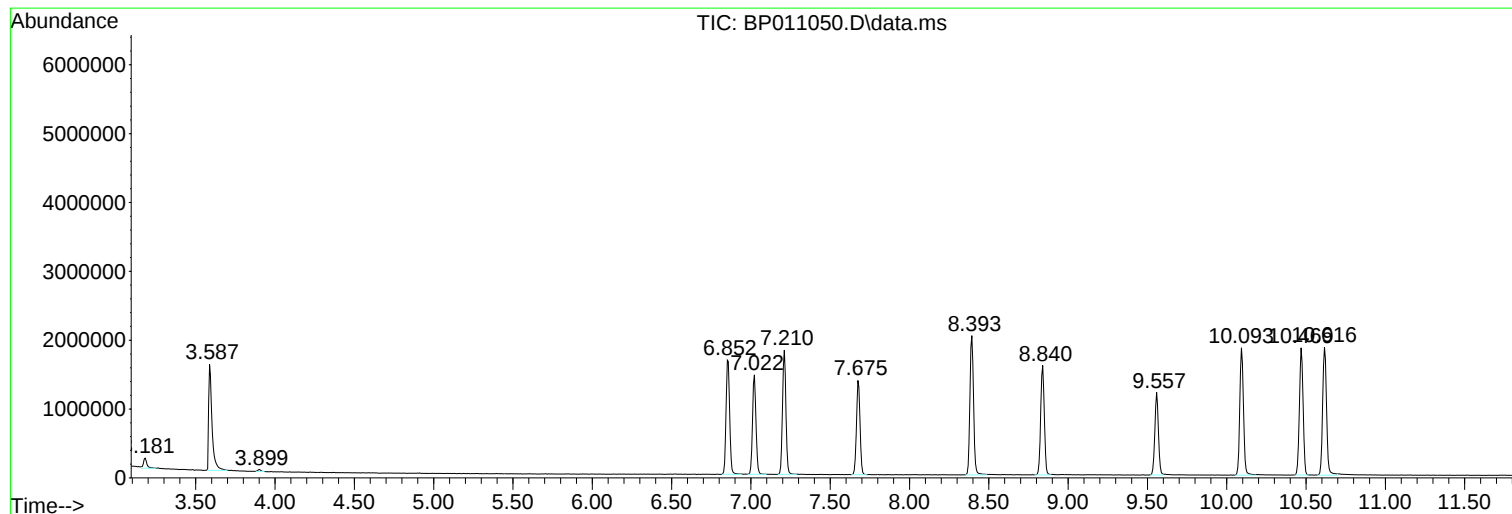

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
Data File : BP011050.D
Acq On : 20 Jul 2022 09:27
Operator : CG/JU
Sample : PB146316BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK316

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
Data File : BP011050.D
Acq On : 20 Jul 2022 09:27
Operator : CG/JU
Sample : PB146316BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK316

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc