

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
 Data File : BP011051.D
 Acq On : 20 Jul 2022 10:01
 Operator : CG/JU
 Sample : N3753-14
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 GBHQ5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011051.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	19	rBV	120696	159518	1.92%	0.182%
2	3.217	19	22	29	rVB	85511	123460	1.49%	0.141%
3	3.587	82	85	108	rBV	1592345	2372092	28.58%	2.700%
4	3.811	118	123	128	rBV	36456	54579	0.66%	0.062%
5	3.899	135	138	144	rVB2	34232	50954	0.61%	0.058%
6	4.805	290	292	300	rVB3	23446	42677	0.51%	0.049%
7	5.399	390	393	399	rVB2	9845	13235	0.16%	0.015%
8	6.852	633	640	654	rBV	1738104	2618464	31.55%	2.980%
9	7.017	662	668	680	rVB	1437281	2192925	26.42%	2.496%
10	7.205	693	700	713	rBV	1718820	2695987	32.49%	3.068%
11	7.675	772	780	787	rBV	1198991	1839442	22.16%	2.093%
12	8.387	893	901	913	rBV	2103640	3255191	39.22%	3.705%
13	8.834	970	977	989	rBV	1591449	2507253	30.21%	2.853%
14	9.252	1044	1048	1054	rVB6	7634	13056	0.16%	0.015%
15	9.552	1090	1099	1110	rBV	1161480	1912692	23.05%	2.177%
16	10.087	1183	1190	1201	rBV	1775651	2970281	35.79%	3.380%
17	10.469	1246	1255	1266	rVB	1537788	2562486	30.88%	2.916%
18	10.610	1271	1279	1296	rBV	1867272	3254663	39.22%	3.704%
19	12.069	1520	1527	1535	rBV	34385	57935	0.70%	0.066%
20	12.281	1559	1563	1567	rBV7	6368	10396	0.13%	0.012%
21	13.304	1732	1737	1739	rBV6	5686	9091	0.11%	0.010%
22	13.663	1795	1798	1802	rBV6	6253	9343	0.11%	0.011%
23	13.757	1807	1814	1825	rBV	3389928	4532837	54.62%	5.159%
24	14.028	1852	1860	1875	rBV	3603010	5245903	63.21%	5.970%
25	14.334	1905	1912	1920	rBV	2223359	3195112	38.50%	3.636%
26	14.551	1942	1949	1969	rBV	1190445	2059566	24.82%	2.344%
27	14.769	1983	1986	1993	rVB	37931	56569	0.68%	0.064%
28	15.340	2076	2083	2093	rBV	4623174	6581188	79.30%	7.490%
29	15.457	2097	2103	2116	rVV	1312363	1808469	21.79%	2.058%
30	15.581	2119	2124	2131	rVB	59238	93030	1.12%	0.106%
31	16.128	2213	2217	2222	rVB6	19049	25992	0.31%	0.030%
32	16.781	2325	2328	2334	rVB7	11886	14912	0.18%	0.017%
33	16.892	2342	2347	2348	rBV4	9626	11576	0.14%	0.013%
34	17.104	2377	2383	2393	rBV	2651375	3691077	44.48%	4.201%
35	17.204	2393	2400	2414	rVV2	5084696	7123719	85.84%	8.107%
36	17.310	2415	2418	2423	rVB6	21918	35591	0.43%	0.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
Data File : BP011051.D
Acq On : 20 Jul 2022 10:01
Operator : CG/JU
Sample : N3753-14
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHQ5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Title : SVOA CALIBRATION

37	17.492	2444	2449	2452	rBV6	5010	10729	0.13%	0.012%
38	19.034	2707	2711	2716	rBV	62063	81686	0.98%	0.093%
39	19.104	2719	2723	2731	rVV	60859	87148	1.05%	0.099%
40	19.457	2778	2783	2791	rBV	6182570	8298962	100.00%	9.445%
41	21.228	3079	3084	3092	rBV	3060578	4040360	48.69%	4.598%
42	23.427	3451	3458	3468	rBV2	4257418	8268623	99.63%	9.410%
43	23.580	3478	3484	3493	rVB	2009054	3880966	46.76%	4.417%




Sum of corrected areas: 87869735

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
Data File : BP011051.D
Acq On : 20 Jul 2022 10:01
Operator : CG/JU
Sample : N3753-14
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHQ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

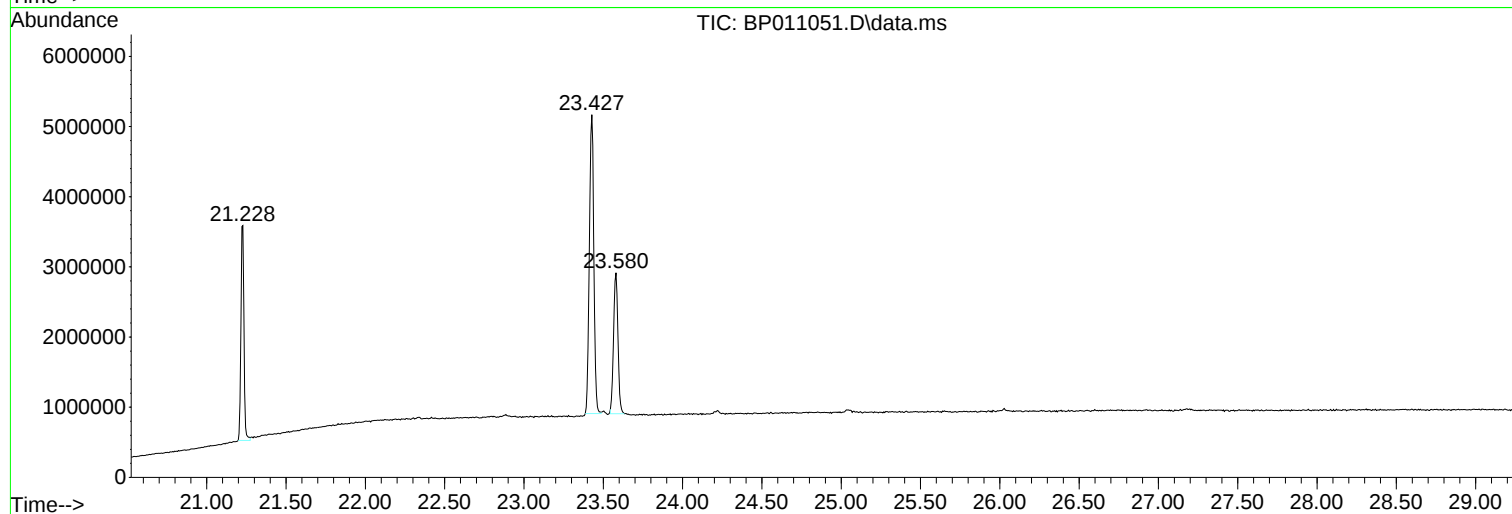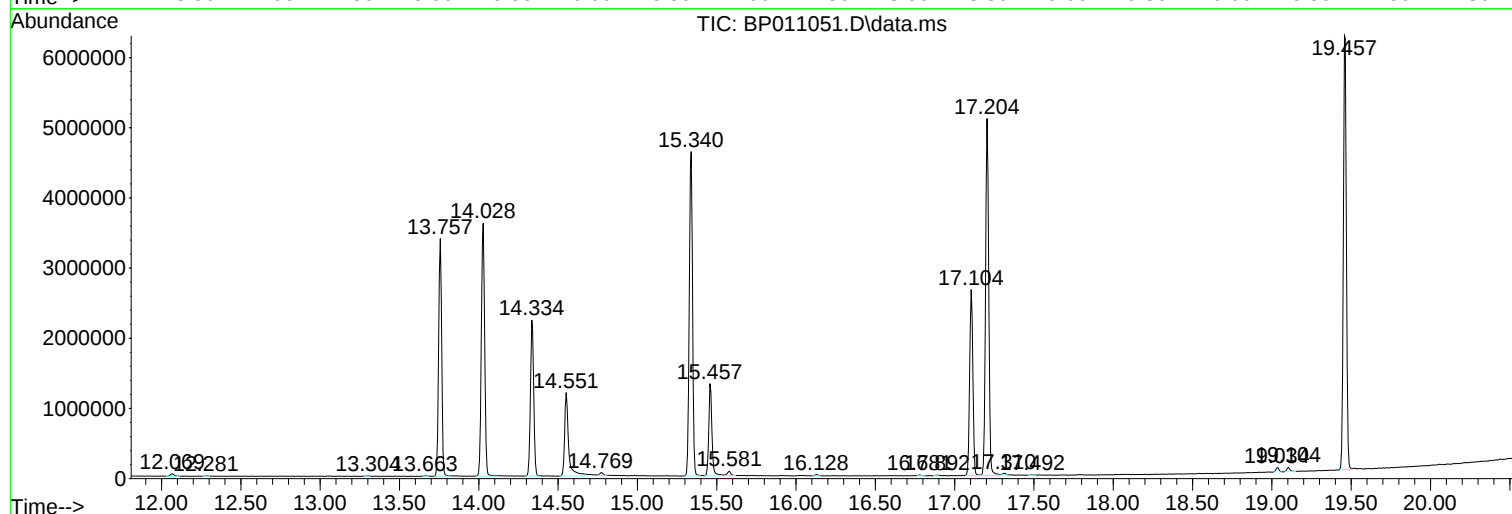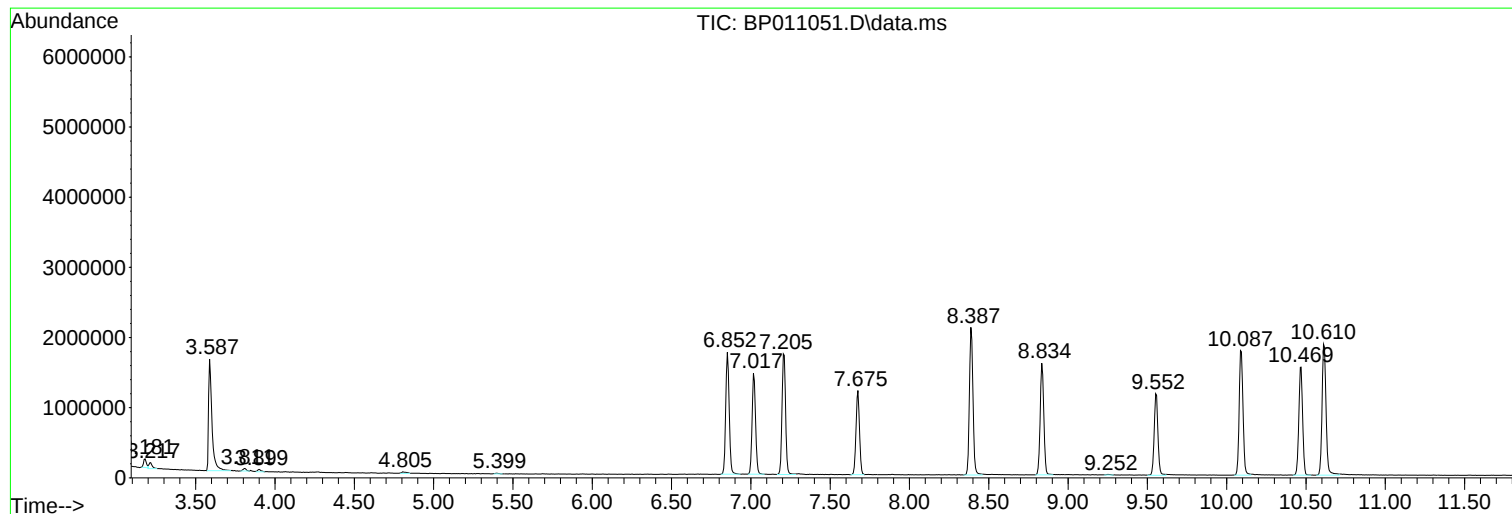

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
Data File : BP011051.D
Acq On : 20 Jul 2022 10:01
Operator : CG/JU
Sample : N3753-14
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHQ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
Data File : BP011051.D
Acq On : 20 Jul 2022 10:01
Operator : CG/JU
Sample : N3753-14
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
GBHQ5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc