

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
 Data File : BP011054.D
 Acq On : 20 Jul 2022 13:55
 Operator : CG/JU
 Sample : PB146316BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK316

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011054.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.181	12	16	24	rVB	150032	200693	2.65%	0.233%
2	3.587	82	85	104	rBV	1573131	2298292	30.38%	2.670%
3	3.899	135	138	145	rVB	31752	48943	0.65%	0.057%
4	6.852	634	640	654	rBV	1627309	2547027	33.67%	2.959%
5	7.022	662	669	679	rVB	1418532	2147185	28.38%	2.495%
6	7.211	694	701	713	rBV	1784611	2672409	35.33%	3.105%
7	7.675	774	780	789	rVB	1429550	2235198	29.55%	2.597%
8	8.393	894	902	915	rBV	1974048	3067006	40.54%	3.563%
9	8.840	970	978	987	rBV	1540433	2444198	32.31%	2.840%
10	9.557	1093	1100	1115	rBV	1148718	1824096	24.11%	2.119%
11	10.093	1184	1191	1205	rBV	1770079	2825446	37.35%	3.283%
12	10.469	1247	1255	1263	rBV	1885037	3048147	40.29%	3.541%
13	10.616	1271	1280	1291	rBV	1731216	2986296	39.48%	3.470%
14	12.069	1521	1527	1535	rBV	31701	53053	0.70%	0.062%
15	13.122	1701	1706	1711	rBV9	4893	8051	0.11%	0.009%
16	13.304	1734	1737	1741	rVB6	6545	9688	0.13%	0.011%
17	13.757	1807	1814	1826	rBV	3016335	4128296	54.57%	4.796%
18	14.028	1853	1860	1877	rBV	3466500	4914822	64.97%	5.710%
19	14.340	1905	1913	1920	rBV	2536280	3679019	48.63%	4.274%
20	14.551	1943	1949	1971	rBV	1029296	1899254	25.11%	2.207%
21	15.340	2074	2083	2093	rBV	4447067	6070063	80.24%	7.052%
22	15.463	2098	2104	2119	rVV	1192722	1625886	21.49%	1.889%
23	15.581	2119	2124	2130	rVB	55586	85146	1.13%	0.099%
24	15.863	2165	2172	2175	rBV9	6607	13389	0.18%	0.016%
25	16.034	2197	2201	2207	rBV8	5250	9974	0.13%	0.012%
26	16.134	2214	2218	2222	rBV5	14452	20269	0.27%	0.024%
27	16.786	2326	2329	2335	rVB7	10137	13055	0.17%	0.015%
28	16.886	2342	2346	2351	rBV3	8559	14522	0.19%	0.017%
29	17.110	2377	2384	2394	rBV	2888123	4231204	55.93%	4.916%
30	17.210	2394	2401	2418	rVV	4545396	6443779	85.18%	7.487%
31	19.039	2708	2712	2717	rBV2	57982	81093	1.07%	0.094%
32	19.110	2720	2724	2728	rBV	55858	71544	0.95%	0.083%
33	19.463	2779	2784	2793	rBV	5622431	7509431	99.27%	8.725%
34	21.227	3080	3084	3090	rBV	3657064	4643324	61.38%	5.395%
35	23.433	3452	3459	3468	rBV2	3984124	7564599	100.00%	8.789%
36	23.586	3479	3485	3496	rVB2	2328344	4636871	61.30%	5.387%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
Data File : BP011054.D
Acq On : 20 Jul 2022 13:55
Operator : CG/JU
Sample : PB146316BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK316

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Title : SVOA CALIBRATION




Sum of corrected areas: 86071268

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
Data File : BP011054.D
Acq On : 20 Jul 2022 13:55
Operator : CG/JU
Sample : PB146316BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK316

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

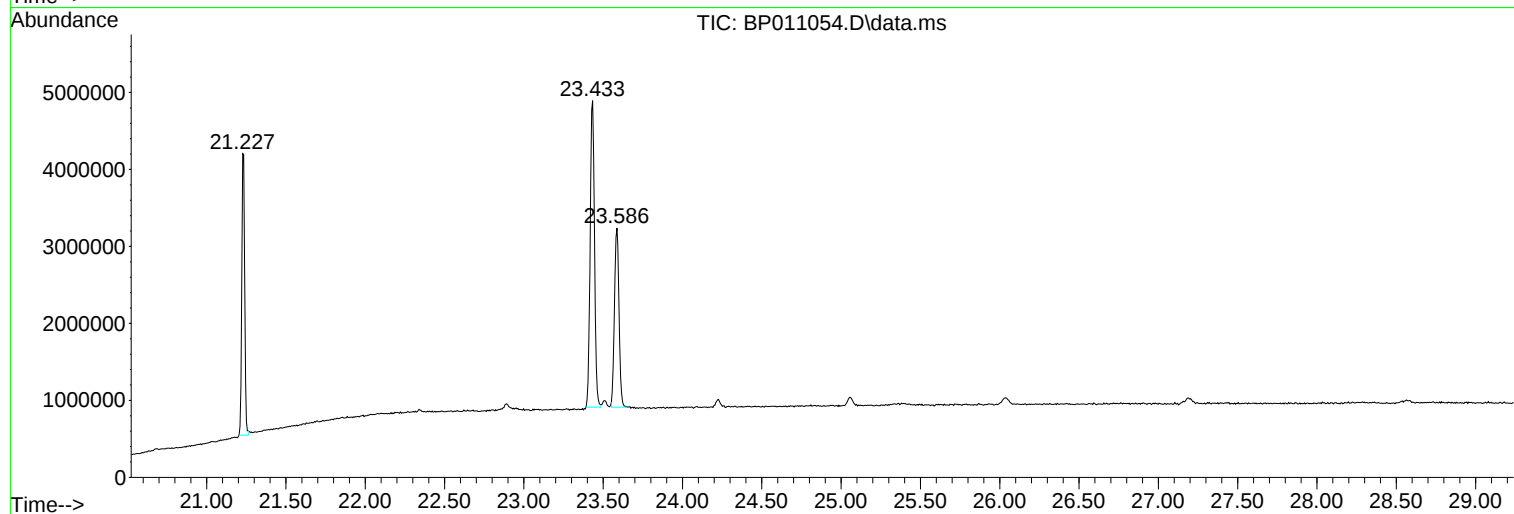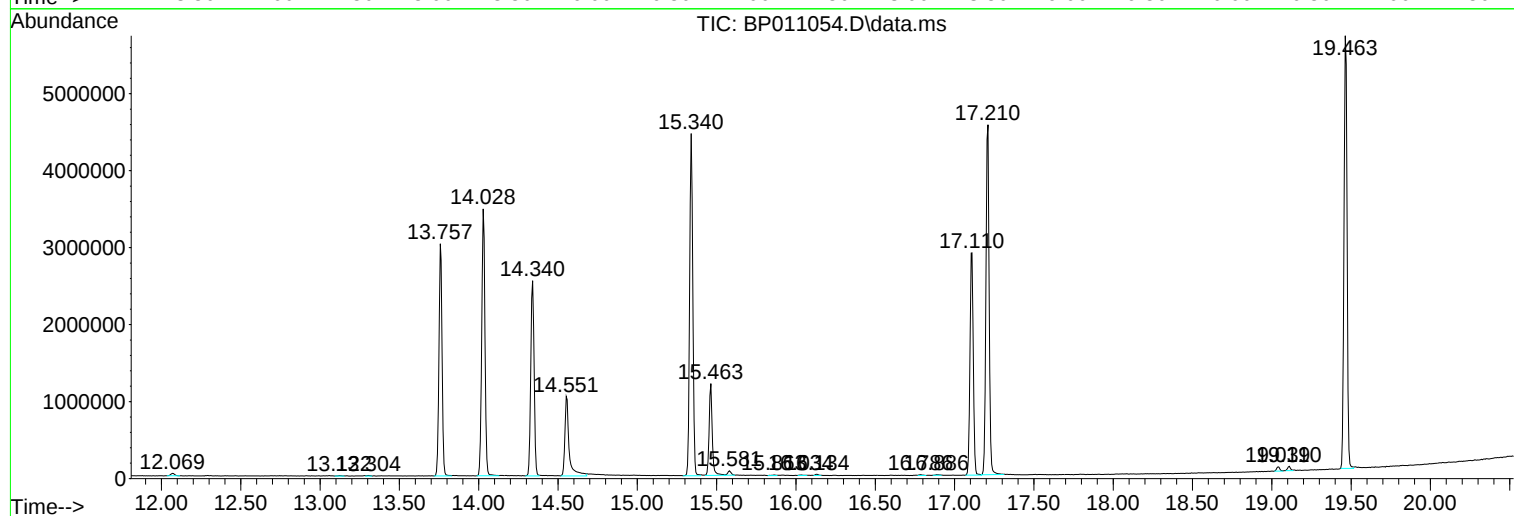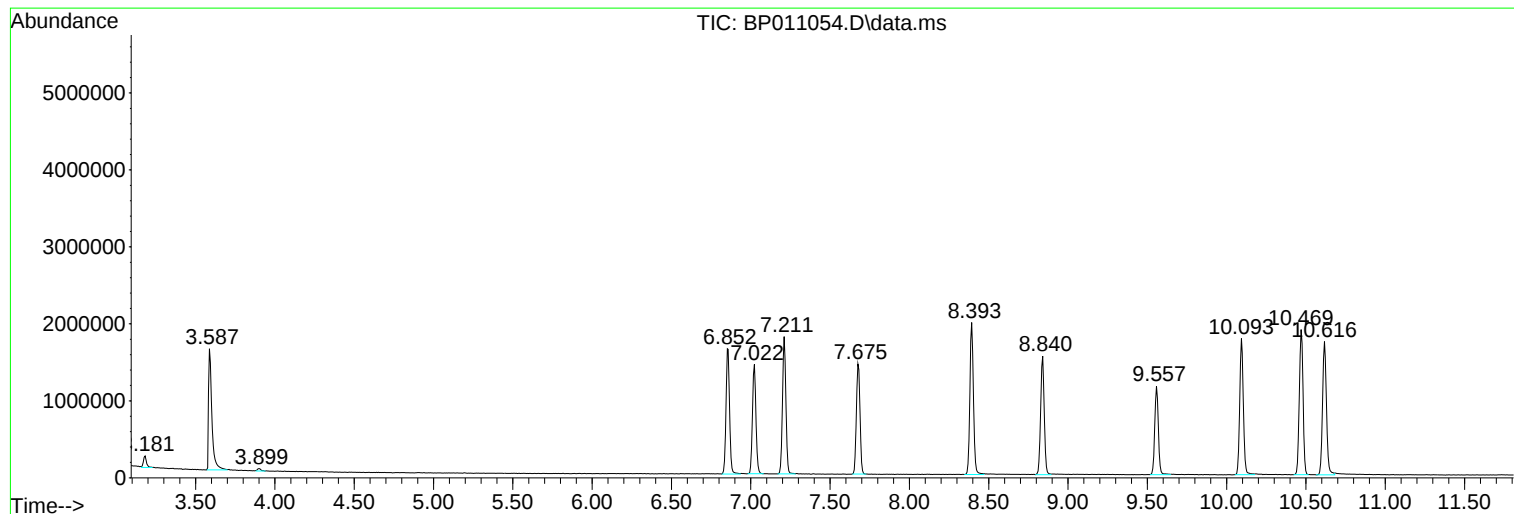

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
Data File : BP011054.D
Acq On : 20 Jul 2022 13:55
Operator : CG/JU
Sample : PB146316BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK316

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072022\
Data File : BP011054.D
Acq On : 20 Jul 2022 13:55
Operator : CG/JU
Sample : PB146316BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK316

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc