
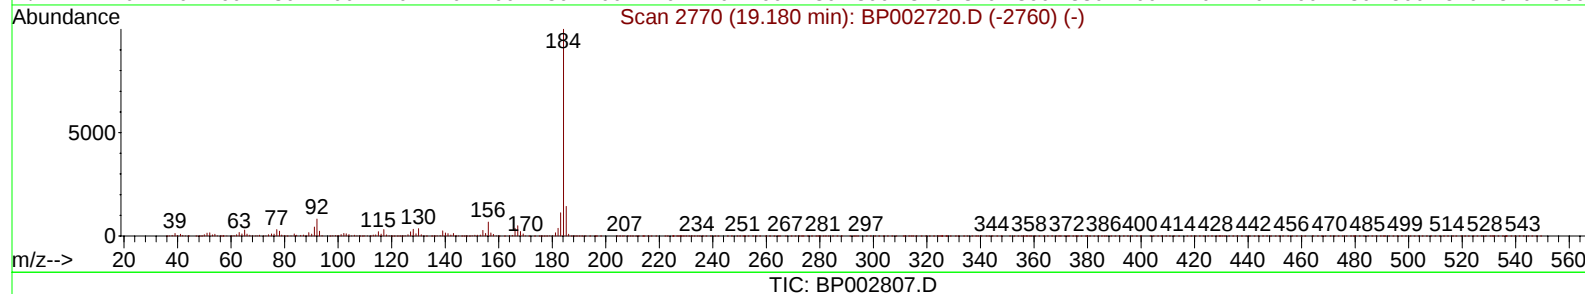
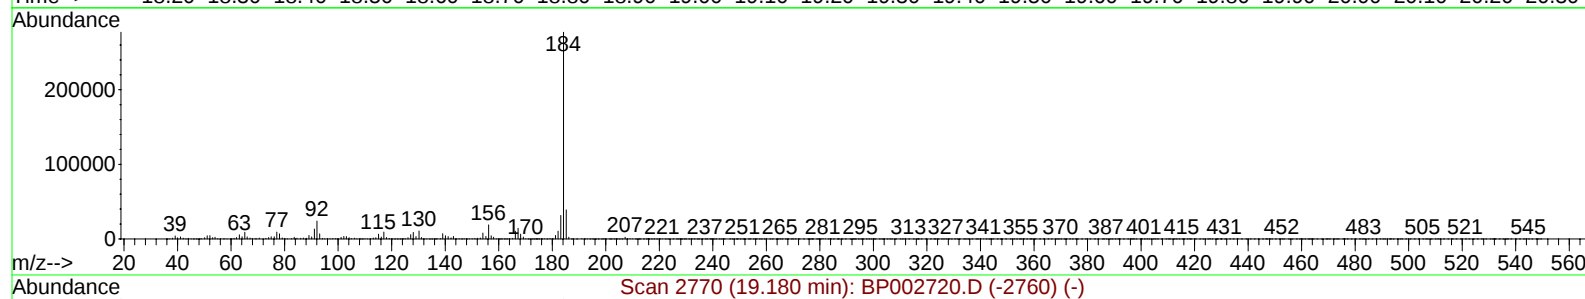


Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP072120\
 Data File : BP002807.D
 Acq On : 21 Jul 2020 09:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 21 16:08:09 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 13 10:54:03 2020
 Response via : Initial Calibration

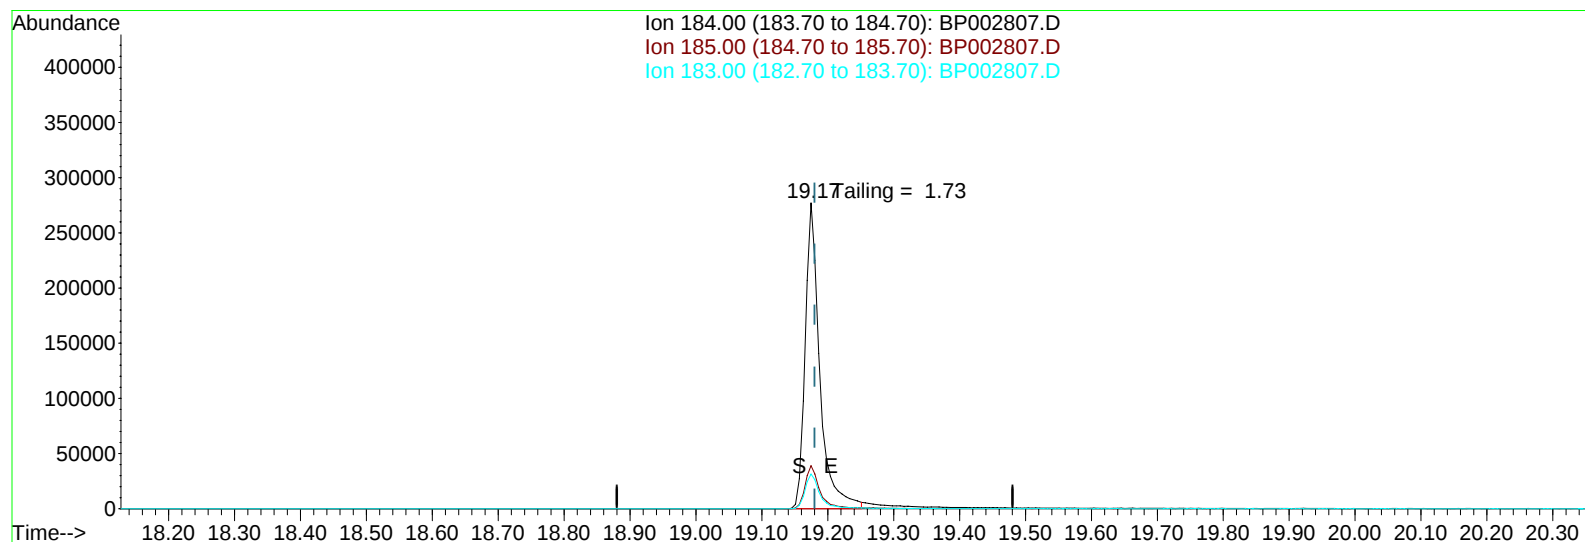

TIC: BP002807.D

(77) Benzidine




19.175min (-0.006) 517560.64ng

response 384862

Ion	Exp%	Act%
184.00	100	100
185.00	14.30	14.09
183.00	11.20	11.35
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP072120\
Data File : BP002807.D
Acq On : 21 Jul 2020 09:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 21 16:08:09 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA P\METHODS\8270-BP071020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 13 10:54:03 2020
Response via : Initial Calibration

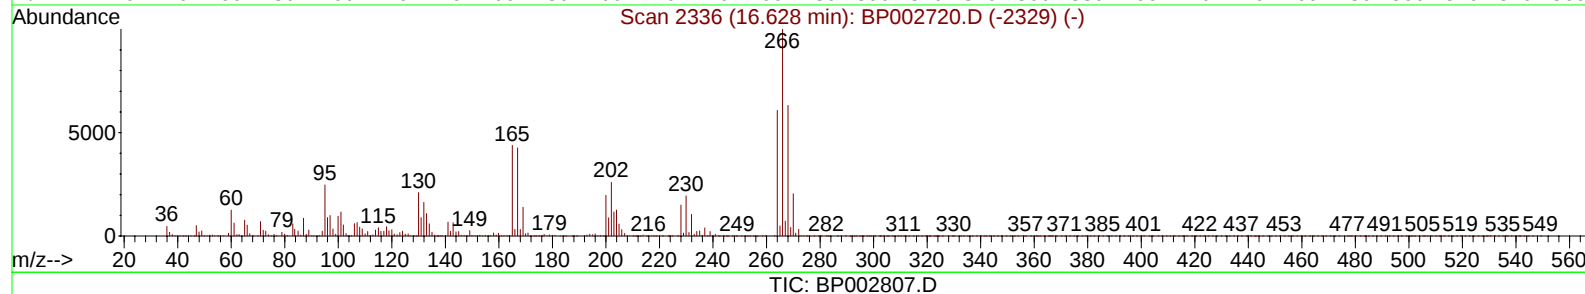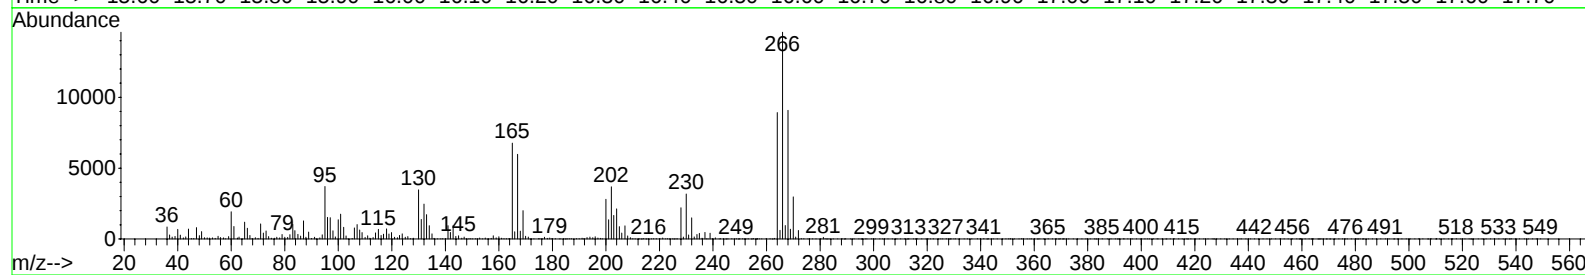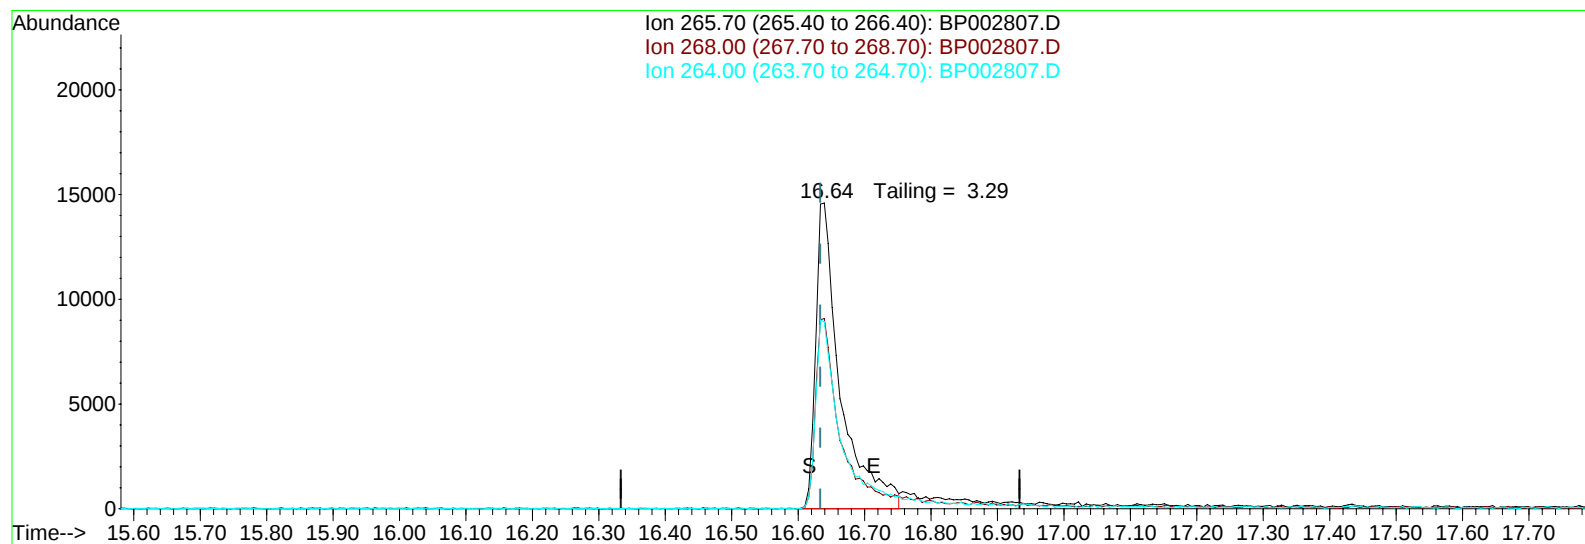

(70) Pentachlorophenol (C)

16.639min (+0.006) 178329.54ng

response 39289

Ion	Exp%	Act%
265.70	100	100
268.00	63.20	62.23
264.00	60.70	61.15
0.00	0.00	0.00