


Data Path : Z:\svoasrv\HPCHEM1\BNA P\Data\BP072120\
 Data File : BP002807.D
 Acq On : 21 Jul 2020 09:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP071020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 13 10:54:03 2020

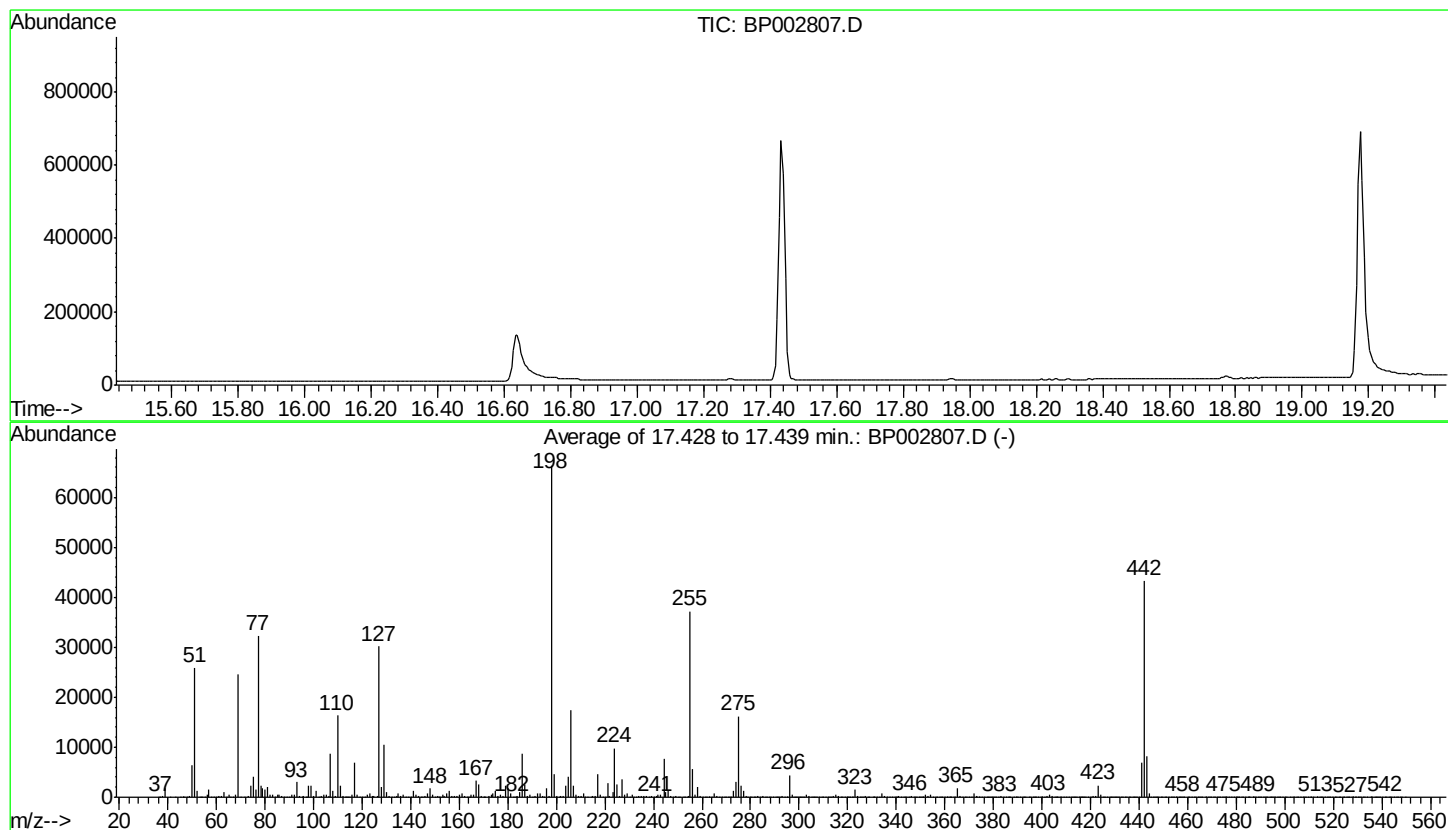

AutoFind: Scans 2472, 2473, 2474; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.1	25949	PASS
68	69	0.00	2	1.8	435	PASS
69	198	0.00	100	37.2	24676	PASS
70	69	0.00	2	0.5	112	PASS
127	198	10	80	45.4	30145	PASS
197	198	0.00	2	0.5	351	PASS
198	198	100	100	100.0	66365	PASS
199	198	5	9	6.9	4597	PASS
275	198	10	60	24.5	16270	PASS
365	198	1	100	2.8	1842	PASS
441	198	0.01	100	10.5	6962	PASS
442	198	50	100	65.4	43418	PASS
443	442	15	24	19.2	8324	PASS