
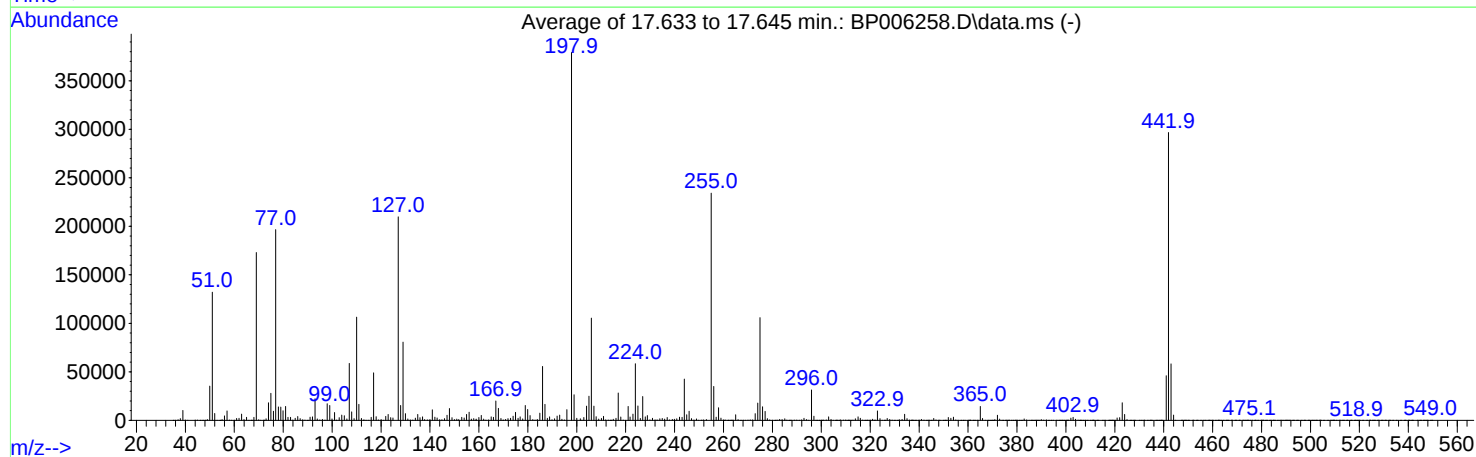


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072121\
 Data File : BP006258.D
 Acq On : 21 Jul 2021 09:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072021.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 21 08:44:35 2021

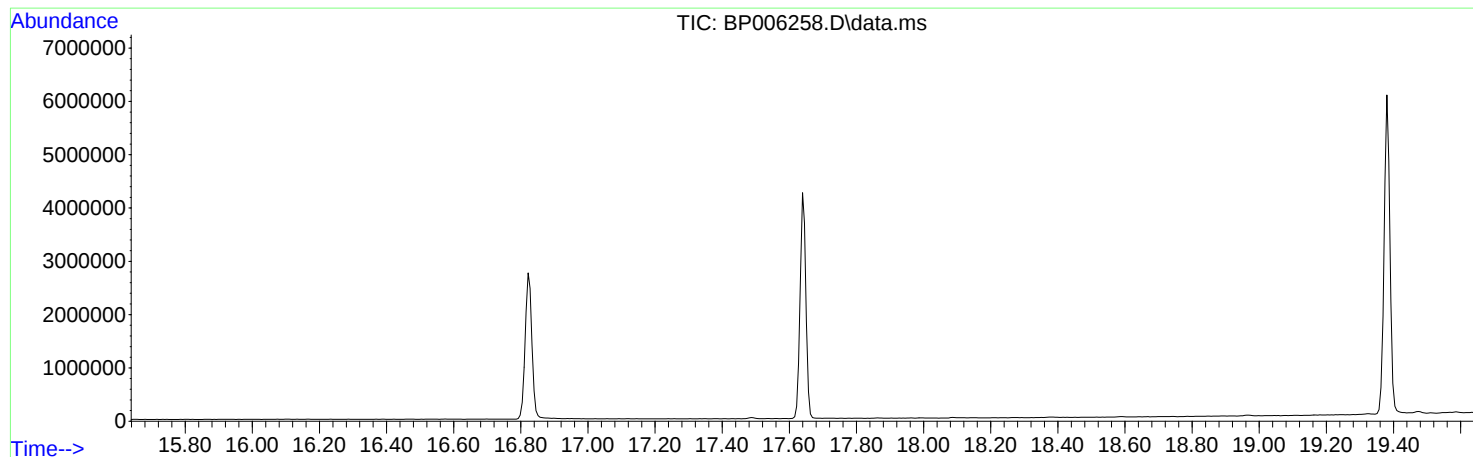




AutoFind: Scans 2473, 2474, 2475; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.8	132093	PASS
68	69	0.00	2	1.8	3134	PASS
69	198	0.00	100	45.6	173066	PASS
70	69	0.00	2	0.4	692	PASS
127	198	10	80	55.3	209756	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	379140	PASS
199	198	5	9	7.0	26404	PASS
275	198	10	60	27.9	105950	PASS
365	198	1	100	3.8	14438	PASS
441	198	0.01	100	12.1	46053	PASS
442	442	100	100	100.0	296701	PASS
443	442	15	24	19.6	58179	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072121\
Data File : BP006258.D
Acq On : 21 Jul 2021 09:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Jul 21 11:15:30 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072021.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 21 08:44:35 2021
Response via : Initial Calibration

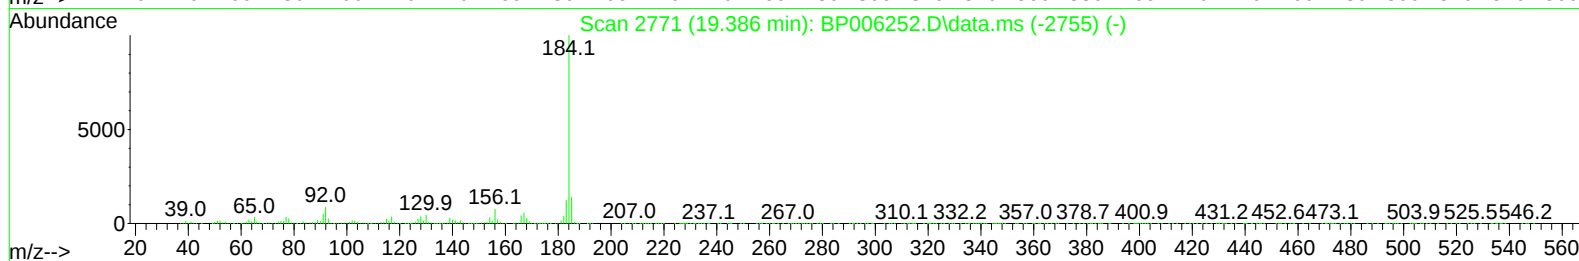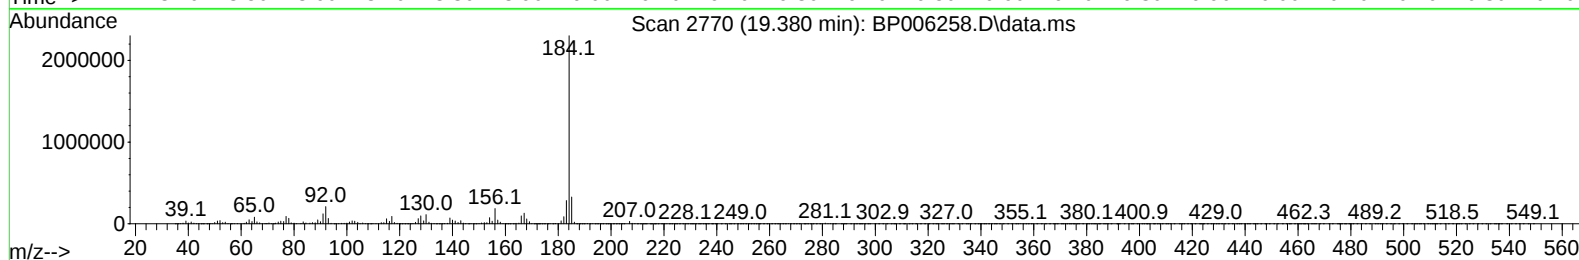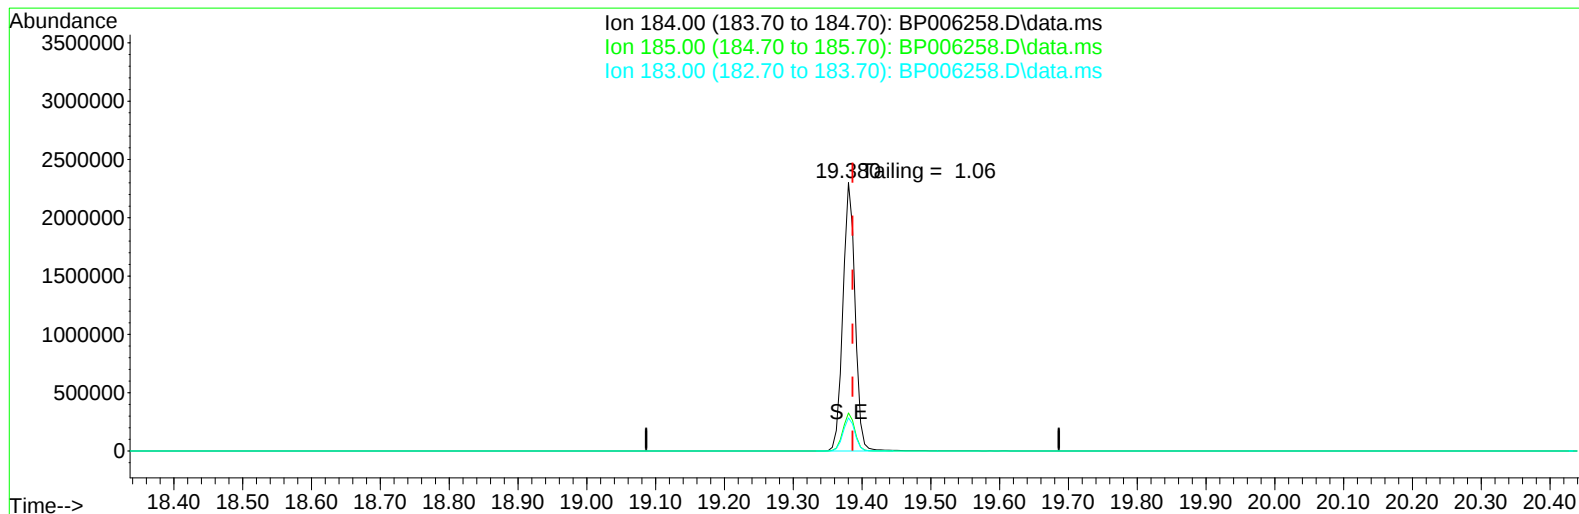

TIC: BP006258.D\data.ms

(77) Benzidine

19.380min (-0.006) 2356779.58 ng m




response 2812378

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.70	14.18
183.00	11.90	12.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072121\
 Data File : BP006258.D
 Acq On : 21 Jul 2021 09:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Jul 21 11:15:30 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP072021.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 21 08:44:35 2021
 Response via : Initial Calibration

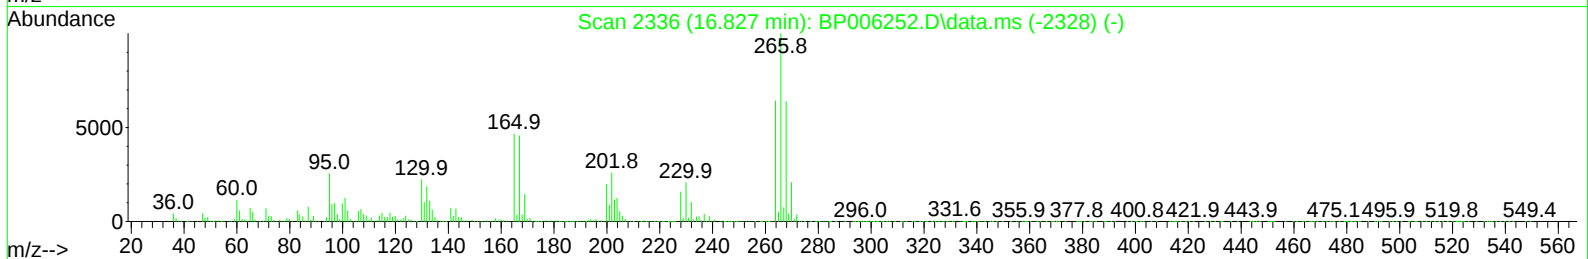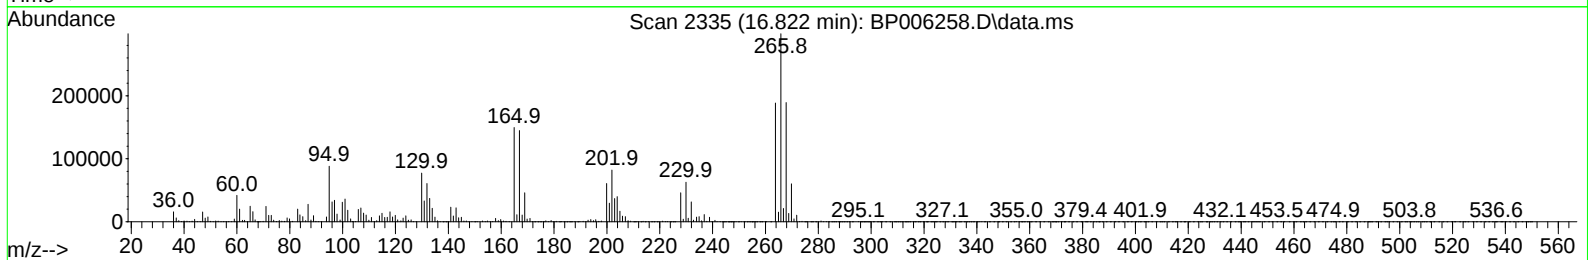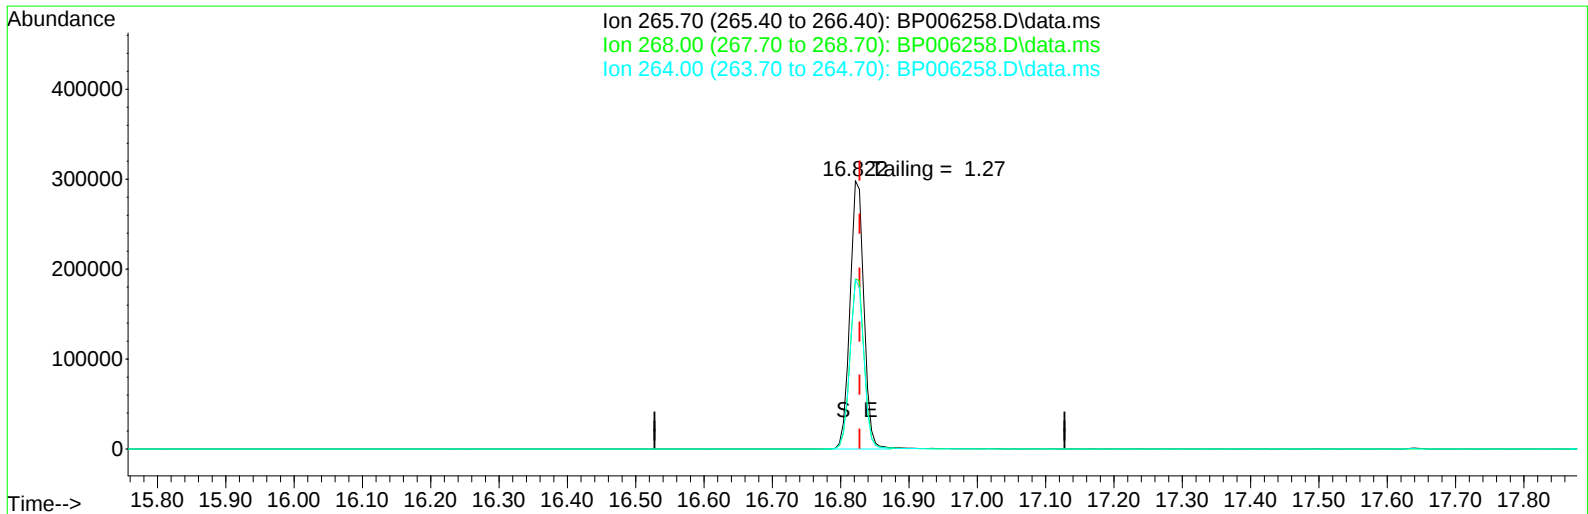

TIC: BP006258.D\data.ms

(70) Pentachlorophenol (C)

16.822min (-0.006) 1411578.30 ng

response 420102

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.50	63.37
264.00	62.90	63.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/21/2021	BNA_P	BP006258.D
Compound Name	Response	Retention Time
DDT	1404333	20.58
DDD	5757	20.15
DDE	1904	19.66
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7661	1411994	0.54

Instrument :
BNA_P
ClientSampleId :
DFTPP