

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
 Data File : BP011066.D
 Acq On : 21 Jul 2022 17:20
 Operator : CG/JU
 Sample : N3709-17
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :

Quant Time: Jul 21 23:24:47 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Jul 19 03:25:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.675	152	372054	20.000	ng/ul	0.00
20) Naphthalene-d8	10.463	136	1497536	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.334	164	820723	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.104	188	1611255	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.227	240	1479838	20.000	ng/ul	# 0.00
88) Perylene-d12	23.580	264	1554173	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.181	96	20685	2.004	ng/uL	0.00
4) Pyridine-d5	3.587	84	483	0.018	ng/ul	0.00
7) Phenol-d5	6.852	99	381545	12.493	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.016	67	277923	14.152	ng/ul	0.00
11) 2-Chlorophenol-d4	7.205	132	349216	14.151	ng/ul	0.00
15) 4-Methylphenol-d8	8.387	113	213021	8.713	ng/ul	-0.01
21) Nitrobenzene-d5	8.834	128	162144	14.857	ng/ul	0.00
24) 2-Nitrophenol-d4	9.551	143	153086	14.176	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.087	165	257657	13.047	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.616	131	262341	8.058	ng/ul	0.00
46) Dimethylphthalate-d6	13.751	166	833937	14.867	ng/ul	-0.01
49) Acenaphthylene-d8	14.022	160	1072306	16.202	ng/ul	0.00
54) 4-Nitrophenol-d4	14.551	143	51402	4.528	ng/ul	0.00
60) Fluorene-d10	15.334	176	752817	15.789	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.457	200	42393	5.317	ng/ul	0.00
73) Anthracene-d10	17.204	188	1046882	15.283	ng/ul	0.00
81) Pyrene-d10	19.457	212	1303739	16.775	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.427	264	1235869	16.556	ng/ul	0.00
Target Compounds						
					Qvalue	
10) Bis(2-Chloroethyl)ether	7.110	93	31908	1.238	ng/ul#	18


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
Data File : BP011066.D
Acq On : 21 Jul 2022 17:20
Operator : CG/JU
Sample : N3709-17
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :

Quant Time: Jul 21 23:24:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Jul 19 03:25:54 2022
Response via : Initial Calibration

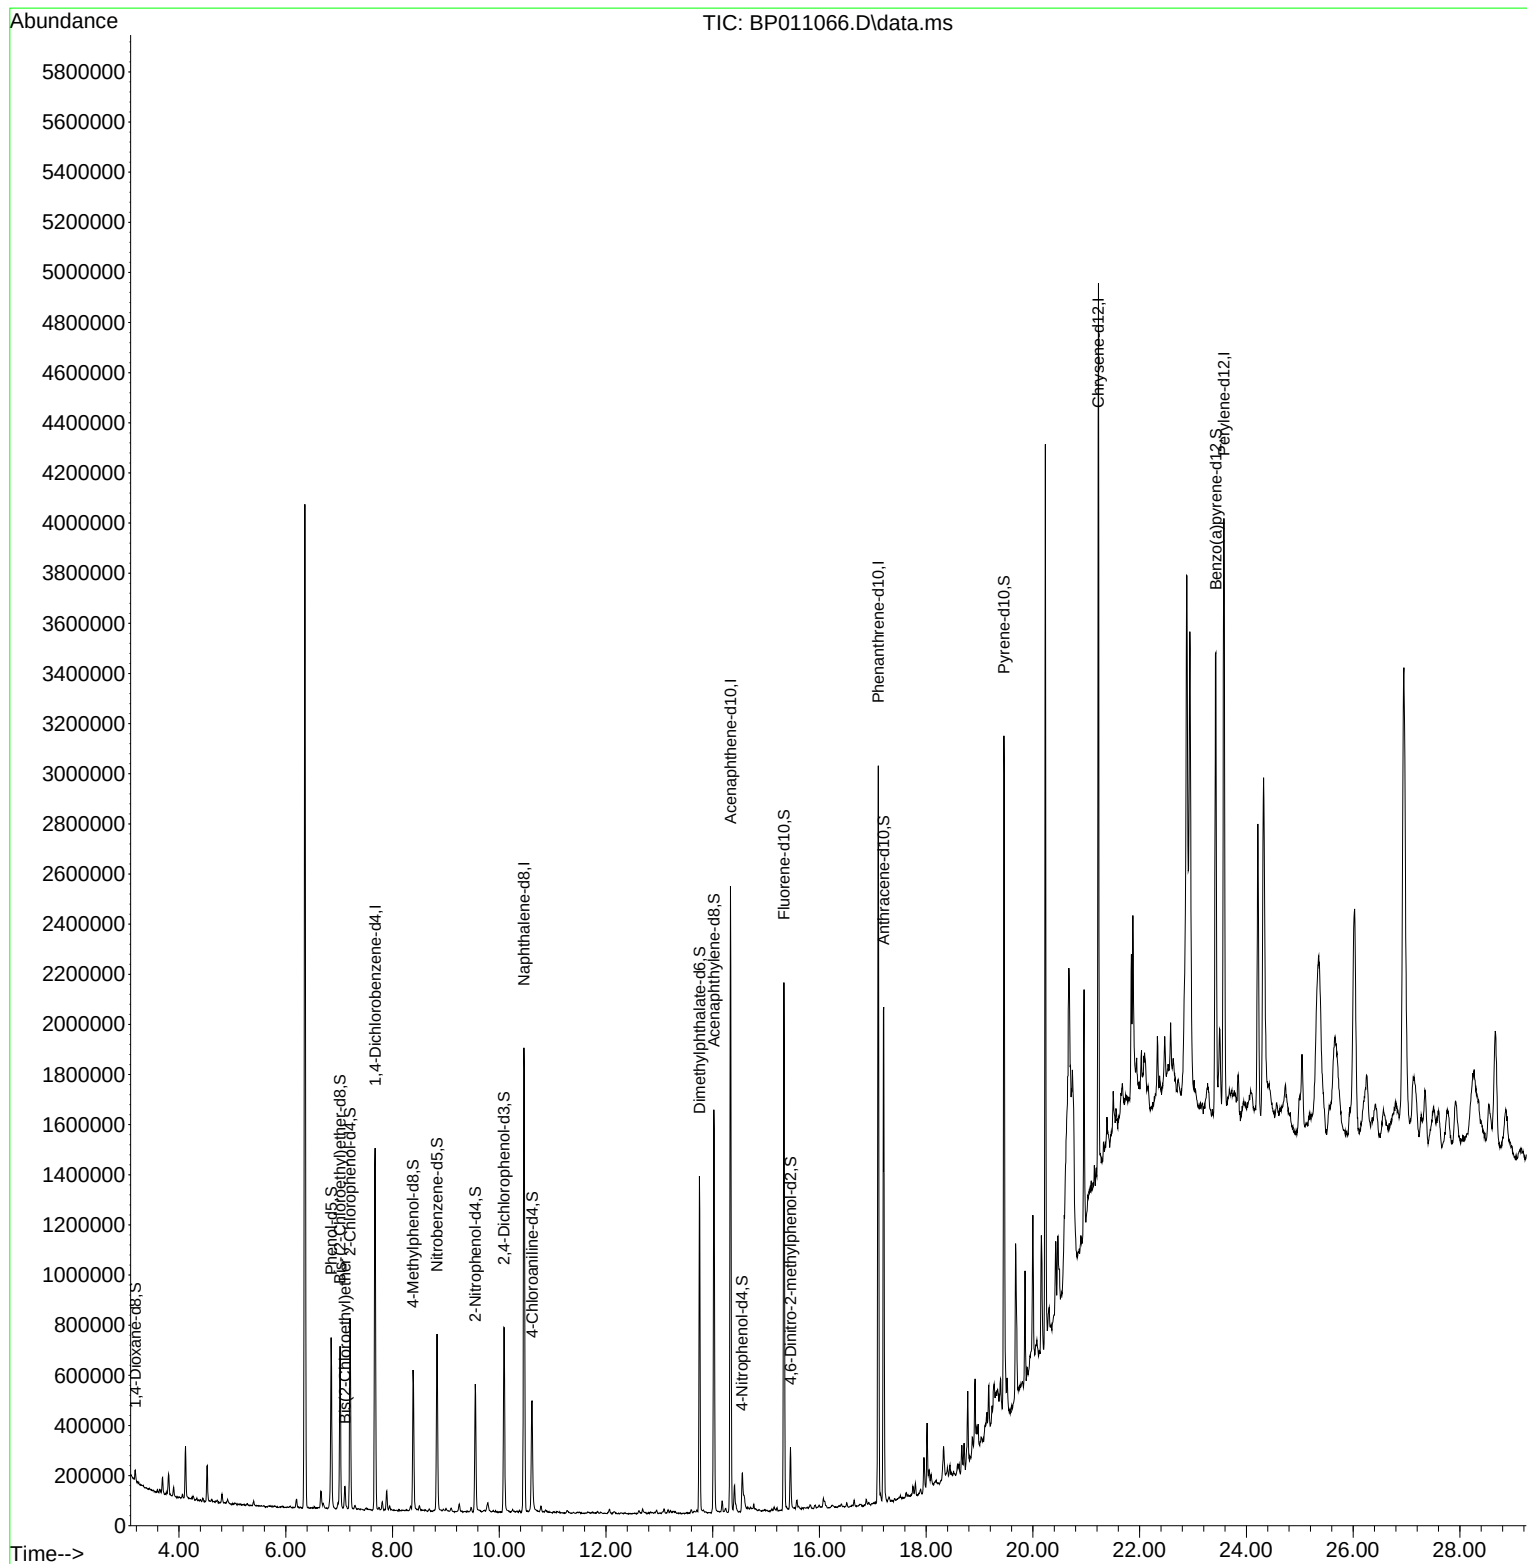

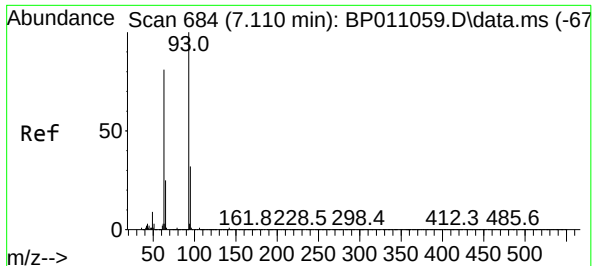

#10

Bis(2-Chloroethyl)ether

Concen: 1.238 ng/ul

RT: 7.110 min Scan# 61

Delta R.T. -0.006 min


Lab File: BP011066.D

Acq: 21 Jul 2022 17:20

Instrument :

BNA_P

ClientSampleId :

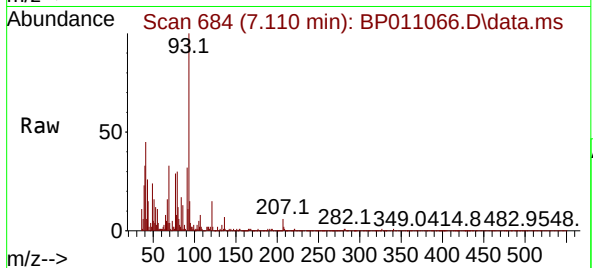

Tgt Ion: 93 Resp: 31908

Ion Ratio Lower Upper

93 100

63 3.0 72.4 108.6#

95 4.2 27.3 40.9#

