

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
 Data File : BP011070.D
 Acq On : 21 Jul 2022 19:38
 Operator : CG/JU
 Sample : N3709-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0B22

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011070.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.176	12	15	23	rVB	93626	137513	2.67%	0.217%
2	3.452	58	62	67	rBV	90561	122396	2.37%	0.193%
3	3.587	82	85	107	rVB	982152	1429902	27.72%	2.254%
4	3.899	134	138	144	rVB	30483	40362	0.78%	0.064%
5	4.799	289	291	298	rBV4	9485	18249	0.35%	0.029%
6	6.311	546	548	551	rBV4	4064	5486	0.11%	0.009%
7	6.681	609	611	615	rVB3	7253	7822	0.15%	0.012%
8	6.852	633	640	652	rVB	1090849	1691681	32.79%	2.667%
9	7.017	662	668	678	rVB	967691	1453571	28.18%	2.291%
10	7.093	678	681	690	rVB	23662	37146	0.72%	0.059%
11	7.205	693	700	709	rBV	1202631	1821054	35.30%	2.871%
12	7.669	770	779	788	rBV	1362342	2124208	41.18%	3.349%
13	7.740	788	791	796	rVB5	11886	21090	0.41%	0.033%
14	8.387	894	901	913	rBV	1338694	2080627	40.33%	3.280%
15	8.834	970	977	985	rBV	1000275	1628098	31.56%	2.567%
16	8.952	994	997	1003	rBV4	13733	17305	0.34%	0.027%
17	8.999	1003	1005	1009	rVB5	5713	7583	0.15%	0.012%
18	9.246	1045	1047	1053	rVB4	10333	14987	0.29%	0.024%
19	9.552	1092	1099	1111	rBV	770169	1247243	24.18%	1.966%
20	10.087	1182	1190	1203	rBV	1174542	1924395	37.31%	3.034%
21	10.281	1218	1223	1228	rBV9	6691	14391	0.28%	0.023%
22	10.463	1246	1254	1266	rBV	1747548	2795068	54.18%	4.406%
23	10.610	1269	1279	1292	rBV	1164258	1976565	38.32%	3.116%
24	11.128	1363	1367	1369	rBV5	5661	6493	0.13%	0.010%
25	11.275	1389	1392	1395	rBV5	5566	6835	0.13%	0.011%
26	11.752	1470	1473	1476	rVB5	4236	5608	0.11%	0.009%
27	11.828	1485	1486	1492	rVB6	4180	5196	0.10%	0.008%
28	12.063	1519	1526	1530	rBV3	26605	47123	0.91%	0.074%
29	12.281	1559	1563	1568	rVV8	3048	5234	0.10%	0.008%
30	12.687	1628	1632	1635	rBV6	4803	6407	0.12%	0.010%
31	12.946	1673	1676	1680	rVB6	6629	9608	0.19%	0.015%
32	13.057	1690	1695	1699	rVB8	3652	5662	0.11%	0.009%
33	13.163	1711	1713	1717	rVB5	6336	6594	0.13%	0.010%
34	13.234	1720	1725	1729	rBV7	7333	13700	0.27%	0.022%
35	13.299	1731	1736	1740	rVB7	5253	8627	0.17%	0.014%
36	13.575	1782	1783	1789	rVB5	3092	5167	0.10%	0.008%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
 Data File : BP011070.D
 Acq On : 21 Jul 2022 19:38
 Operator : CG/JU
 Sample : N3709-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0B22

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	13.751	1805	1813	1825	rBV	2041326	2736553	53.05%	4.314%
38	14.022	1850	1859	1873	rBV	2376923	3384854	65.62%	5.336%
39	14.246	1893	1897	1901	rVB7	7307	8824	0.17%	0.014%
40	14.334	1905	1912	1920	rBV	2277210	3240629	62.82%	5.108%
41	14.551	1943	1949	1967	rBV	514574	980501	19.01%	1.546%
42	14.769	1983	1986	1997	rVB	16629	34769	0.67%	0.055%
43	14.887	2000	2006	2012	rVB	16937	30121	0.58%	0.047%
44	14.981	2019	2022	2026	rVB6	6439	7885	0.15%	0.012%
45	15.093	2038	2041	2046	rVB2	29417	41835	0.81%	0.066%
46	15.151	2046	2051	2054	rBV	10844	14019	0.27%	0.022%
47	15.210	2057	2061	2062	rBV4	5641	6580	0.13%	0.010%
48	15.334	2075	2082	2089	rBV	2979939	4085649	79.20%	6.441%
49	15.457	2097	2103	2118	rBV	536567	768782	14.90%	1.212%
50	15.575	2118	2123	2127	rVB	33908	49071	0.95%	0.077%
51	15.863	2170	2172	2177	rVB5	8720	6815	0.13%	0.011%
52	16.040	2194	2202	2205	rBV7	18942	37688	0.73%	0.059%
53	16.128	2213	2217	2224	rVB7	14723	21706	0.42%	0.034%
54	16.381	2255	2260	2263	rBV6	8248	13769	0.27%	0.022%
55	16.516	2279	2283	2286	rBV6	6425	8357	0.16%	0.013%
56	16.875	2341	2344	2349	rBV7	11331	19516	0.38%	0.031%
57	16.910	2349	2350	2356	rVB6	6730	9242	0.18%	0.015%
58	17.034	2368	2371	2376	rVB6	9194	14199	0.28%	0.022%
59	17.104	2376	2383	2390	rBV	2470050	3599539	69.78%	5.674%
60	17.204	2393	2400	2411	rVV2	2929708	4237708	82.15%	6.680%
61	17.310	2413	2418	2426	rVB5	50457	79659	1.54%	0.126%
62	17.798	2496	2501	2505	rVV	105236	130384	2.53%	0.206%
63	18.010	2533	2537	2543	rBV3	57269	84517	1.64%	0.133%
64	19.034	2707	2711	2715	rBV2	42437	55926	1.08%	0.088%
65	19.098	2720	2722	2727	rVB	32258	39422	0.76%	0.062%
66	19.457	2777	2783	2790	rBV	3905504	5001422	96.96%	7.884%
67	20.951	3034	3037	3044	rBV2	256081	449582	8.72%	0.709%
68	21.222	3079	3083	3090	rBV	3397758	4038555	78.29%	6.366%
69	23.422	3451	3457	3465	rVB2	2866189	5158494	100.00%	8.132%
70	23.574	3477	3483	3493	rVB2	2195106	4290605	83.18%	6.764%




Sum of corrected areas: 63436173

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
Data File : BP011070.D
Acq On : 21 Jul 2022 19:38
Operator : CG/JU
Sample : N3709-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0B22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

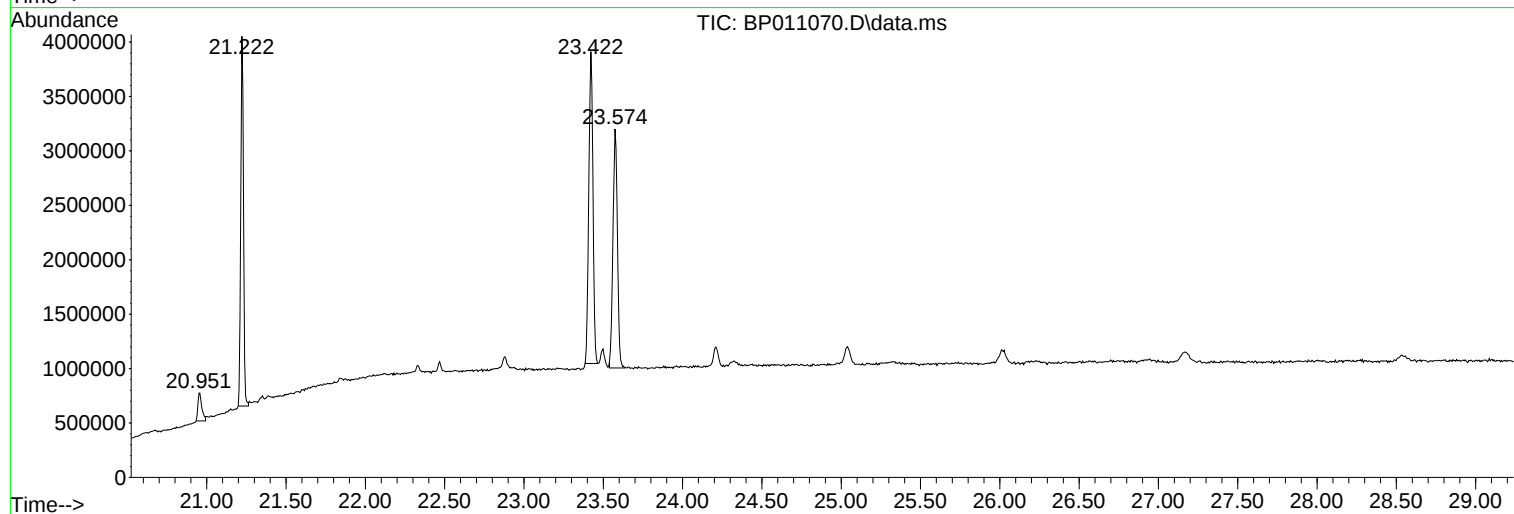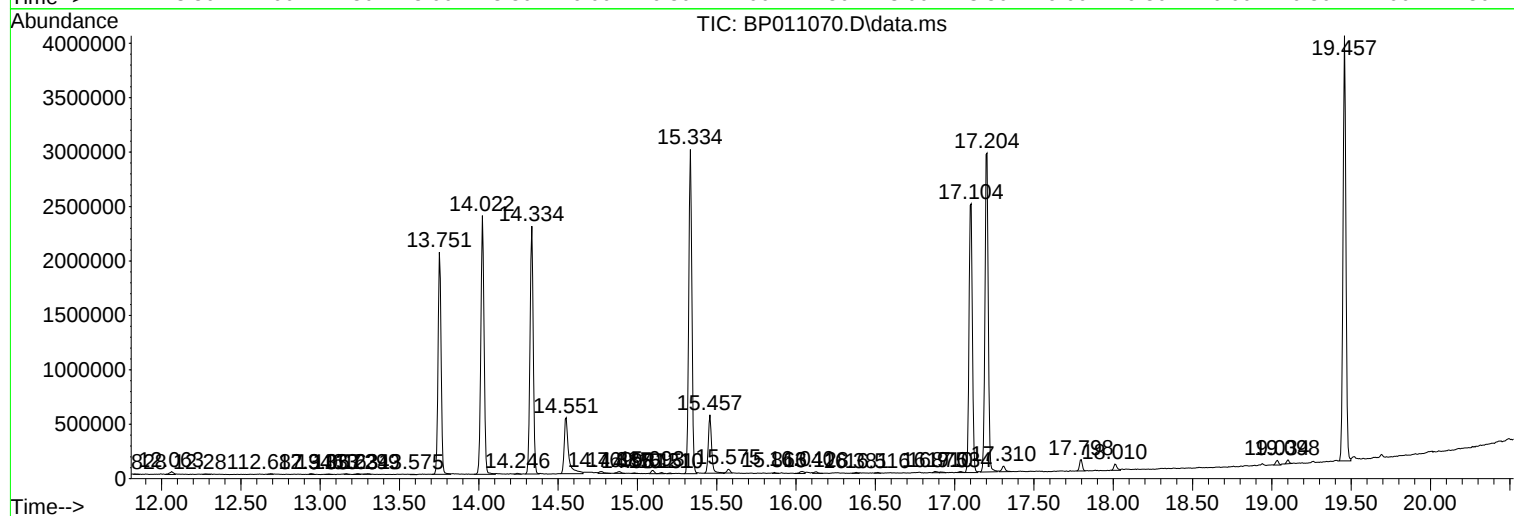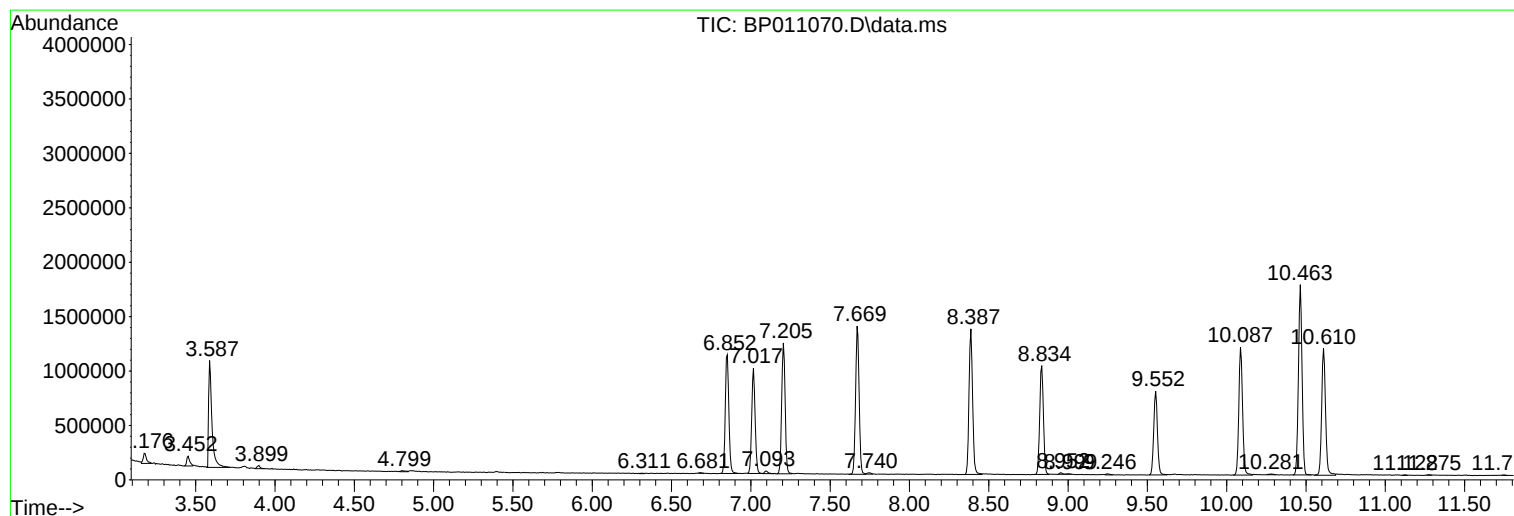

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
Data File : BP011070.D
Acq On : 21 Jul 2022 19:38
Operator : CG/JU
Sample : N3709-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0B22










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.951	2.23 ng/ul	449582	Chrysene-d12	21.222

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Pentacos-1-ene	350	C25H50	016980-85-1	94
2			Nonacos-1-ene	406	C29H58	018835-35-3	91
3			n-Tetracosanol-1	354	C24H50O	000506-51-4	91
4			1-Tricosene	322	C23H46	018835-32-0	91
5			Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	91

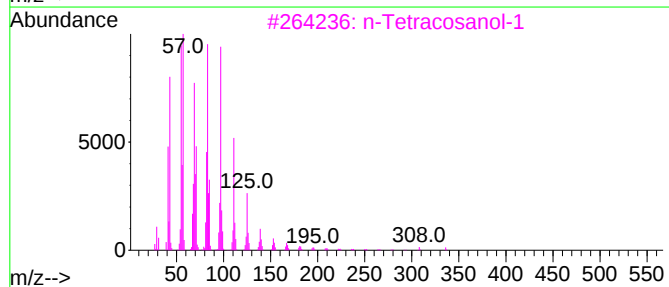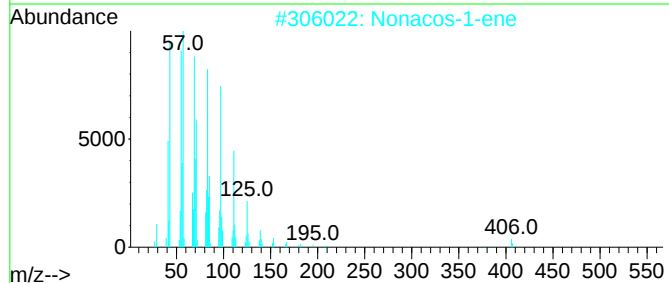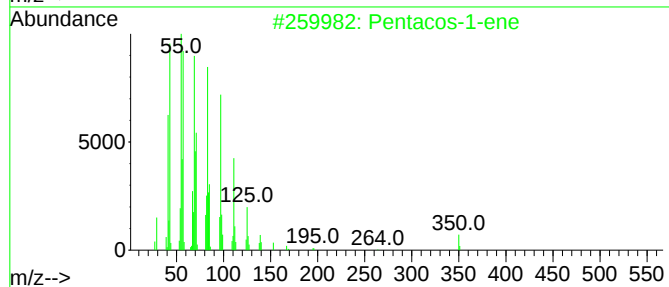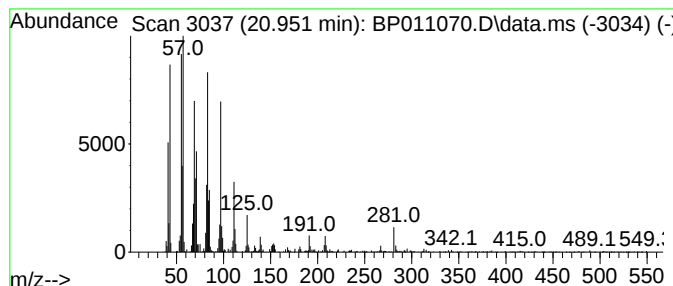

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
Data File : BP011070.D
Acq On : 21 Jul 2022 19:38
Operator : CG/JU
Sample : N3709-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0B22

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	20.951	2.2	ng/u1	449582	5	21.222	4038560	20.0