

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
 Data File : BP011074.D
 Acq On : 21 Jul 2022 22:31
 Operator : CG/JU
 Sample : PB146324BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK324

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011074.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.176	11	15	22	rVB	204367	245998	2.91%	0.249%
2	3.581	81	84	104	rBV	2106302	2904115	34.39%	2.934%
3	3.893	133	137	142	rVB	38126	52009	0.62%	0.053%
4	6.846	633	639	657	rBV	2114701	3317410	39.29%	3.352%
5	7.017	661	668	677	rVB	1841002	2788639	33.03%	2.817%
6	7.205	693	700	711	rBV	2311266	3514555	41.62%	3.551%
7	7.669	772	779	788	rBV	1830714	2812546	33.31%	2.842%
8	8.387	894	901	915	rBV	2482339	3917710	46.40%	3.958%
9	8.834	970	977	987	rBV	1939868	3129462	37.06%	3.162%
10	9.552	1091	1099	1109	rBV	1516356	2427913	28.75%	2.453%
11	10.087	1182	1190	1201	rBV	2214766	3606422	42.71%	3.644%
12	10.463	1245	1254	1261	rBV	2261825	3708149	43.92%	3.746%
13	10.610	1271	1279	1293	rBV	2179099	3675838	43.53%	3.714%
14	12.063	1520	1526	1534	rBV	40632	75643	0.90%	0.076%
15	13.051	1689	1694	1700	rBV10	3839	9226	0.11%	0.009%
16	13.293	1729	1735	1742	rVB7	6728	13011	0.15%	0.013%
17	13.751	1806	1813	1826	rBV	3447488	4695403	55.61%	4.744%
18	13.840	1826	1828	1834	rVB7	6178	10355	0.12%	0.010%
19	14.022	1852	1859	1873	rBV	4078927	5829442	69.04%	5.890%
20	14.334	1904	1912	1920	rBV	2834329	4101925	48.58%	4.144%
21	14.546	1941	1948	1968	rBV	1180469	2077702	24.61%	2.099%
22	14.975	2017	2021	2026	rVB8	5429	9625	0.11%	0.010%
23	15.334	2075	2082	2091	rBV	4861413	6806760	80.62%	6.877%
24	15.457	2096	2103	2114	rVV	1315631	1835059	21.73%	1.854%
25	15.575	2118	2123	2134	rVB	57947	99174	1.17%	0.100%
26	15.910	2174	2180	2187	rVB	4326	10668	0.13%	0.011%
27	16.022	2194	2199	2203	rBV8	5882	9598	0.11%	0.010%
28	16.122	2213	2216	2223	rVB5	20844	29523	0.35%	0.030%
29	16.587	2290	2295	2299	rBV8	4433	9033	0.11%	0.009%
30	16.775	2321	2327	2331	rBV9	10278	18314	0.22%	0.019%
31	16.881	2341	2345	2351	rVB6	6583	11860	0.14%	0.012%
32	17.098	2375	2382	2392	rBV	3062450	4286743	50.77%	4.331%
33	17.198	2393	2399	2414	rVV	5186639	6877625	81.45%	6.949%
34	19.028	2706	2710	2717	rBV2	63875	90693	1.07%	0.092%
35	19.098	2718	2722	2728	rVV	55272	78073	0.92%	0.079%
36	19.457	2777	2783	2791	rBV	5690066	7765108	91.97%	7.845%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
Data File : BP011074.D
Acq On : 21 Jul 2022 22:31
Operator : CG/JU
Sample : PB146324BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK324

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Title : SVOA CALIBRATION

37	21.222	3078	3083	3094	rBV	3736849	4691189	55.56%	4.740%
38	23.416	3450	3456	3465	rVB2	4538514	8443490	100.00%	8.531%
39	23.569	3476	3482	3491	rVB2	2568735	4993897	59.14%	5.045%


Sum of corrected areas: 98979905

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
Data File : BP011074.D
Acq On : 21 Jul 2022 22:31
Operator : CG/JU
Sample : PB146324BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

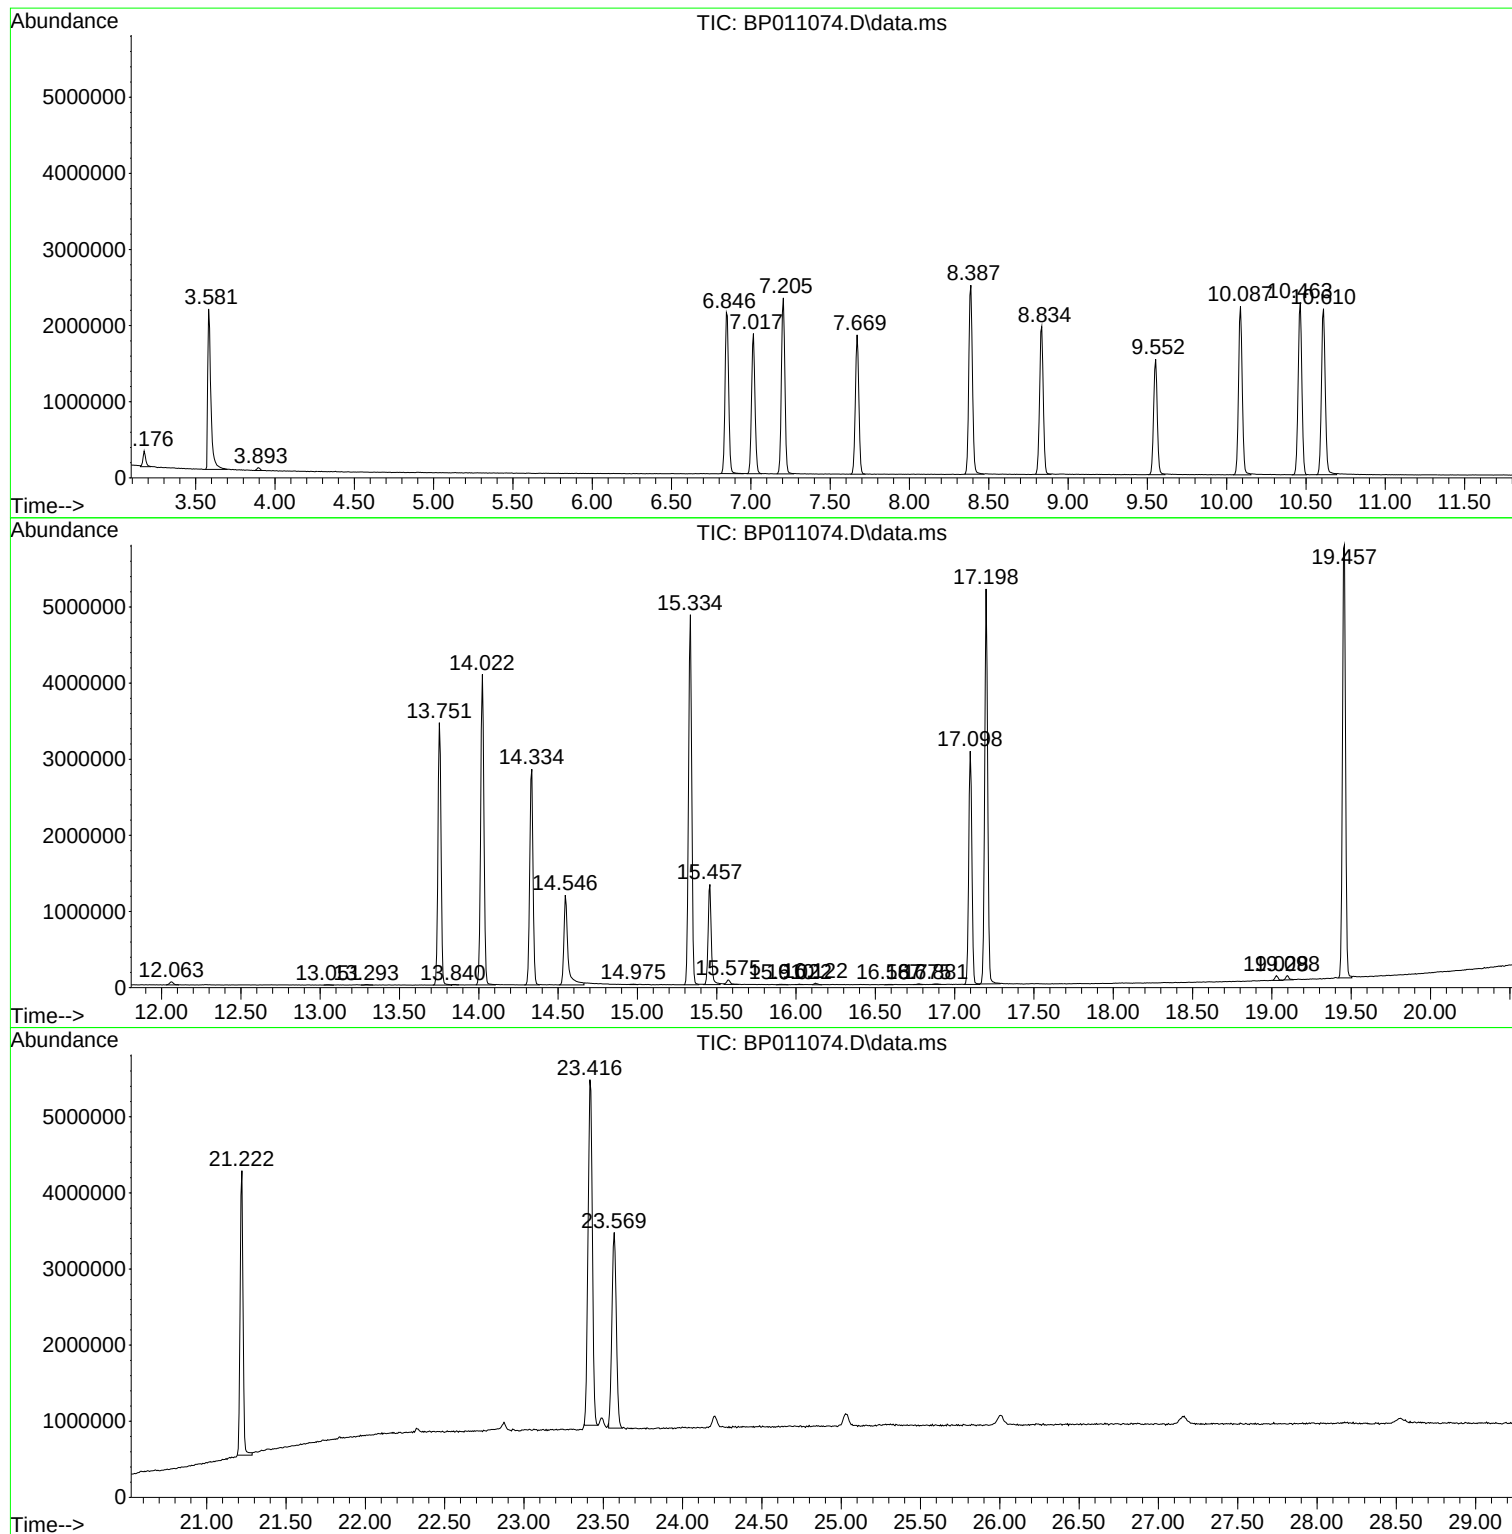

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
Data File : BP011074.D
Acq On : 21 Jul 2022 22:31
Operator : CG/JU
Sample : PB146324BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
Data File : BP011074.D
Acq On : 21 Jul 2022 22:31
Operator : CG/JU
Sample : PB146324BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------