

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
 Data File : BP011078.D
 Acq On : 22 Jul 2022 00:49
 Operator : CG/JU
 Sample : N3709-08 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0B24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

Signal : TIC: BP011078.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.899	134	138	143	rVB	41086	63912	0.97%	0.141%
2	6.164	519	523	526	rBV6	8937	13858	0.21%	0.030%
3	6.228	532	534	539	rVB2	17170	21938	0.33%	0.048%
4	6.311	544	548	551	rBV5	10006	15050	0.23%	0.033%
5	6.481	574	577	583	rVB7	8832	16279	0.25%	0.036%
6	6.664	604	608	614	rVB3	32894	47313	0.72%	0.104%
7	6.769	622	626	628	rBV5	6710	8348	0.13%	0.018%
8	6.805	629	632	635	rVV5	20607	32141	0.49%	0.071%
9	6.858	635	641	650	rVB	189061	318301	4.84%	0.700%
10	7.016	661	668	675	rBV	229982	366599	5.58%	0.807%
11	7.087	675	680	688	rVV	209775	316397	4.81%	0.696%
12	7.158	688	692	695	rVV5	23125	38879	0.59%	0.086%
13	7.211	695	701	710	rVV	221398	362484	5.51%	0.797%
14	7.316	713	719	723	rVB4	21159	36278	0.55%	0.080%
15	7.675	771	780	794	rVB	2264140	3673329	55.88%	8.082%
16	7.799	797	801	807	rVB7	17017	30200	0.46%	0.066%
17	7.893	813	817	824	rBV	42817	72869	1.11%	0.160%
18	7.946	824	826	832	rVB6	11478	18885	0.29%	0.042%
19	8.152	858	861	862	rBV3	11602	10121	0.15%	0.022%
20	8.205	866	870	882	rVB3	42940	92921	1.41%	0.204%
21	8.340	885	893	896	rVV2	25788	45568	0.69%	0.100%
22	8.393	896	902	913	rVV2	247187	415378	6.32%	0.914%
23	8.487	915	918	924	rVV7	10417	23874	0.36%	0.053%
24	8.546	924	928	932	rVV5	19824	34739	0.53%	0.076%
25	8.575	932	933	937	rVB4	12519	11690	0.18%	0.026%
26	8.775	963	967	971	rVB5	24923	39859	0.61%	0.088%
27	8.834	971	977	985	rBV	245949	414459	6.30%	0.912%
28	8.975	997	1001	1002	rBV4	11308	14830	0.23%	0.033%
29	9.105	1016	1023	1024	rBV6	4813	9480	0.14%	0.021%
30	9.252	1043	1048	1052	rVV8	10580	18079	0.28%	0.040%
31	9.299	1052	1056	1062	rVB8	10218	20678	0.31%	0.045%
32	9.358	1062	1066	1068	rBV4	10570	14886	0.23%	0.033%
33	9.375	1068	1069	1075	rVB6	11523	12713	0.19%	0.028%
34	9.558	1093	1100	1107	rBV	109896	191112	2.91%	0.420%
35	9.810	1139	1143	1145	rBV5	5516	7375	0.11%	0.016%
36	9.875	1148	1154	1159	rBV7	16401	30469	0.46%	0.067%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
 Data File : BP011078.D
 Acq On : 22 Jul 2022 00:49
 Operator : CG/JU
 Sample : N3709-08 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0B24

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
 Title : SVOA CALIBRATION

37	10.093	1182	1191	1199	rBV	208397	356083	5.42%	0.783%
38	10.469	1246	1255	1262	rBV	3061573	5089905	77.43%	11.198%
39	10.616	1273	1280	1289	rBV	116008	210810	3.21%	0.464%
40	11.287	1390	1394	1397	rBV6	4942	8980	0.14%	0.020%
41	11.499	1427	1430	1434	rBV6	7670	11148	0.17%	0.025%
42	11.757	1469	1474	1478	rVB8	4248	7579	0.12%	0.017%
43	11.904	1494	1499	1504	rBV6	8500	15768	0.24%	0.035%
44	12.063	1519	1526	1531	rVB10	7584	19065	0.29%	0.042%
45	12.140	1533	1539	1545	rVB7	11145	19401	0.30%	0.043%
46	12.281	1557	1563	1565	rBV7	6992	10139	0.15%	0.022%
47	12.363	1573	1577	1585	rVB6	9267	18502	0.28%	0.041%
48	12.887	1653	1666	1673	rBV3	111375	177111	2.69%	0.390%
49	13.051	1690	1694	1698	rBV6	6717	10079	0.15%	0.022%
50	13.163	1707	1713	1719	rBV4	19926	32405	0.49%	0.071%
51	13.304	1734	1737	1743	rVB8	8595	14942	0.23%	0.033%
52	13.357	1743	1746	1749	rBV4	5449	8614	0.13%	0.019%
53	13.504	1769	1771	1778	rVB8	9132	16278	0.25%	0.036%
54	13.657	1793	1797	1801	rVB7	12996	17543	0.27%	0.039%
55	13.757	1808	1814	1820	rVB	387753	536543	8.16%	1.180%
56	13.828	1822	1826	1829	rVB5	11696	14600	0.22%	0.032%
57	13.946	1840	1846	1852	rVB5	6493	16158	0.25%	0.036%
58	14.028	1852	1860	1865	rBV	648075	984280	14.97%	2.165%
59	14.245	1893	1897	1903	rVB3	24938	35601	0.54%	0.078%
60	14.340	1905	1913	1921	rBV	4323062	6351109	96.62%	13.973%
61	14.587	1951	1955	1959	rVB7	18610	28440	0.43%	0.063%
62	15.204	2057	2060	2066	rVB	35476	39686	0.60%	0.087%
63	15.340	2077	2083	2088	rBV	827985	1224166	18.62%	2.693%
64	16.075	2205	2208	2210	rBV2	58058	76415	1.16%	0.168%
65	16.875	2341	2344	2349	rBV2	68807	101733	1.55%	0.224%
66	17.104	2378	2383	2389	rBV	4733600	6573506	100.00%	14.462%
67	17.204	2395	2400	2406	rBV2	868502	1200415	18.26%	2.641%
68	18.839	2676	2678	2682	rVB2	283462	321895	4.90%	0.708%
69	19.192	2734	2738	2742	rBV	1252558	1537026	23.38%	3.382%
70	19.463	2780	2784	2793	rVB	828787	1314474	20.00%	2.892%
71	19.898	2855	2858	2865	rBV	851637	1117454	17.00%	2.458%
72	21.227	3080	3084	3091	rVB	4261838	5309728	80.77%	11.682%
73	23.586	3480	3485	3493	rVB2	2919301	5764452	87.69%	12.682%




Sum of corrected areas: 45453324

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
Data File : BP011078.D
Acq On : 22 Jul 2022 00:49
Operator : CG/JU
Sample : N3709-08 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0B24

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

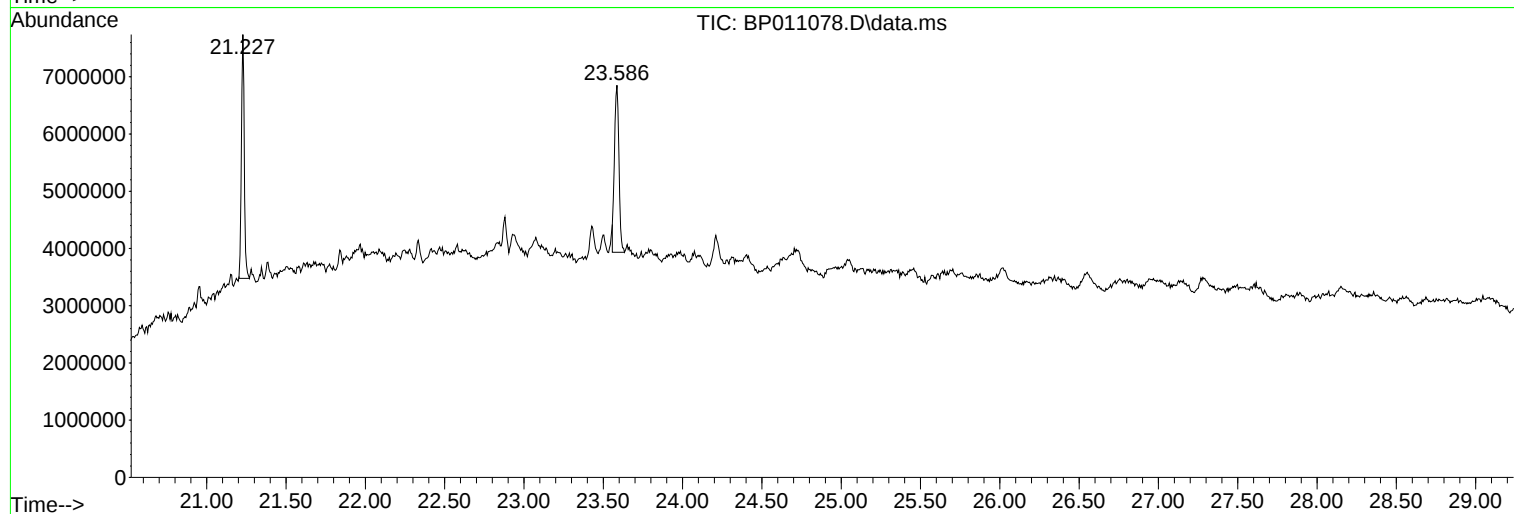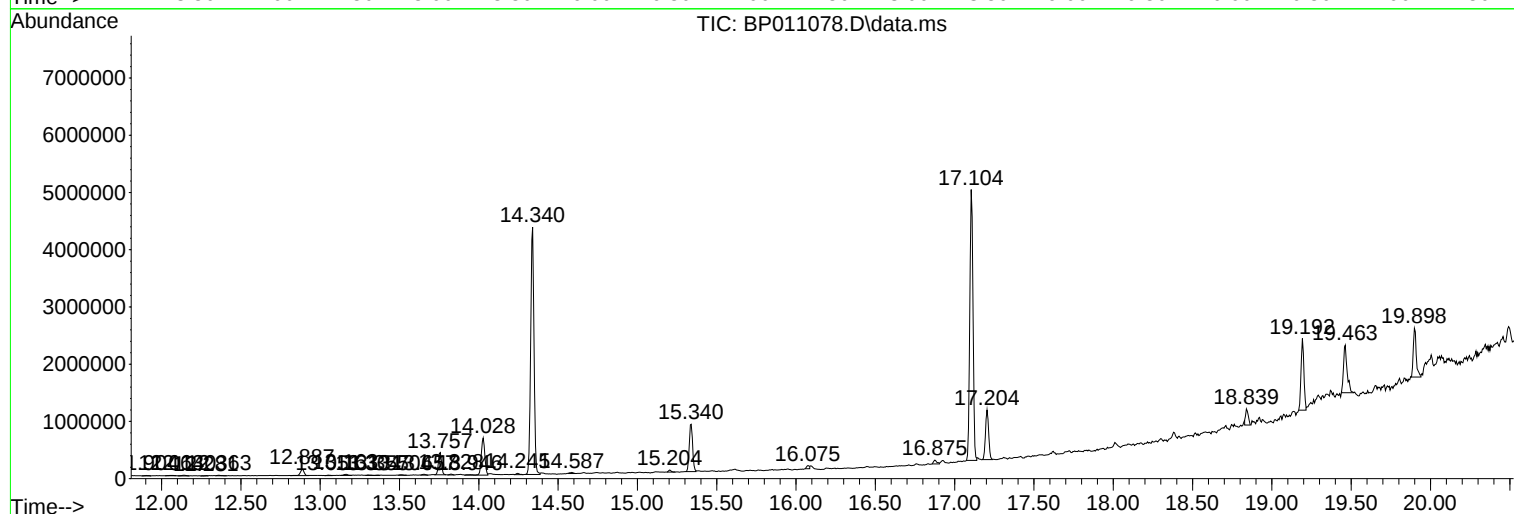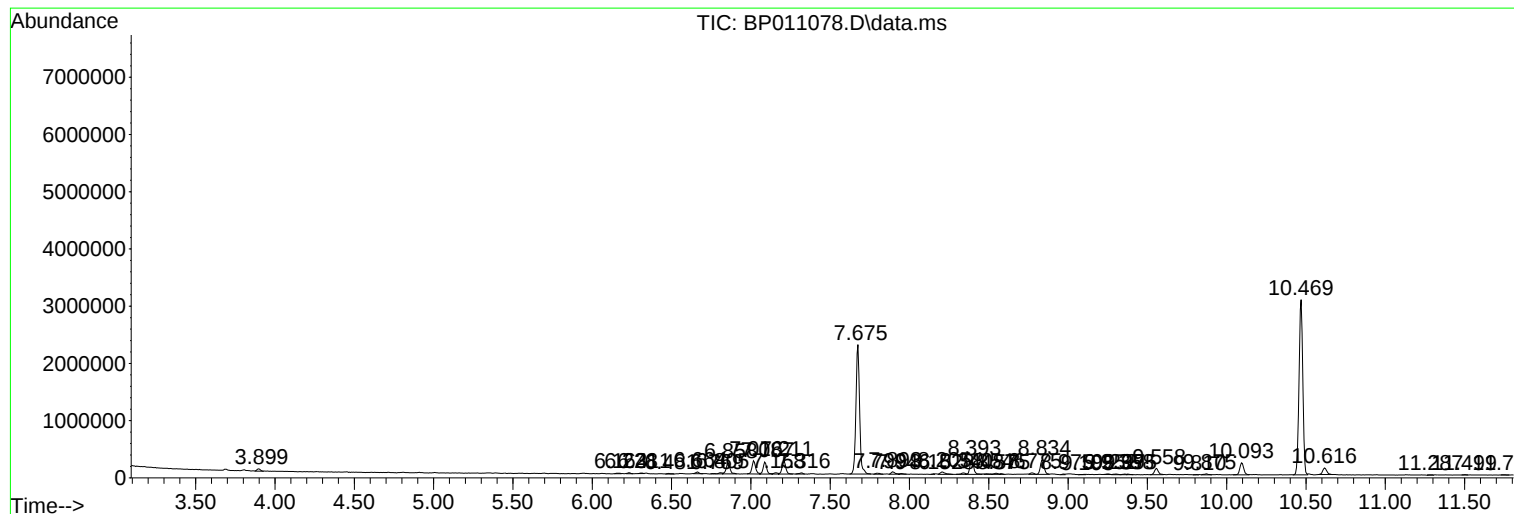

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
Data File : BP011078.D
Acq On : 22 Jul 2022 00:49
Operator : CG/JU
Sample : N3709-08 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0B24










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 10,18-Bisnorabieta-5,7,9(10... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
19.192	5.79 ng/ul	1537030	Chrysene-d12	21.227

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	10,18-Bisnorabieta-5,7,9(10),11,...	238	C18H22	006566-19-4	99		
2	3,4'-Diisopropylbiphenyl	238	C18H22	061434-46-6	76		
3	4,4'-Diisopropylbiphenyl	238	C18H22	018970-30-4	60		
4	4,4'-Diacetyl biphenyl	238	C16H14O2	000787-69-9	49		
5	2-Propenoic acid, 3-(3,4,5-trime...	238	C12H14O5	000090-50-6	49		

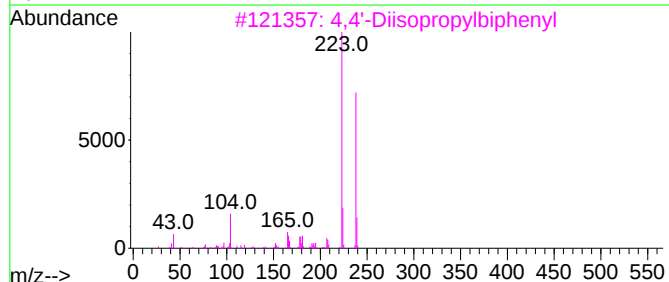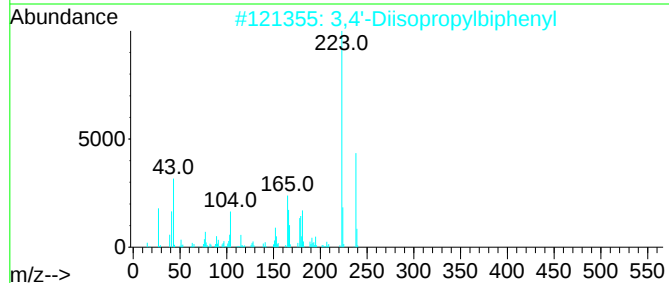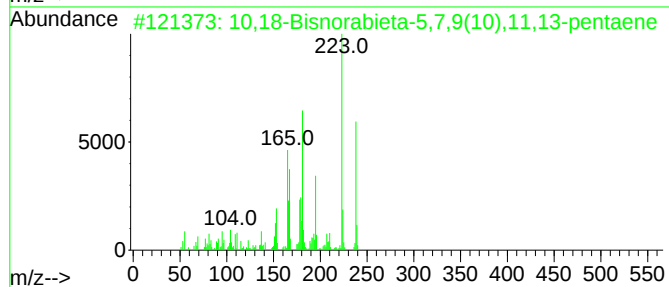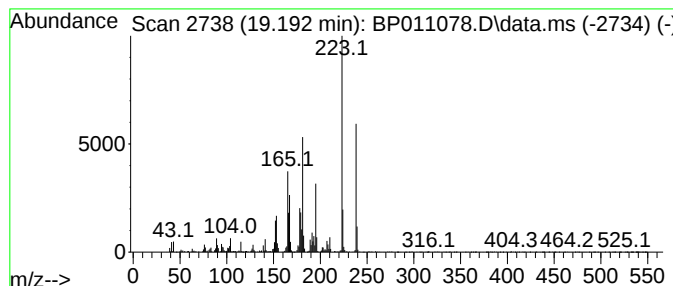

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
Data File : BP011078.D
Acq On : 22 Jul 2022 00:49
Operator : CG/JU
Sample : N3709-08 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0B24










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Retene Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
19.898	4.21 ng/ul	1117450	Chrysene-d12	21.227

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Retene	234	C18H18	000483-65-8	99
2			2-Isopropyl-10-methylphenanthrene	234	C18H18	066552-97-4	95
3			Retene	234	C18H18	000483-65-8	95
4			Retene	234	C18H18	000483-65-8	95
5			Quinoline, 2-(3-tolyl)-	219	C16H13N	024641-30-3	83

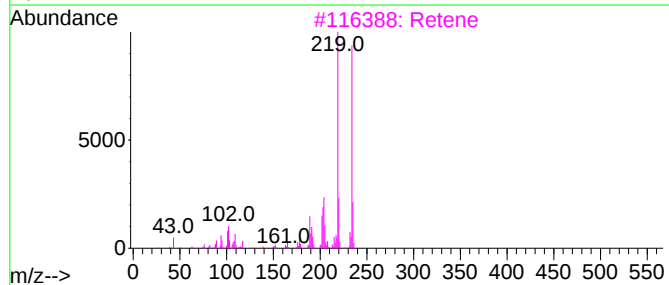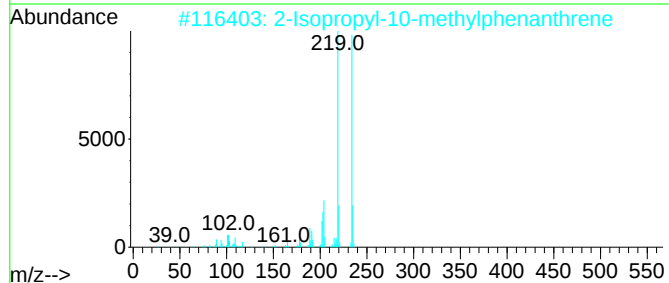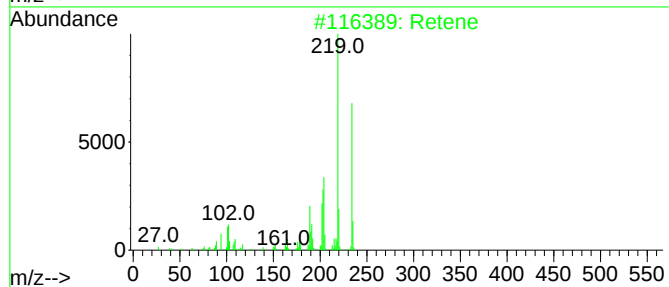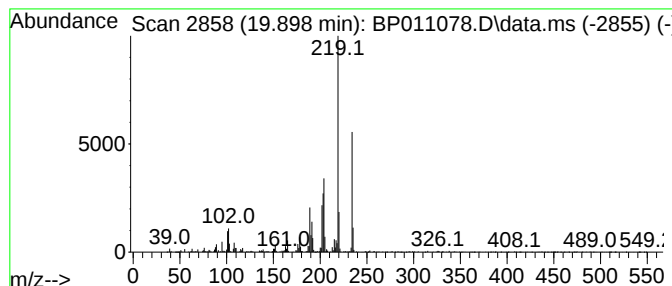

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP072122\
Data File : BP011078.D
Acq On : 22 Jul 2022 00:49
Operator : CG/JU
Sample : N3709-08 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0B24

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP071422.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
10,18-Bisnorabi...	19.192	5.8	ng/ul	1537030	5	21.227	5309730	20.0
Retene	19.898	4.2	ng/ul	1117450	5	21.227	5309730	20.0